

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015199.D
 Acq On : 27 Mar 2020 06:59
 Operator : SY/MD
 Sample : L1976-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTJ6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	65	70	85	rVB	256403	271638	14.90%	1.668%
2	1.579	147	152	166	rVB	224992	256998	14.10%	1.578%
3	2.119	314	320	334	rVB	441252	623162	34.19%	3.827%
4	3.322	691	694	698	rBV4	2312	1146	0.06%	0.007%
5	3.550	762	765	767	rBV3	2089	1280	0.07%	0.008%
6	3.592	774	778	780	rBV5	1332	1212	0.07%	0.007%
7	3.637	788	792	795	rBV5	1801	1519	0.08%	0.009%
8	3.759	827	830	831	rBV3	1928	1094	0.06%	0.007%
9	3.939	873	886	925	rBV2	258685	828958	45.48%	5.091%
10	4.376	1008	1022	1046	rBV	311807	767799	42.12%	4.715%
11	4.563	1078	1080	1083	rBV3	1913	1082	0.06%	0.007%
12	4.891	1180	1182	1185	rVB4	1489	433	0.02%	0.003%
13	4.913	1188	1189	1192	rVB3	1764	702	0.04%	0.004%
14	4.933	1192	1195	1196	rBV3	1509	936	0.05%	0.006%
15	4.962	1201	1204	1205	rBV2	1317	771	0.04%	0.005%
16	5.074	1224	1239	1267	rVB2	740170	1822780	100.00%	11.194%
17	5.550	1384	1387	1388	rBV3	1399	694	0.04%	0.004%
18	5.643	1402	1416	1437	rBV	685270	1368153	75.06%	8.402%
19	5.939	1494	1508	1523	rBV	205367	410173	22.50%	2.519%
20	6.097	1544	1557	1576	rBV	434543	876944	48.11%	5.386%
21	6.466	1669	1672	1675	rBV4	2192	1614	0.09%	0.010%
22	6.524	1687	1690	1692	rBV3	1828	1116	0.06%	0.007%
23	6.537	1692	1694	1697	rVV4	2242	1596	0.09%	0.010%
24	6.566	1701	1703	1709	rVB6	3343	3032	0.17%	0.019%
25	6.595	1709	1712	1713	rBV2	1428	817	0.04%	0.005%
26	6.617	1717	1719	1721	rBV3	2007	1115	0.06%	0.007%
27	6.900	1804	1807	1810	rBV4	2174	1718	0.09%	0.011%
28	7.010	1831	1841	1861	rVB2	175636	312059	17.12%	1.916%
29	7.158	1885	1887	1890	rBV3	1673	818	0.04%	0.005%
30	7.338	1930	1943	1965	rBV	838040	1471497	80.73%	9.037%
31	7.534	2001	2004	2007	rBV4	2666	1852	0.10%	0.011%
32	7.643	2028	2038	2056	rBV2	126777	219174	12.02%	1.346%
33	7.801	2084	2087	2090	rBV5	1922	1665	0.09%	0.010%
34	8.116	2175	2185	2217	rBV3	580355	1194406	65.53%	7.335%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015199.D
 Acq On : 27 Mar 2020 06:59
 Operator : SY/MD
 Sample : L1976-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTJ6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

35	8.656	2349	2353	2355	rBV4	1500	963	0.05%	0.006%
36	8.704	2364	2368	2370	rBV5	2129	1857	0.10%	0.011%
37	8.768	2385	2388	2390	rBV3	1819	1008	0.06%	0.006%
38	8.875	2409	2421	2443	rBV	1070717	1726837	94.74%	10.605%
39	9.157	2507	2509	2513	rBV5	2406	1907	0.10%	0.012%
40	9.238	2531	2534	2536	rBV4	1475	1023	0.06%	0.006%
41	9.270	2540	2544	2546	rBV5	2641	2190	0.12%	0.013%
42	9.360	2570	2572	2575	rBV4	1406	1119	0.06%	0.007%
43	9.418	2587	2590	2591	rBV2	2172	1211	0.07%	0.007%
44	9.476	2605	2608	2610	rBV4	1291	997	0.05%	0.006%
45	9.518	2618	2621	2625	rVB6	2552	1814	0.10%	0.011%
46	9.550	2625	2631	2633	rBV6	2459	2437	0.13%	0.015%
47	9.620	2651	2653	2656	rVB3	1358	674	0.04%	0.004%
48	9.775	2698	2701	2702	rBV3	1022	690	0.04%	0.004%
49	9.833	2713	2719	2721	rBV6	2809	3063	0.17%	0.019%
50	9.942	2751	2753	2757	rBV5	2130	1311	0.07%	0.008%
51	9.965	2757	2760	2765	rBV7	2023	2027	0.11%	0.012%
52	10.016	2774	2776	2779	rBV4	1097	680	0.04%	0.004%
53	10.116	2805	2807	2811	rVB4	2117	1417	0.08%	0.009%
54	10.154	2817	2819	2821	rBV3	1419	726	0.04%	0.004%
55	10.238	2834	2845	2859	rBV	667028	1035579	56.81%	6.360%
56	10.460	2912	2914	2916	rBV3	1615	1010	0.06%	0.006%
57	10.611	2959	2961	2963	rBV3	1536	658	0.04%	0.004%
58	10.704	2988	2990	2992	rBV3	1462	539	0.03%	0.003%
59	10.794	3016	3018	3019	rBV2	1851	761	0.04%	0.005%
60	10.878	3039	3044	3051	rBV2	3000	3779	0.21%	0.023%
61	10.955	3064	3068	3070	rVB5	1533	1112	0.06%	0.007%
62	11.042	3093	3095	3097	rBV3	1522	846	0.05%	0.005%
63	11.273	3154	3167	3182	rBV	1010633	1564275	85.82%	9.607%
64	11.479	3228	3231	3233	rBV4	1864	1155	0.06%	0.007%
65	11.521	3240	3244	3248	rBV6	2328	1810	0.10%	0.011%
66	11.563	3251	3257	3268	rVB7	8031	13488	0.74%	0.083%
67	11.646	3272	3283	3300	rBV	904239	1429983	78.45%	8.782%
68	11.903	3359	3363	3364	rBV3	2508	1765	0.10%	0.011%
69	11.968	3382	3383	3388	rVB5	2168	1546	0.08%	0.009%
70	11.993	3388	3391	3394	rBV5	1614	1045	0.06%	0.006%
71	12.125	3426	3432	3433	rBV6	1612	1674	0.09%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015199.D
Acq On : 27 Mar 2020 06:59
Operator : SY/MD
Sample : L1976-17
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTJ6

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Title : VOC Analysis

72	12.672	3597	3602	3604	rBV5	3022	2376	0.13%	0.015%
73	12.755	3624	3628	3630	rBV5	2101	1379	0.08%	0.008%
74	12.807	3641	3644	3647	rBV4	1272	952	0.05%	0.006%
75	13.218	3768	3772	3773	rBV3	1588	1212	0.07%	0.007%
76	13.408	3827	3831	3835	rBV6	2726	2066	0.11%	0.013%
77	13.469	3848	3850	3853	rBV3	2555	1471	0.08%	0.009%
78	13.813	3954	3957	3962	rVB7	2451	2249	0.12%	0.014%
79	13.839	3962	3965	3968	rBV4	1620	1311	0.07%	0.008%
80	14.080	4032	4040	4043	rBV9	2604	3239	0.18%	0.020%
81	14.215	4080	4082	4085	rVB3	1365	578	0.03%	0.004%
82	14.369	4126	4130	4131	rBV3	1741	1226	0.07%	0.008%


Sum of corrected areas: 16282988

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015199.D
Acq On : 27 Mar 2020 06:59
Operator : SY/MD
Sample : L1976-17
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTJ6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

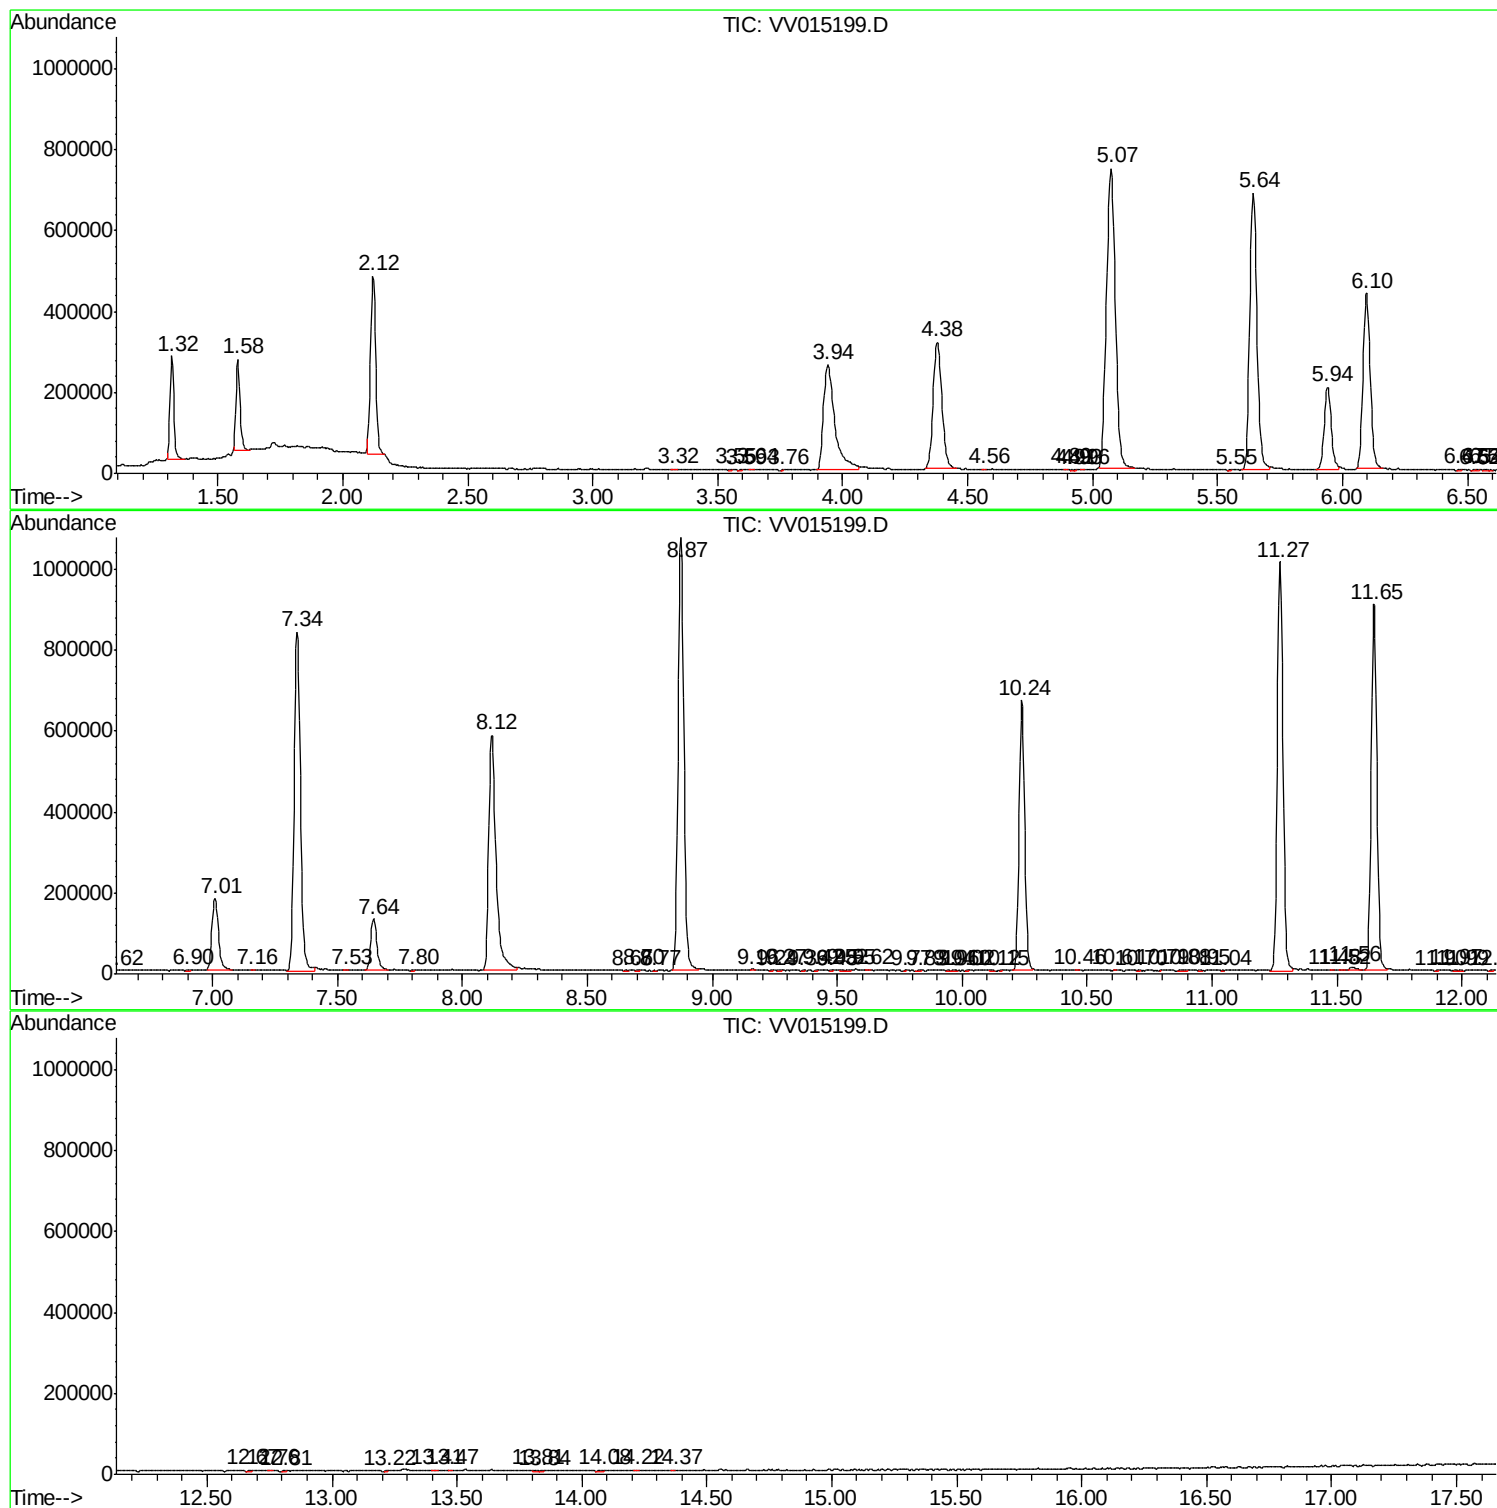

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032620\
Data File : VV015199.D
Acq On : 27 Mar 2020 06:59
Operator : SY/MD
Sample : L1976-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTJ6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032620\
Data File : VV015199.D
Acq On : 27 Mar 2020 06:59
Operator : SY/MD
Sample : L1976-17
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
ETTJ6

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc