

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015200.D
 Acq On : 27 Mar 2020 09:38
 Operator : SY/MD
 Sample : VIBLK74
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK74

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	81	rVB	240990	253800	14.35%	1.743%
2	1.579	146	152	165	rVB	206413	245975	13.91%	1.689%
3	2.119	314	320	334	rVB	440183	615116	34.79%	4.224%
4	3.209	658	659	661	rBV3	952	497	0.03%	0.003%
5	3.466	733	739	740	rBV6	1797	1824	0.10%	0.013%
6	3.505	749	751	752	rBV2	1797	883	0.05%	0.006%
7	3.646	792	795	799	rBV6	2130	1843	0.10%	0.013%
8	3.736	820	823	826	rBV4	1894	1770	0.10%	0.012%
9	3.900	871	874	875	rBV3	1881	1166	0.07%	0.008%
10	3.942	875	887	929	rVV	109161	443271	25.07%	3.044%
11	4.379	1008	1023	1046	rVB	270195	662322	37.46%	4.549%
12	4.762	1140	1142	1146	rBV5	2194	1587	0.09%	0.011%
13	4.826	1159	1162	1164	rBV4	1853	1206	0.07%	0.008%
14	4.939	1195	1197	1201	rBV5	2421	1470	0.08%	0.010%
15	5.074	1223	1239	1260	rBV2	633097	1577887	89.24%	10.836%
16	5.264	1294	1298	1300	rBV5	2120	1810	0.10%	0.012%
17	5.322	1314	1316	1318	rBV4	2388	1361	0.08%	0.009%
18	5.643	1403	1416	1435	rBV	709530	1400825	79.23%	9.620%
19	5.894	1491	1494	1497	rBV4	2844	2133	0.12%	0.015%
20	5.942	1497	1509	1526	rVB6	44808	97978	5.54%	0.673%
21	6.096	1544	1557	1573	rBV2	368866	744812	42.12%	5.115%
22	6.251	1603	1605	1609	rBV4	1899	917	0.05%	0.006%
23	6.424	1654	1659	1664	rBV7	2662	3469	0.20%	0.024%
24	6.492	1678	1680	1683	rBV4	1609	959	0.05%	0.007%
25	6.524	1687	1690	1695	rVV6	1954	1596	0.09%	0.011%
26	6.614	1716	1718	1720	rBV3	1202	773	0.04%	0.005%
27	6.653	1729	1730	1734	rBV3	1743	892	0.05%	0.006%
28	6.694	1741	1743	1746	rVB4	2050	821	0.05%	0.006%
29	6.723	1750	1752	1755	rBV3	916	531	0.03%	0.004%
30	6.820	1780	1782	1785	rBV4	1112	790	0.04%	0.005%
31	7.010	1830	1841	1862	rBV	230398	419339	23.72%	2.880%
32	7.148	1882	1884	1886	rBV3	1218	697	0.04%	0.005%
33	7.338	1930	1943	1964	rBV	747959	1295136	73.25%	8.894%
34	7.643	2029	2038	2056	rVB2	159382	268985	15.21%	1.847%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015200.D
 Acq On : 27 Mar 2020 09:38
 Operator : SY/MD
 Sample : VIBLK74
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK74

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

35	7.945	2130	2132	2133	rBV3	1555	653	0.04%	0.004%
36	8.048	2161	2164	2167	rBV4	1850	990	0.06%	0.007%
37	8.077	2170	2173	2174	rBV3	1523	684	0.04%	0.005%
38	8.119	2174	2186	2213	rBV2	441256	916444	51.83%	6.294%
39	8.440	2284	2286	2289	rBV3	1544	947	0.05%	0.007%
40	8.456	2289	2291	2294	rBV4	1329	808	0.05%	0.006%
41	8.505	2303	2306	2309	rVB5	2048	1415	0.08%	0.010%
42	8.653	2350	2352	2354	rBV3	1178	627	0.04%	0.004%
43	8.743	2378	2380	2381	rBV2	1661	671	0.04%	0.005%
44	8.804	2397	2399	2400	rBV2	929	470	0.03%	0.003%
45	8.874	2407	2421	2442	rBV	1099679	1768150	100.00%	12.143%
46	9.141	2502	2504	2505	rBV2	1572	671	0.04%	0.005%
47	9.241	2532	2535	2537	rBV4	2289	1199	0.07%	0.008%
48	9.299	2547	2553	2554	rBV6	1777	1800	0.10%	0.012%
49	9.363	2571	2573	2575	rBV3	1278	609	0.03%	0.004%
50	9.537	2623	2627	2630	rBV5	2071	1975	0.11%	0.014%
51	9.669	2665	2668	2669	rBV3	1902	921	0.05%	0.006%
52	9.714	2678	2682	2688	rBV9	3249	3654	0.21%	0.025%
53	9.743	2688	2691	2692	rBV3	1433	859	0.05%	0.006%
54	9.855	2721	2726	2731	rBV7	2187	2760	0.16%	0.019%
55	10.055	2784	2788	2791	rBV6	1949	1857	0.11%	0.013%
56	10.116	2805	2807	2810	rBV4	1681	794	0.04%	0.005%
57	10.238	2830	2845	2862	rBV	542632	854988	48.35%	5.872%
58	10.476	2912	2919	2923	rBV9	2238	3114	0.18%	0.021%
59	10.665	2974	2978	2982	rBV7	1735	1890	0.11%	0.013%
60	10.704	2988	2990	2993	rBV4	774	481	0.03%	0.003%
61	10.739	2999	3001	3006	rVB6	3353	1937	0.11%	0.013%
62	10.762	3006	3008	3012	rBV5	1871	1581	0.09%	0.011%
63	10.800	3016	3020	3022	rBV5	2285	1762	0.10%	0.012%
64	10.862	3035	3039	3041	rBV4	2091	1735	0.10%	0.012%
65	10.881	3043	3045	3048	rVV4	1677	821	0.05%	0.006%
66	10.968	3067	3072	3075	rBV6	2800	2703	0.15%	0.019%
67	11.013	3082	3086	3089	rBV5	2604	1956	0.11%	0.013%
68	11.106	3113	3115	3116	rBV2	1978	909	0.05%	0.006%
69	11.273	3155	3167	3183	rBV	1055298	1624143	91.86%	11.154%
70	11.498	3232	3237	3239	rBV6	1772	1613	0.09%	0.011%
71	11.569	3255	3259	3265	rBV8	2575	2707	0.15%	0.019%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015200.D
 Acq On : 27 Mar 2020 09:38
 Operator : SY/MD
 Sample : VIBLK74
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK74

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

72	11.649	3271	3284	3299	rBV	809052	1257449	71.12%	8.636%
73	11.958	3376	3380	3382	rBV5	2093	1381	0.08%	0.009%
74	12.009	3394	3396	3398	rBV3	1103	538	0.03%	0.004%
75	12.022	3398	3400	3402	rBV3	2219	937	0.05%	0.006%
76	12.083	3417	3419	3423	rBV6	1525	1100	0.06%	0.008%
77	12.202	3454	3456	3458	rBV3	1041	598	0.03%	0.004%
78	12.366	3504	3507	3510	rBV4	2026	1179	0.07%	0.008%
79	12.382	3510	3512	3514	rVV2	1265	557	0.03%	0.004%
80	12.556	3562	3566	3568	rVB3	1693	1064	0.06%	0.007%
81	12.768	3629	3632	3634	rBV4	1924	1315	0.07%	0.009%
82	12.813	3643	3646	3648	rBV4	2180	1467	0.08%	0.010%
83	12.955	3688	3690	3692	rBV3	932	516	0.03%	0.004%
84	13.000	3702	3704	3707	rBV2	1082	728	0.04%	0.005%
85	13.090	3730	3732	3736	rBV5	1654	1175	0.07%	0.008%
86	13.157	3751	3753	3757	rBV5	1598	1195	0.07%	0.008%
87	13.289	3788	3794	3798	rBV9	3625	4975	0.28%	0.034%
88	13.334	3803	3808	3812	rBV7	2235	2504	0.14%	0.017%
89	13.357	3812	3815	3817	rBV3	2525	1283	0.07%	0.009%
90	13.389	3823	3825	3829	rBV5	1953	1299	0.07%	0.009%
91	13.508	3858	3862	3864	rBV6	2095	1784	0.10%	0.012%
92	13.582	3882	3885	3887	rBV3	2158	1310	0.07%	0.009%
93	13.813	3955	3957	3963	rBV6	2074	1738	0.10%	0.012%
94	13.939	3992	3996	3997	rBV4	1851	1191	0.07%	0.008%
95	14.109	4047	4049	4050	rBV2	1846	744	0.04%	0.005%
96	14.183	4070	4072	4075	rBV4	2020	1061	0.06%	0.007%
97	14.279	4099	4102	4105	rBV5	2201	1733	0.10%	0.012%
98	14.302	4105	4109	4110	rBV4	1951	1403	0.08%	0.010%
99	14.479	4160	4164	4167	rBV5	2305	2281	0.13%	0.016%
100	14.588	4195	4198	4199	rBV3	1818	1013	0.06%	0.007%


Sum of corrected areas: 14561257

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015200.D
Acq On : 27 Mar 2020 09:38
Operator : SY/MD
Sample : VIBLK74
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK74

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

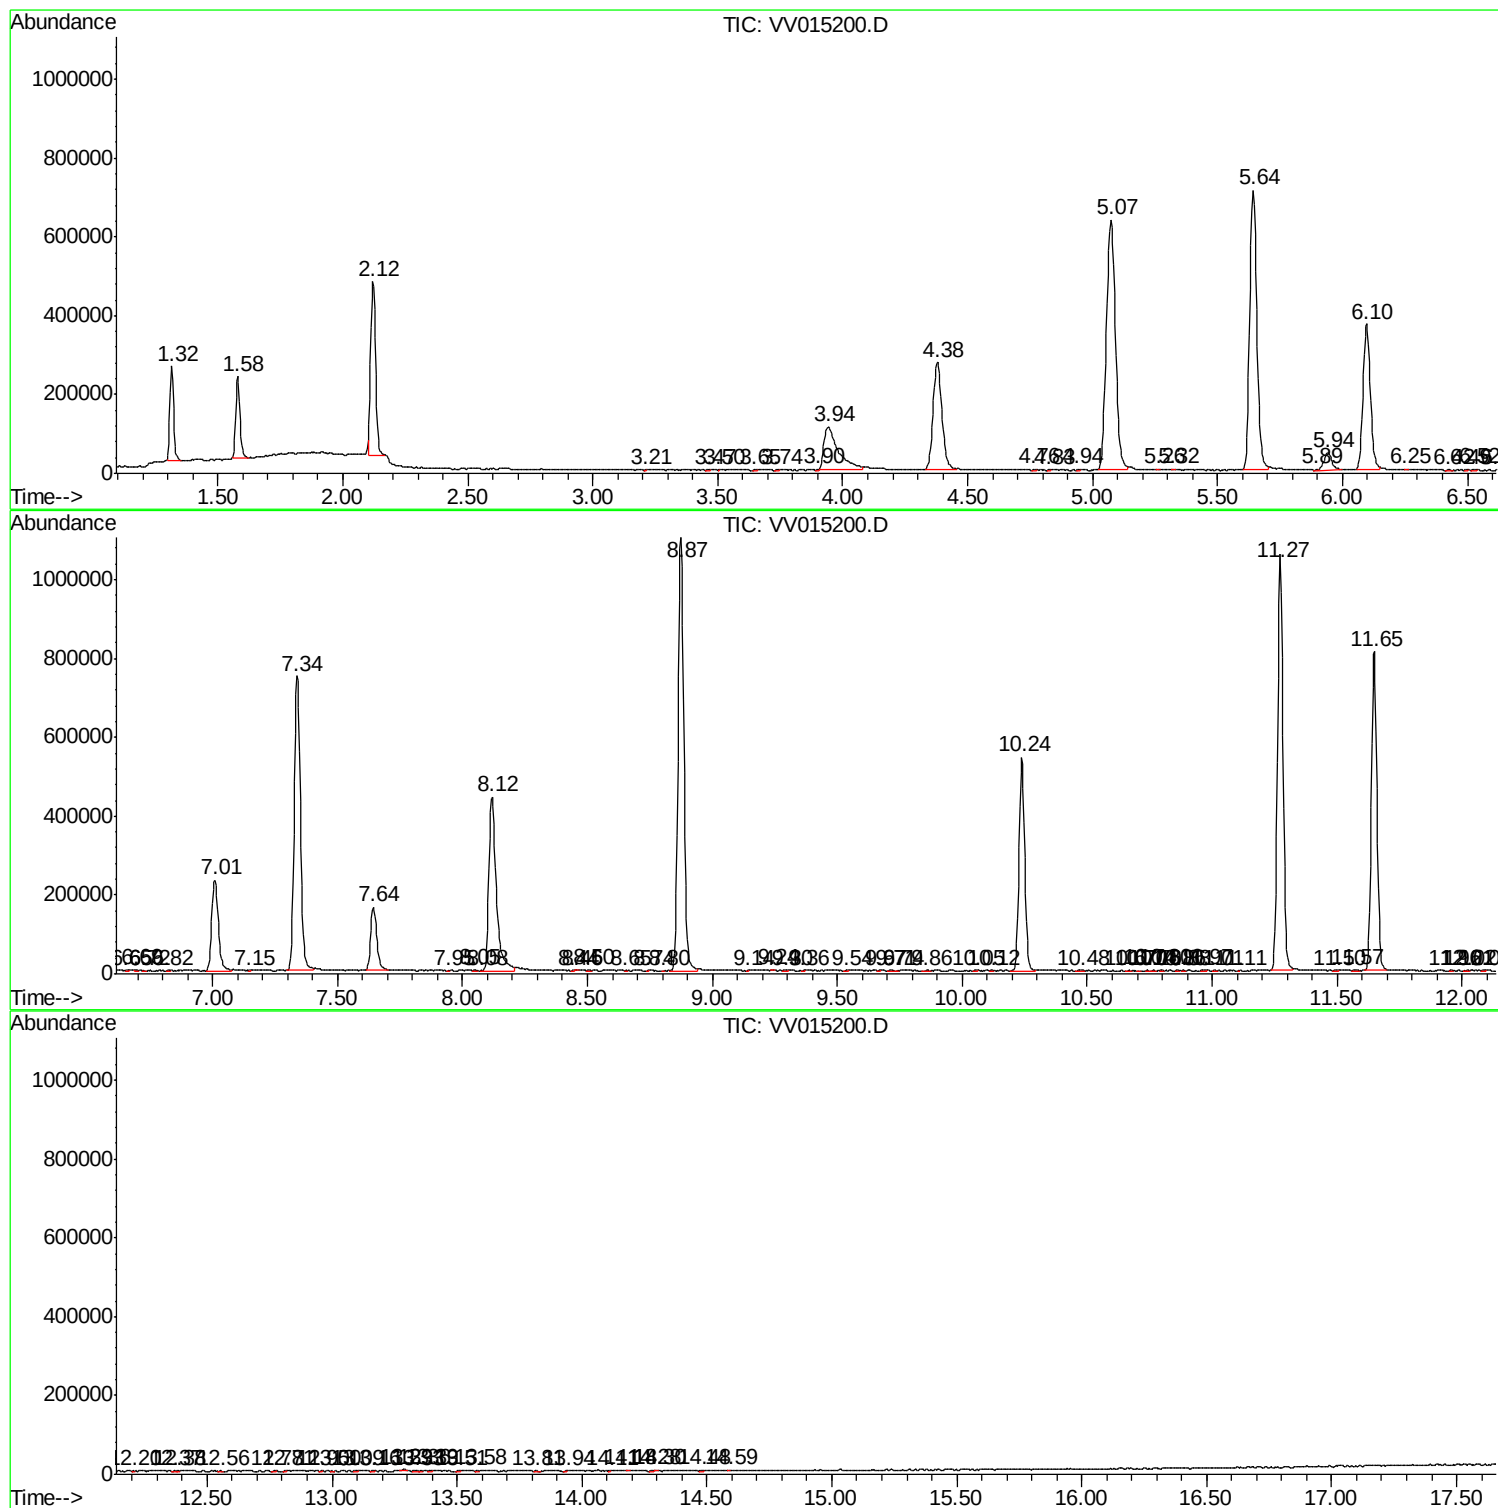

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032620\
Data File : VV015200.D
Acq On : 27 Mar 2020 09:38
Operator : SY/MD
Sample : VIBLK74
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK74

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032620\
Data File : VV015200.D
Acq On : 27 Mar 2020 09:38
Operator : SY/MD
Sample : VIBLK74
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VIBLK74

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc