

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015203.D
 Acq On : 27 Mar 2020 10:58
 Operator : SY/MD
 Sample : L1976-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTJ5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	65	70	81	rVB	236770	242507	15.77%	1.815%
2	1.579	147	152	164	rBV	193908	218214	14.19%	1.633%
3	2.119	314	320	346	rVB	431373	681008	44.28%	5.098%
4	3.135	633	636	644	rBV9	1960	2261	0.15%	0.017%
5	3.492	745	747	749	rBV4	1390	680	0.04%	0.005%
6	3.679	802	805	807	rBV3	2240	1462	0.10%	0.011%
7	3.704	811	813	816	rVV4	2048	1001	0.07%	0.007%
8	3.939	872	886	915	rBV	115785	394945	25.68%	2.956%
9	4.380	1011	1023	1042	rVB	257360	616552	40.09%	4.615%
10	4.544	1072	1074	1078	rBV3	2150	1801	0.12%	0.013%
11	4.614	1094	1096	1099	rBV4	1573	760	0.05%	0.006%
12	4.630	1099	1101	1105	rVB5	2080	1433	0.09%	0.011%
13	4.666	1109	1112	1115	rBV4	2459	2176	0.14%	0.016%
14	4.801	1152	1154	1155	rBV2	1600	809	0.05%	0.006%
15	4.852	1167	1170	1172	rBV4	1523	1078	0.07%	0.008%
16	4.865	1172	1174	1177	rVB4	2073	1115	0.07%	0.008%
17	4.884	1177	1180	1184	rBV5	1521	1212	0.08%	0.009%
18	4.904	1184	1186	1188	rBV3	1701	981	0.06%	0.007%
19	5.000	1212	1216	1219	rBV5	2292	1972	0.13%	0.015%
20	5.074	1219	1239	1267	rVV2	610204	1537986	100.00%	11.513%
21	5.399	1336	1340	1343	rBV4	2723	2069	0.13%	0.015%
22	5.495	1367	1370	1372	rBV3	2137	1245	0.08%	0.009%
23	5.643	1403	1416	1441	rBV	592845	1179549	76.69%	8.830%
24	6.097	1545	1557	1575	rBV	354749	701968	45.64%	5.255%
25	6.306	1618	1622	1623	rBV3	2873	1828	0.12%	0.014%
26	6.389	1646	1648	1650	rBV3	1340	740	0.05%	0.006%
27	6.479	1671	1676	1679	rBV6	2473	2516	0.16%	0.019%
28	6.515	1685	1687	1690	rBV4	1781	934	0.06%	0.007%
29	6.556	1696	1700	1702	rBV4	2145	1932	0.13%	0.014%
30	6.588	1708	1710	1714	rBV5	1245	775	0.05%	0.006%
31	6.643	1724	1727	1730	rBV5	2847	2092	0.14%	0.016%
32	6.794	1771	1774	1778	rVB6	2793	2115	0.14%	0.016%
33	6.814	1778	1780	1783	rVB4	1566	937	0.06%	0.007%
34	6.871	1796	1798	1801	rBV4	1579	1034	0.07%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015203.D
 Acq On : 27 Mar 2020 10:58
 Operator : SY/MD
 Sample : L1976-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTJ5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

35	6.920	1810	1813	1816	rBV5	1818	1553	0.10%	0.012%
36	7.010	1830	1841	1859	rVV	217477	389927	25.35%	2.919%
37	7.283	1922	1926	1930	rVB7	2090	1652	0.11%	0.012%
38	7.338	1930	1943	1960	rBV	705793	1227415	79.81%	9.188%
39	7.531	1997	2003	2004	rBV6	1995	1870	0.12%	0.014%
40	7.566	2010	2014	2018	rBV6	2409	1878	0.12%	0.014%
41	7.643	2028	2038	2052	rBV	156032	260102	16.91%	1.947%
42	8.116	2174	2185	2221	rBV2	434125	894978	58.19%	6.700%
43	8.341	2252	2255	2257	rBV4	2191	1288	0.08%	0.010%
44	8.531	2309	2314	2319	rBV7	3041	3378	0.22%	0.025%
45	8.569	2324	2326	2328	rBV3	1377	788	0.05%	0.006%
46	8.614	2337	2340	2341	rBV3	1948	1259	0.08%	0.009%
47	8.717	2371	2372	2376	rVB4	1526	720	0.05%	0.005%
48	8.736	2376	2378	2381	rBV4	1362	1133	0.07%	0.008%
49	8.875	2409	2421	2439	rVV	920611	1475664	95.95%	11.046%
50	9.277	2544	2546	2553	rVB8	1760	1629	0.11%	0.012%
51	9.312	2553	2557	2558	rBV4	2435	1455	0.09%	0.011%
52	9.408	2584	2587	2591	rVB5	2012	1432	0.09%	0.011%
53	9.437	2591	2596	2599	rBV7	2458	2028	0.13%	0.015%
54	9.739	2687	2690	2695	rVV6	1690	1677	0.11%	0.013%
55	9.810	2710	2712	2718	rVB7	2465	2193	0.14%	0.016%
56	9.839	2718	2721	2722	rBV3	2071	1196	0.08%	0.009%
57	10.141	2811	2815	2819	rBV6	1440	1146	0.07%	0.009%
58	10.161	2819	2821	2823	rBV3	1544	686	0.04%	0.005%
59	10.238	2835	2845	2863	rVB	514746	814454	52.96%	6.097%
60	10.392	2890	2893	2895	rVB3	2405	1160	0.08%	0.009%
61	10.405	2895	2897	2898	rBV2	1937	924	0.06%	0.007%
62	10.457	2910	2913	2917	rBV5	1370	873	0.06%	0.007%
63	10.521	2930	2933	2936	rBV4	2356	1724	0.11%	0.013%
64	10.553	2940	2943	2944	rBV3	1308	774	0.05%	0.006%
65	10.633	2964	2968	2969	rBV4	2219	1272	0.08%	0.010%
66	10.694	2984	2987	2990	rBV3	2461	1418	0.09%	0.011%
67	10.723	2990	2996	2997	rBV4	1858	1669	0.11%	0.012%
68	10.749	3002	3004	3006	rVB2	1556	727	0.05%	0.005%
69	10.858	3036	3038	3041	rBV4	2316	1498	0.10%	0.011%
70	10.874	3041	3043	3046	rBV3	2196	1503	0.10%	0.011%
71	11.051	3096	3098	3100	rBV2	1452	754	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015203.D
 Acq On : 27 Mar 2020 10:58
 Operator : SY/MD
 Sample : L1976-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTJ5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

72	11.100	3109	3113	3114	rBV4	1562	956	0.06%	0.007%
73	11.109	3114	3116	3118	rBV3	2244	1355	0.09%	0.010%
74	11.273	3155	3167	3187	rBV	891609	1371726	89.19%	10.268%
75	11.489	3229	3234	3237	rBV6	2798	2624	0.17%	0.020%
76	11.563	3248	3257	3267	rBV6	11288	21021	1.37%	0.157%
77	11.649	3272	3284	3298	rBV	771334	1207977	78.54%	9.043%
78	11.862	3348	3350	3352	rBV2	1511	929	0.06%	0.007%
79	12.141	3435	3437	3439	rBV3	1811	1131	0.07%	0.008%
80	12.228	3462	3464	3466	rBV3	1706	949	0.06%	0.007%
81	12.241	3466	3468	3471	rVV4	2172	1288	0.08%	0.010%
82	12.292	3482	3484	3486	rBV3	1906	1176	0.08%	0.009%
83	12.498	3543	3548	3554	rBV10	1792	2617	0.17%	0.020%
84	12.588	3572	3576	3577	rBV3	1522	1200	0.08%	0.009%
85	12.675	3601	3603	3611	rBV8	2674	2411	0.16%	0.018%
86	12.749	3623	3626	3629	rBV4	2814	1598	0.10%	0.012%
87	12.913	3673	3677	3678	rBV3	1966	1644	0.11%	0.012%
88	12.961	3689	3692	3696	rVB5	2509	1601	0.10%	0.012%
89	12.990	3697	3701	3703	rBV5	2178	1590	0.10%	0.012%
90	13.032	3711	3714	3715	rBV2	1970	1315	0.09%	0.010%
91	13.096	3732	3734	3735	rBV2	1888	679	0.04%	0.005%
92	13.283	3790	3792	3796	rBV5	2667	2352	0.15%	0.018%
93	13.495	3854	3858	3859	rBV4	2695	1844	0.12%	0.014%
94	13.868	3970	3974	3977	rBV5	2550	2014	0.13%	0.015%
95	14.025	4018	4023	4026	rBV8	2732	2999	0.19%	0.022%
96	14.064	4033	4035	4038	rBV3	2378	1417	0.09%	0.011%
97	14.154	4061	4063	4064	rBV2	1985	979	0.06%	0.007%
98	14.270	4095	4099	4102	rBV4	2712	2338	0.15%	0.018%
99	14.325	4113	4116	4117	rBV2	1844	997	0.06%	0.007%
100	14.823	4267	4271	4275	rBV6	2653	2558	0.17%	0.019%


Sum of corrected areas: 13358769

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015203.D
Acq On : 27 Mar 2020 10:58
Operator : SY/MD
Sample : L1976-16
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
ETTJ5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

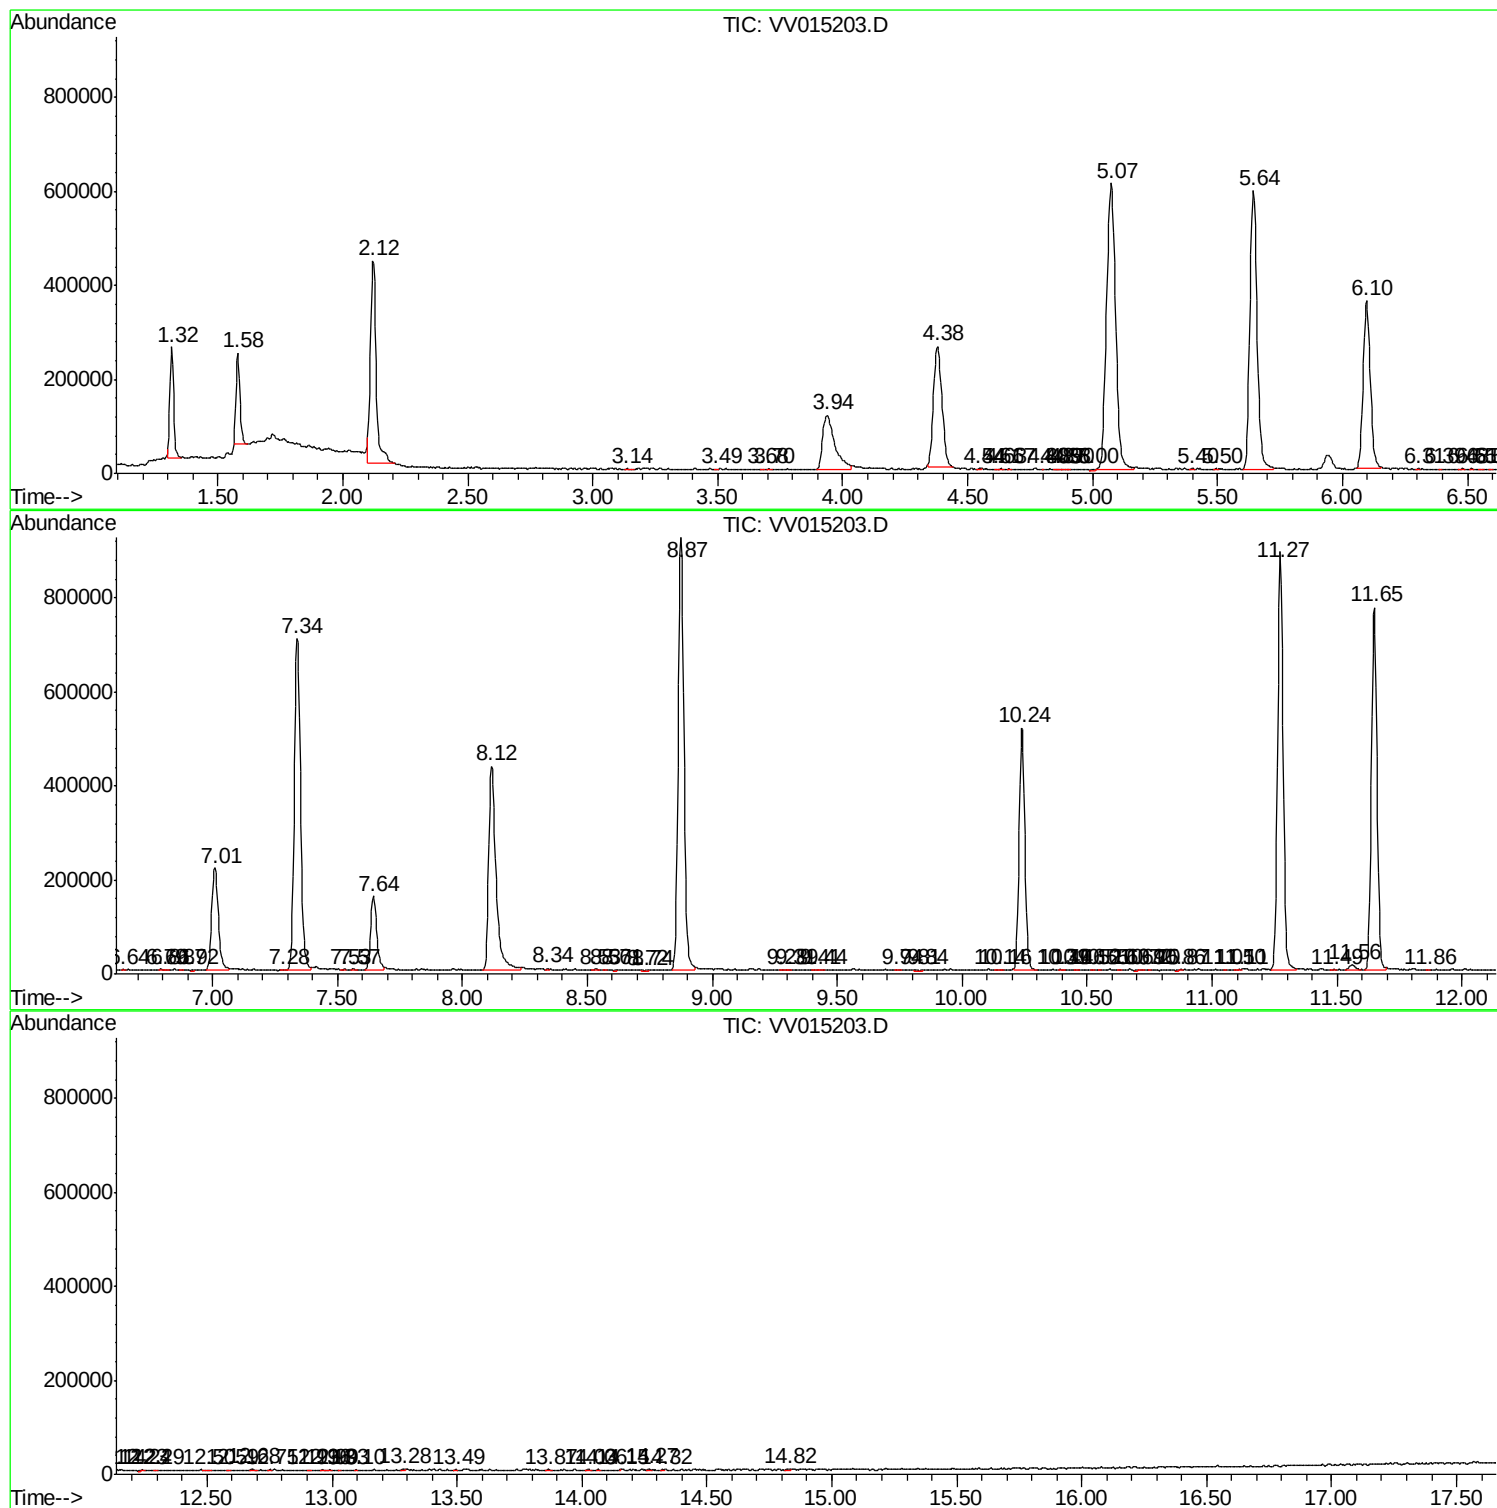

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032620\
Data File : VV015203.D
Acq On : 27 Mar 2020 10:58
Operator : SY/MD
Sample : L1976-16
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
ETTJ5

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032620\
Data File : VV015203.D
Acq On : 27 Mar 2020 10:58
Operator : SY/MD
Sample : L1976-16
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
ETTJ5

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc