

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015204.D
 Acq On : 27 Mar 2020 11:23
 Operator : SY/MD
 Sample : L1976-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTJ6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	64	69	82	rVB	251909	267759	14.22%	1.751%
2	1.579	147	152	167	rVB	215738	241555	12.82%	1.579%
3	2.119	314	320	350	rVB	477670	760984	40.40%	4.976%
4	3.090	618	622	624	rBV3	2657	2114	0.11%	0.014%
5	3.373	708	710	711	rVB2	2386	603	0.03%	0.004%
6	3.437	725	730	733	rBV6	2988	3029	0.16%	0.020%
7	3.608	780	783	785	rBV4	1824	1087	0.06%	0.007%
8	3.939	871	886	914	rBV	119750	421038	22.35%	2.753%
9	4.380	1010	1023	1049	rVB	280919	696279	36.97%	4.552%
10	4.527	1067	1069	1070	rBV3	2018	882	0.05%	0.006%
11	4.749	1136	1138	1139	rBV2	1116	339	0.02%	0.002%
12	4.762	1139	1142	1143	rBV3	1634	913	0.05%	0.006%
13	4.952	1197	1201	1203	rBV5	1678	975	0.05%	0.006%
14	4.968	1203	1206	1210	rBV4	2405	1622	0.09%	0.011%
15	4.994	1212	1214	1216	rBV3	1652	726	0.04%	0.005%
16	5.074	1223	1239	1259	rBV2	661307	1642183	87.19%	10.737%
17	5.482	1363	1366	1368	rBV4	2566	2063	0.11%	0.013%
18	5.592	1395	1400	1402	rBV6	2658	2670	0.14%	0.017%
19	5.643	1402	1416	1436	rVV	755531	1500472	79.67%	9.811%
20	5.843	1476	1478	1481	rBV4	1847	1140	0.06%	0.007%
21	6.097	1544	1557	1577	rBV	388602	780517	41.44%	5.103%
22	6.389	1646	1648	1650	rBV3	1676	787	0.04%	0.005%
23	6.479	1673	1676	1681	rBV6	2372	2705	0.14%	0.018%
24	6.608	1712	1716	1719	rBV6	2038	1848	0.10%	0.012%
25	6.756	1760	1762	1764	rBV3	1878	995	0.05%	0.007%
26	6.794	1772	1774	1778	rVB5	2583	1445	0.08%	0.009%
27	6.823	1780	1783	1784	rBV3	1056	578	0.03%	0.004%
28	6.887	1800	1803	1805	rBV4	1518	1044	0.06%	0.007%
29	6.936	1816	1818	1822	rBV5	2172	1608	0.09%	0.011%
30	7.010	1830	1841	1855	rBV2	239425	425130	22.57%	2.780%
31	7.338	1931	1943	1960	rBV	771926	1339878	71.14%	8.761%
32	7.643	2028	2038	2053	rBV	170154	288307	15.31%	1.885%
33	7.833	2094	2097	2101	rVB6	1962	1489	0.08%	0.010%
34	8.116	2174	2185	2215	rBV2	491011	972577	51.64%	6.359%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015204.D
 Acq On : 27 Mar 2020 11:23
 Operator : SY/MD
 Sample : L1976-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTJ6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

35	8.739	2376	2379	2384	rBV7	1987	2356	0.13%	0.015%
36	8.875	2409	2421	2437	rBV	1162451	1883473	100.00%	12.315%
37	9.241	2533	2535	2540	rVB5	1870	1343	0.07%	0.009%
38	9.315	2553	2558	2561	rBV5	2267	1936	0.10%	0.013%
39	9.331	2561	2563	2565	rVB2	1166	393	0.02%	0.003%
40	9.418	2587	2590	2592	rBV3	1990	1356	0.07%	0.009%
41	9.530	2622	2625	2629	rBV4	2873	2897	0.15%	0.019%
42	9.817	2712	2714	2716	rBV3	994	388	0.02%	0.003%
43	9.839	2717	2721	2724	rVB5	1635	1274	0.07%	0.008%
44	9.916	2742	2745	2749	rBV6	1867	1221	0.06%	0.008%
45	9.971	2760	2762	2765	rVB3	1576	706	0.04%	0.005%
46	10.026	2775	2779	2782	rBV5	2327	1675	0.09%	0.011%
47	10.058	2787	2789	2790	rBV2	1449	571	0.03%	0.004%
48	10.106	2801	2804	2806	rBV4	2527	1862	0.10%	0.012%
49	10.151	2815	2818	2820	rBV2	1692	965	0.05%	0.006%
50	10.238	2833	2845	2862	rBV	574450	896241	47.58%	5.860%
51	10.466	2911	2916	2917	rBV4	1692	1339	0.07%	0.009%
52	10.485	2920	2922	2924	rBV3	1050	452	0.02%	0.003%
53	10.514	2927	2931	2932	rBV4	1505	1218	0.06%	0.008%
54	10.829	3027	3029	3030	rBV2	1608	690	0.04%	0.005%
55	10.932	3059	3061	3062	rBV2	1803	738	0.04%	0.005%
56	11.051	3094	3098	3100	rBV5	2552	2108	0.11%	0.014%
57	11.270	3155	3166	3179	rBV	1139004	1739581	92.36%	11.374%
58	11.321	3179	3182	3188	rVB	26807	17880	0.95%	0.117%
59	11.444	3217	3220	3222	rBV4	2271	1409	0.07%	0.009%
60	11.534	3245	3248	3249	rBV2	1203	507	0.03%	0.003%
61	11.563	3249	3257	3261	rBV5	8505	13315	0.71%	0.087%
62	11.646	3272	3283	3302	rBV	845490	1323342	70.26%	8.652%
63	11.836	3341	3342	3346	rVB3	1888	904	0.05%	0.006%
64	11.910	3363	3365	3367	rBV3	1352	743	0.04%	0.005%
65	12.019	3396	3399	3405	rVB6	3242	3024	0.16%	0.020%
66	12.090	3418	3421	3423	rBV4	1862	1138	0.06%	0.007%
67	12.328	3493	3495	3498	rBV4	2170	1029	0.05%	0.007%
68	12.437	3527	3529	3530	rBV2	1263	440	0.02%	0.003%
69	12.563	3565	3568	3570	rBV4	1545	1051	0.06%	0.007%
70	12.649	3594	3595	3597	rBV2	991	486	0.03%	0.003%
71	12.894	3669	3671	3672	rBV2	1703	759	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015204.D
 Acq On : 27 Mar 2020 11:23
 Operator : SY/MD
 Sample : L1976-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTJ6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

72	12.971	3692	3695	3697	rBV4	1379	830	0.04%	0.005%
73	13.058	3720	3722	3724	rBV3	2745	1520	0.08%	0.010%
74	13.128	3742	3744	3745	rVB2	1166	326	0.02%	0.002%
75	13.148	3748	3750	3753	rBV3	1965	1389	0.07%	0.009%
76	13.286	3790	3793	3796	rBV5	4521	3167	0.17%	0.021%
77	13.389	3823	3825	3829	rBV5	1710	1224	0.06%	0.008%
78	13.743	3929	3935	3937	rBV6	2511	2510	0.13%	0.016%
79	14.045	4026	4029	4031	rVB3	1979	921	0.05%	0.006%
80	14.379	4131	4133	4136	rBV3	1498	919	0.05%	0.006%
81	14.569	4190	4192	4195	rBV4	1870	1144	0.06%	0.007%
82	14.694	4229	4231	4233	rBV3	1706	738	0.04%	0.005%
83	14.935	4303	4306	4308	rBV5	2338	1661	0.09%	0.011%


Sum of corrected areas: 15294500

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015204.D
Acq On : 27 Mar 2020 11:23
Operator : SY/MD
Sample : L1976-17
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTJ6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

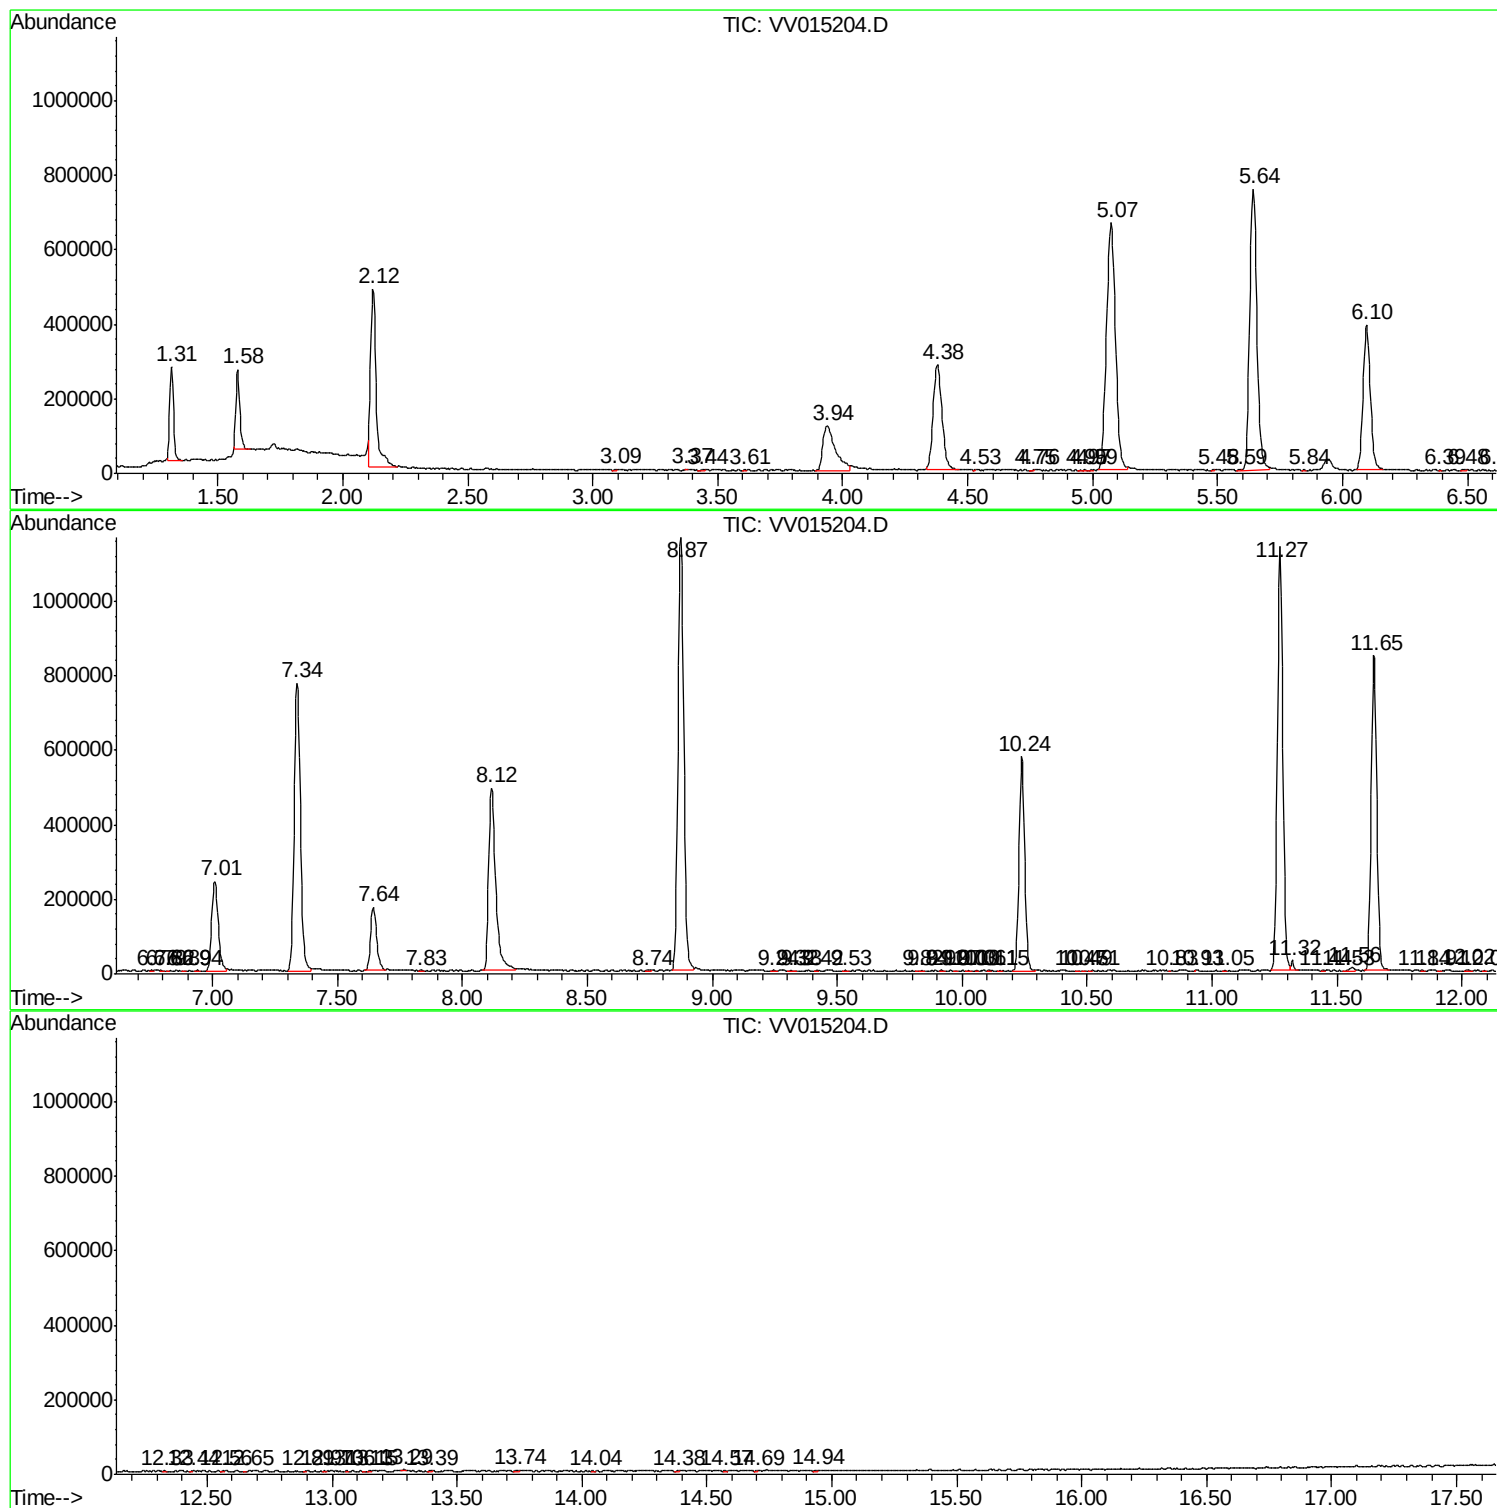

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032620\
Data File : VV015204.D
Acq On : 27 Mar 2020 11:23
Operator : SY/MD
Sample : L1976-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTJ6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032620\
Data File : VV015204.D
Acq On : 27 Mar 2020 11:23
Operator : SY/MD
Sample : L1976-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTJ6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc