

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015206.D
 Acq On : 27 Mar 2020 12:11
 Operator : SY/MD
 Sample : L1976-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTJ3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	65	70	80	rVB	254476	251135	12.84%	1.632%
2	1.579	147	152	166	rVB	215300	254796	13.02%	1.656%
3	2.119	313	320	333	rVB	448917	638185	32.62%	4.148%
4	2.843	543	545	551	rVB7	2624	1817	0.09%	0.012%
5	3.270	676	678	680	rBV3	1662	947	0.05%	0.006%
6	3.489	744	746	749	rBV4	1065	586	0.03%	0.004%
7	3.508	749	752	754	rVV4	1182	611	0.03%	0.004%
8	3.544	761	763	768	rBV6	2168	1749	0.09%	0.011%
9	3.566	768	770	773	rBV4	1614	1133	0.06%	0.007%
10	3.656	796	798	800	rBV3	1073	737	0.04%	0.005%
11	3.698	804	811	813	rBV7	2311	2359	0.12%	0.015%
12	3.859	859	861	863	rBV3	1398	803	0.04%	0.005%
13	3.942	870	887	915	rBV	103250	394993	20.19%	2.567%
14	4.380	1008	1023	1047	rBV	280147	692466	35.39%	4.500%
15	4.646	1102	1106	1111	rVB8	2549	2423	0.12%	0.016%
16	5.074	1222	1239	1264	rBV2	657174	1657088	84.69%	10.770%
17	5.588	1396	1399	1401	rBV3	2308	1342	0.07%	0.009%
18	5.643	1403	1416	1440	rVV	781508	1574133	80.45%	10.230%
19	5.875	1485	1488	1491	rVB4	1872	1096	0.06%	0.007%
20	5.894	1491	1494	1495	rBV2	2090	1144	0.06%	0.007%
21	5.942	1499	1509	1524	rVB8	25263	54625	2.79%	0.355%
22	6.096	1542	1557	1575	rBV	387790	794320	40.60%	5.162%
23	6.267	1607	1610	1612	rBV4	2282	1865	0.10%	0.012%
24	6.350	1634	1636	1637	rBV2	899	476	0.02%	0.003%
25	6.402	1651	1652	1655	rBV3	1157	718	0.04%	0.005%
26	6.678	1736	1738	1741	rVB3	2511	1061	0.05%	0.007%
27	6.733	1751	1755	1757	rBV5	1839	1691	0.09%	0.011%
28	6.897	1803	1806	1808	rBV4	2051	1229	0.06%	0.008%
29	6.955	1822	1824	1826	rBV3	997	511	0.03%	0.003%
30	7.010	1829	1841	1862	rVV	238160	434404	22.20%	2.823%
31	7.151	1876	1885	1889	rBV	2759	4153	0.21%	0.027%
32	7.231	1909	1910	1913	rVB4	1658	839	0.04%	0.005%
33	7.338	1931	1943	1963	rBV	783113	1347767	68.88%	8.759%
34	7.643	2028	2038	2054	rBV	164786	290486	14.85%	1.888%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015206.D
 Acq On : 27 Mar 2020 12:11
 Operator : SY/MD
 Sample : L1976-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTJ3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

35	8.022	2154	2156	2157	rBV2	1846	719	0.04%	0.005%
36	8.058	2161	2167	2171	rBV9	1965	2013	0.10%	0.013%
37	8.119	2175	2186	2212	rBV2	457615	939363	48.01%	6.105%
38	8.373	2263	2265	2267	rBV3	2189	1243	0.06%	0.008%
39	8.498	2302	2304	2306	rBV3	2248	1059	0.05%	0.007%
40	8.611	2333	2339	2342	rBV7	1966	1993	0.10%	0.013%
41	8.730	2373	2376	2379	rBV5	2404	1724	0.09%	0.011%
42	8.756	2381	2384	2385	rBV3	1836	1087	0.06%	0.007%
43	8.788	2392	2394	2396	rBV3	1356	553	0.03%	0.004%
44	8.874	2409	2421	2439	rBV	1220340	1956629	100.00%	12.716%
45	9.408	2585	2587	2588	rBV2	1275	407	0.02%	0.003%
46	9.418	2588	2590	2592	rVB3	1911	733	0.04%	0.005%
47	9.456	2600	2602	2606	rVB5	1771	1217	0.06%	0.008%
48	9.514	2618	2620	2623	rBV3	1720	886	0.05%	0.006%
49	9.550	2629	2631	2633	rBV3	1196	496	0.03%	0.003%
50	9.572	2634	2638	2639	rBV3	2218	1409	0.07%	0.009%
51	9.669	2666	2668	2671	rBV4	1255	830	0.04%	0.005%
52	9.717	2680	2683	2686	rBV6	1756	981	0.05%	0.006%
53	9.749	2690	2693	2700	rVB7	1842	2098	0.11%	0.014%
54	9.778	2700	2702	2703	rBV2	1325	583	0.03%	0.004%
55	9.797	2707	2708	2710	rBV2	1393	645	0.03%	0.004%
56	9.829	2715	2718	2720	rBV4	1517	1011	0.05%	0.007%
57	9.862	2726	2728	2730	rBV3	1474	633	0.03%	0.004%
58	10.106	2803	2804	2807	rBV3	1434	888	0.05%	0.006%
59	10.238	2834	2845	2861	rBV	568379	881639	45.06%	5.730%
60	10.450	2906	2911	2914	rBV6	2538	1989	0.10%	0.013%
61	10.601	2952	2958	2960	rBV6	2150	2335	0.12%	0.015%
62	10.746	2998	3003	3004	rBV5	1649	1321	0.07%	0.009%
63	10.804	3018	3021	3025	rVB5	863	602	0.03%	0.004%
64	10.826	3026	3028	3030	rVB4	1344	422	0.02%	0.003%
65	10.852	3033	3036	3037	rBV3	1236	724	0.04%	0.005%
66	10.926	3056	3059	3060	rBV3	2172	1069	0.05%	0.007%
67	11.048	3094	3097	3100	rBV5	1153	846	0.04%	0.005%
68	11.090	3107	3110	3113	rBV3	2220	1895	0.10%	0.012%
69	11.138	3124	3125	3128	rBV3	1047	472	0.02%	0.003%
70	11.273	3155	3167	3186	rBV	1187082	1818197	92.92%	11.817%
71	11.649	3273	3284	3301	rVB	842680	1312076	67.06%	8.527%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015206.D
 Acq On : 27 Mar 2020 12:11
 Operator : SY/MD
 Sample : L1976-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTJ3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

72	11.868	3350	3352	3353	rBV2	1190	305	0.02%	0.002%
73	11.935	3369	3373	3378	rBV8	2678	2943	0.15%	0.019%
74	12.035	3402	3404	3405	rBV2	1534	604	0.03%	0.004%
75	12.206	3453	3457	3459	rBV4	2160	1656	0.08%	0.011%
76	12.386	3509	3513	3518	rVB7	2567	2381	0.12%	0.015%
77	12.411	3518	3521	3522	rBV3	1326	815	0.04%	0.005%
78	12.434	3526	3528	3530	rBV3	1253	665	0.03%	0.004%
79	12.553	3560	3565	3568	rBV8	2124	2315	0.12%	0.015%
80	12.665	3595	3600	3603	rBV7	3989	3732	0.19%	0.024%
81	12.701	3609	3611	3612	rBV2	1290	654	0.03%	0.004%
82	12.794	3637	3640	3643	rVB4	2150	1221	0.06%	0.008%
83	12.865	3659	3662	3665	rBV5	1448	890	0.05%	0.006%
84	12.987	3698	3700	3704	rBV4	1284	831	0.04%	0.005%
85	13.016	3704	3709	3712	rBV7	1952	2279	0.12%	0.015%
86	13.074	3725	3727	3729	rBV3	1976	950	0.05%	0.006%
87	13.218	3770	3772	3774	rVB3	2395	878	0.04%	0.006%
88	13.231	3774	3776	3779	rVB4	1622	874	0.04%	0.006%
89	13.257	3782	3784	3785	rBV2	1411	590	0.03%	0.004%
90	13.353	3811	3814	3816	rBV3	2381	1483	0.08%	0.010%
91	13.370	3816	3819	3821	rBV3	1026	544	0.03%	0.004%
92	13.418	3830	3834	3837	rBV7	1218	846	0.04%	0.005%
93	13.508	3860	3862	3865	rBV4	1023	619	0.03%	0.004%
94	13.524	3865	3867	3868	rBV2	1673	670	0.03%	0.004%
95	13.935	3993	3995	3999	rBV4	1811	1632	0.08%	0.011%


Sum of corrected areas: 15386852

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015206.D
Acq On : 27 Mar 2020 12:11
Operator : SY/MD
Sample : L1976-14
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTJ3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

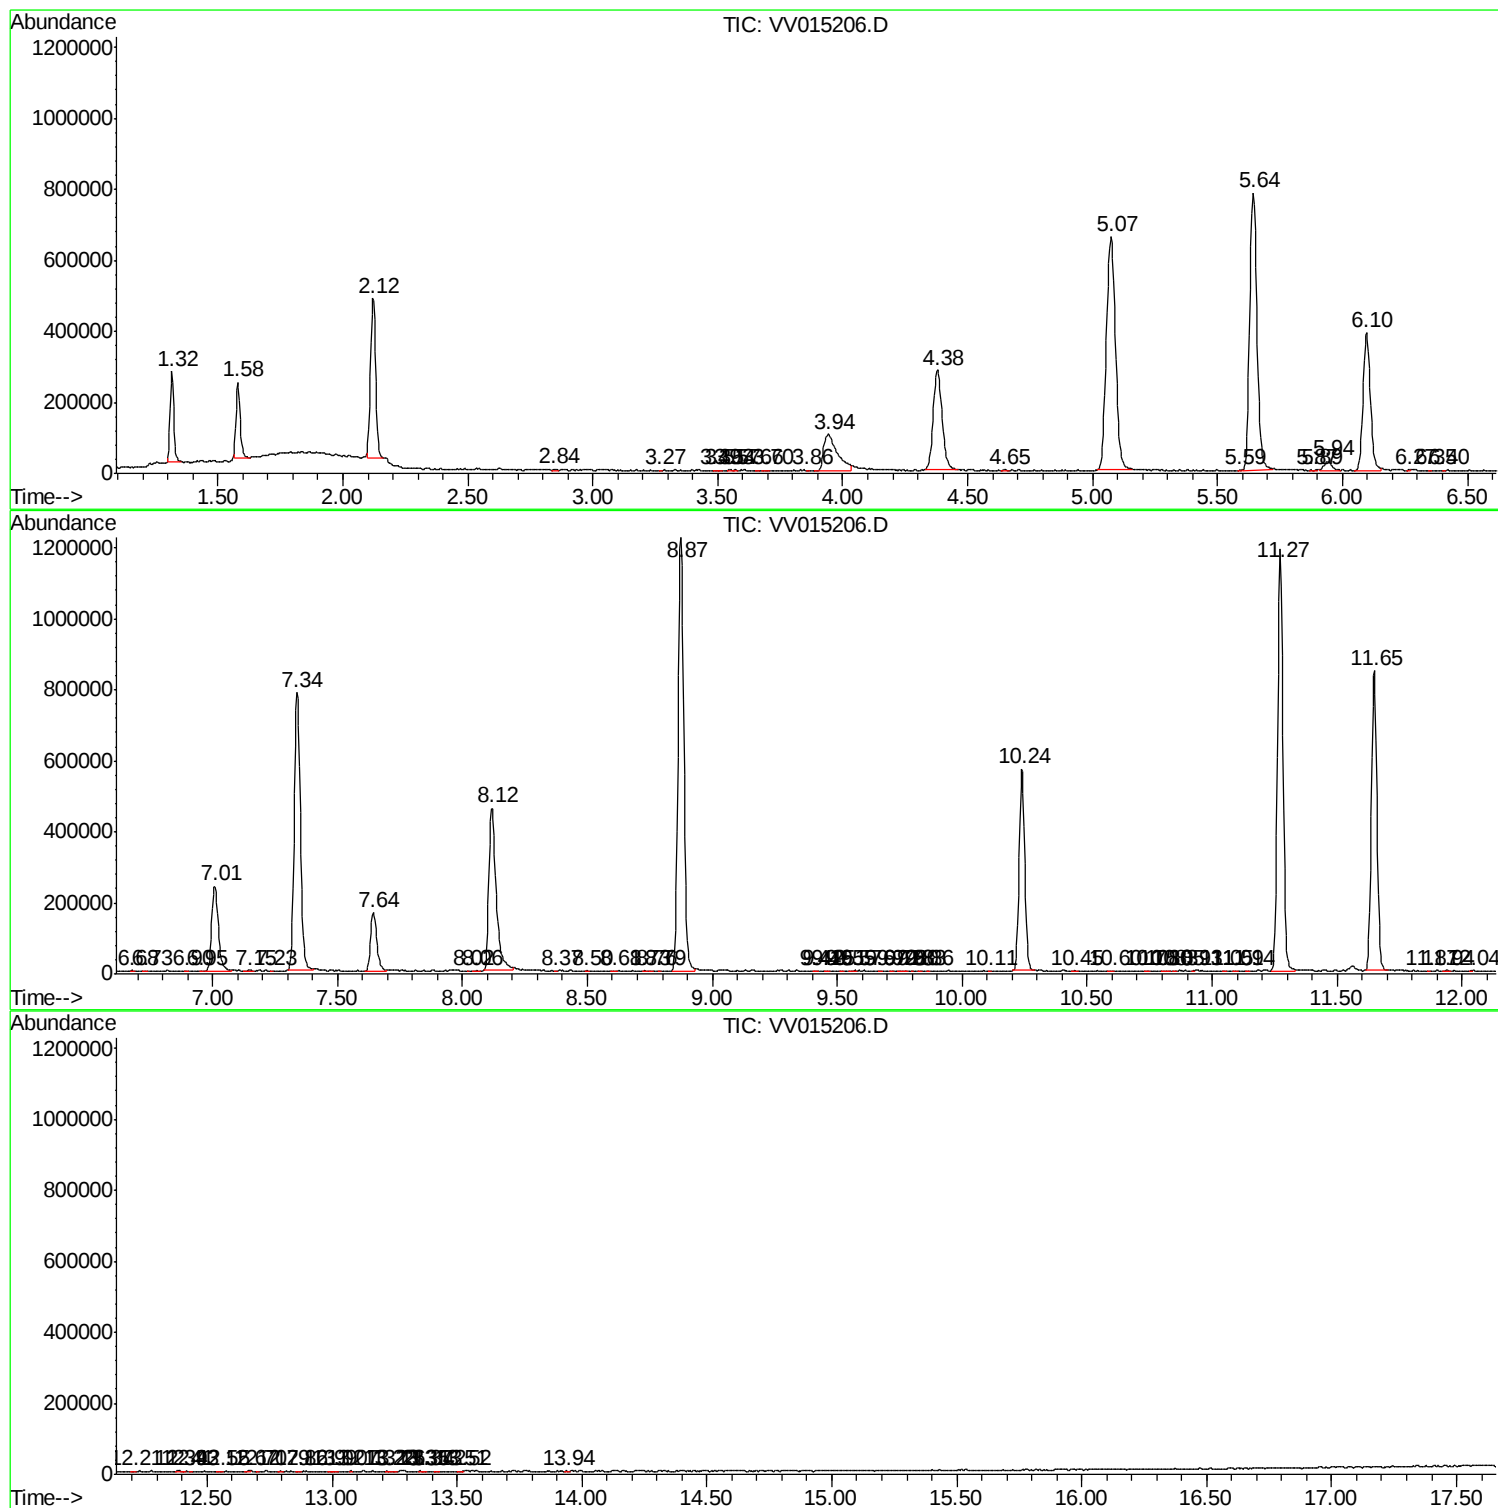

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032620\
Data File : VV015206.D
Acq On : 27 Mar 2020 12:11
Operator : SY/MD
Sample : L1976-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTJ3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032620\
Data File : VV015206.D
Acq On : 27 Mar 2020 12:11
Operator : SY/MD
Sample : L1976-14
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
ETTJ3

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc