

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015207.D
 Acq On : 27 Mar 2020 12:36
 Operator : SY/MD
 Sample : VIBLK75
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK75

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	81	rVB	248017	255482	12.58%	1.610%
2	1.576	146	151	166	rVB	219164	257778	12.69%	1.624%
3	2.119	313	320	341	rVB	488105	751194	36.98%	4.734%
4	2.875	553	555	556	rBV2	1525	499	0.02%	0.003%
5	3.428	723	727	729	rBV5	1890	1536	0.08%	0.010%
6	3.627	787	789	791	rBV3	1330	633	0.03%	0.004%
7	3.711	812	815	818	rBV4	1521	1102	0.05%	0.007%
8	3.878	865	867	869	rBV2	2411	1458	0.07%	0.009%
9	3.942	874	887	921	rBV2	106921	437615	21.54%	2.758%
10	4.377	1010	1022	1047	rVB	286216	699405	34.43%	4.407%
11	4.666	1110	1112	1117	rBV6	1551	1176	0.06%	0.007%
12	4.798	1149	1153	1156	rBV4	1810	1647	0.08%	0.010%
13	4.920	1189	1191	1193	rBV3	1498	520	0.03%	0.003%
14	5.074	1218	1239	1261	rBV2	673069	1689880	83.18%	10.649%
15	5.393	1336	1338	1339	rBV2	1624	773	0.04%	0.005%
16	5.470	1358	1362	1364	rBV5	1813	1421	0.07%	0.009%
17	5.499	1369	1371	1373	rBV3	1961	1160	0.06%	0.007%
18	5.640	1401	1415	1438	rBV	819478	1625664	80.02%	10.245%
19	5.881	1488	1490	1493	rBV3	2098	1239	0.06%	0.008%
20	6.097	1544	1557	1577	rBV	389964	790765	38.92%	4.983%
21	6.434	1659	1662	1665	rBV5	2178	1645	0.08%	0.010%
22	6.470	1671	1673	1674	rBV2	1814	822	0.04%	0.005%
23	6.920	1811	1813	1818	rBV5	1627	1230	0.06%	0.008%
24	6.965	1825	1827	1829	rBV3	1055	566	0.03%	0.004%
25	7.010	1829	1841	1858	rBV	239362	438233	21.57%	2.762%
26	7.338	1931	1943	1961	rBV	774251	1339842	65.95%	8.443%
27	7.643	2027	2038	2056	rBV2	169515	295348	14.54%	1.861%
28	8.116	2174	2185	2215	rBV2	491338	1017522	50.09%	6.412%
29	8.547	2317	2319	2322	rBV4	1731	1237	0.06%	0.008%
30	8.785	2391	2393	2396	rVB4	1736	992	0.05%	0.006%
31	8.820	2402	2404	2407	rBV4	2242	1244	0.06%	0.008%
32	8.875	2410	2421	2449	rVB	1260243	2031589	100.00%	12.803%
33	9.190	2517	2519	2521	rBV4	2289	1076	0.05%	0.007%
34	9.293	2547	2551	2554	rBV4	2861	2250	0.11%	0.014%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015207.D
 Acq On : 27 Mar 2020 12:36
 Operator : SY/MD
 Sample : VIBLK75
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK75

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

35	9.306	2554	2555	2558	rBV3	888	642	0.03%	0.004%
36	9.322	2558	2560	2562	rBV3	1158	625	0.03%	0.004%
37	9.335	2562	2564	2567	rBV4	1206	806	0.04%	0.005%
38	9.373	2574	2576	2577	rVB2	1193	341	0.02%	0.002%
39	9.405	2583	2586	2587	rBV3	1417	833	0.04%	0.005%
40	9.431	2591	2594	2597	rBB4	1084	683	0.03%	0.004%
41	9.524	2619	2623	2625	rBV5	2076	1524	0.08%	0.010%
42	9.592	2642	2644	2647	rBV2	2445	1149	0.06%	0.007%
43	9.656	2662	2664	2667	rVB5	2009	1029	0.05%	0.006%
44	9.955	2754	2757	2760	rBV6	2511	1700	0.08%	0.011%
45	10.093	2799	2800	2801	rBV	1587	506	0.02%	0.003%
46	10.151	2813	2818	2822	rBV7	2225	2113	0.10%	0.013%
47	10.193	2829	2831	2833	rVB3	2297	1070	0.05%	0.007%
48	10.238	2833	2845	2861	rBV	583354	917152	45.14%	5.780%
49	10.476	2917	2919	2921	rBV3	986	536	0.03%	0.003%
50	10.563	2942	2946	2951	rBV7	3570	3523	0.17%	0.022%
51	10.662	2975	2977	2980	rBV4	1145	653	0.03%	0.004%
52	10.733	2996	2999	3001	rBV4	1582	599	0.03%	0.004%
53	10.746	3001	3003	3005	rBV3	1217	639	0.03%	0.004%
54	10.762	3005	3008	3009	rBV2	1111	728	0.04%	0.005%
55	10.801	3016	3020	3021	rBV3	1872	1313	0.06%	0.008%
56	10.904	3048	3052	3056	rBV7	2652	2021	0.10%	0.013%
57	10.932	3056	3061	3063	rVV6	1816	1531	0.08%	0.010%
58	11.077	3103	3106	3108	rBV4	2314	1767	0.09%	0.011%
59	11.273	3155	3167	3186	rBV	1222791	1900941	93.57%	11.979%
60	11.514	3240	3242	3244	rBV3	1522	720	0.04%	0.005%
61	11.527	3244	3246	3248	rBV3	1817	1115	0.05%	0.007%
62	11.537	3248	3249	3250	rBV	2144	720	0.04%	0.005%
63	11.650	3272	3284	3299	rBV	850425	1331875	65.56%	8.393%
64	11.810	3331	3334	3338	rBV5	2193	1619	0.08%	0.010%
65	11.971	3382	3384	3389	rBV4	2214	1863	0.09%	0.012%
66	12.010	3392	3396	3399	rBV5	2679	2500	0.12%	0.016%
67	12.048	3406	3408	3409	rBV2	2103	969	0.05%	0.006%
68	12.235	3462	3466	3469	rVB6	2852	2219	0.11%	0.014%
69	12.254	3469	3472	3474	rBV4	2358	1723	0.08%	0.011%
70	12.315	3489	3491	3496	rVB5	2393	1405	0.07%	0.009%
71	12.350	3501	3502	3503	rBV	374	87	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015207.D
Acq On : 27 Mar 2020 12:36
Operator : SY/MD
Sample : VIBLK75
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK75

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Title : VOC Analysis

72	12.360	3503	3505	3507	rVB3	1381	547	0.03%	0.003%
73	12.437	3526	3529	3534	rBV6	1988	1526	0.08%	0.010%
74	12.678	3597	3604	3608	rBV10	2722	3566	0.18%	0.022%
75	12.743	3622	3624	3629	rBV5	2000	1165	0.06%	0.007%
76	13.174	3752	3758	3760	rBV7	2260	2086	0.10%	0.013%
77	13.212	3766	3770	3771	rBV3	2004	1333	0.07%	0.008%
78	13.254	3781	3783	3786	rBV4	1697	1029	0.05%	0.006%
79	13.444	3840	3842	3844	rVB3	1411	542	0.03%	0.003%
80	13.511	3859	3863	3865	rBV4	2362	2184	0.11%	0.014%
81	13.646	3902	3905	3908	rBV4	2727	2095	0.10%	0.013%
82	13.849	3964	3968	3971	rBV5	2030	1304	0.06%	0.008%
83	13.865	3971	3973	3977	rBV3	1641	870	0.04%	0.005%
84	14.122	4049	4053	4054	rBV4	2749	1845	0.09%	0.012%
85	15.122	4360	4364	4368	rBV5	3186	2726	0.13%	0.017%


Sum of corrected areas: 15868600

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015207.D
Acq On : 27 Mar 2020 12:36
Operator : SY/MD
Sample : VIBLK75
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK75

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

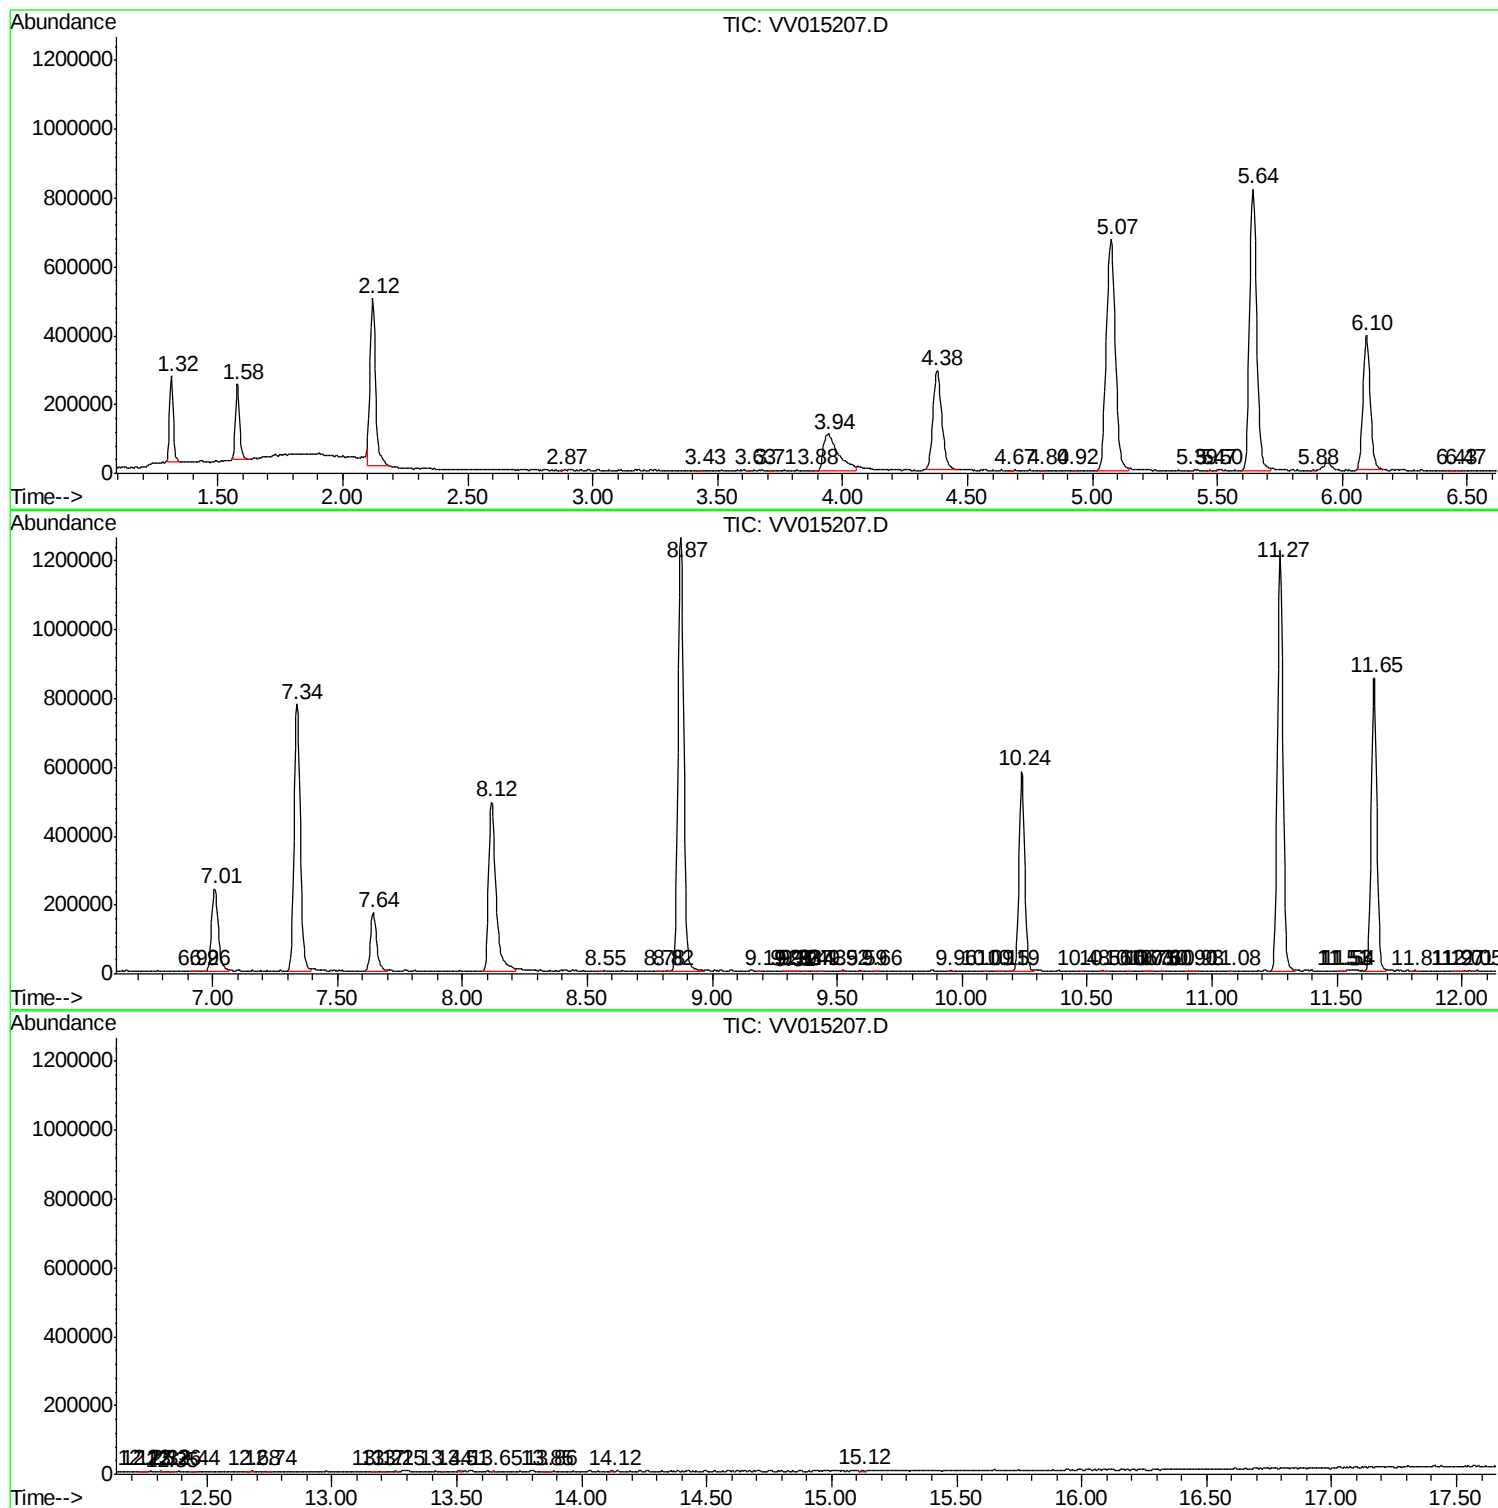

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032620\
Data File : VV015207.D
Acq On : 27 Mar 2020 12:36
Operator : SY/MD
Sample : VIBLK75
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK75

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032620\
Data File : VV015207.D
Acq On : 27 Mar 2020 12:36
Operator : SY/MD
Sample : VIBLK75
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VIBLK75

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc