

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015208.D
 Acq On : 27 Mar 2020 13:00
 Operator : SY/MD
 Sample : L2045-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	65	70	83	rVB	236182	241329	11.88%	1.562%
2	1.579	146	152	165	rVB	212691	251285	12.37%	1.626%
3	2.119	314	320	332	rVB	437728	604134	29.74%	3.910%
4	3.103	623	626	629	rBV5	2356	1802	0.09%	0.012%
5	3.151	637	641	642	rBV4	2478	1759	0.09%	0.011%
6	3.405	718	720	721	rBV2	1712	715	0.04%	0.005%
7	3.470	736	740	744	rVB6	2744	2523	0.12%	0.016%
8	3.733	818	822	823	rBV3	2857	1737	0.09%	0.011%
9	3.839	853	855	861	rBV7	1765	1667	0.08%	0.011%
10	3.942	876	887	909	rBV2	96843	363046	17.87%	2.350%
11	4.380	1010	1023	1048	rVB2	274089	684996	33.72%	4.433%
12	5.074	1222	1239	1268	rBV2	652606	1650581	81.25%	10.683%
13	5.338	1317	1321	1323	rBV4	1480	1075	0.05%	0.007%
14	5.399	1337	1340	1341	rBV2	1599	743	0.04%	0.005%
15	5.643	1401	1416	1440	rBV	821490	1636331	80.55%	10.591%
16	6.036	1536	1538	1542	rBV4	1780	1137	0.06%	0.007%
17	6.097	1544	1557	1582	rVB	384077	786648	38.72%	5.091%
18	6.302	1618	1621	1624	rBV4	2301	1516	0.07%	0.010%
19	6.499	1679	1682	1686	rBV6	2184	1888	0.09%	0.012%
20	6.630	1720	1723	1725	rBV4	1564	909	0.04%	0.006%
21	6.679	1736	1738	1740	rBV3	1913	902	0.04%	0.006%
22	6.852	1789	1792	1797	rVB7	3126	2717	0.13%	0.018%
23	6.875	1797	1799	1801	rBV3	2691	1565	0.08%	0.010%
24	7.010	1831	1841	1865	rVB	237677	419691	20.66%	2.716%
25	7.228	1906	1909	1912	rBV5	2600	1892	0.09%	0.012%
26	7.257	1916	1918	1920	rBV2	1984	1185	0.06%	0.008%
27	7.338	1931	1943	1965	rBV	774868	1319150	64.93%	8.538%
28	7.643	2029	2038	2055	rBV	165199	278058	13.69%	1.800%
29	7.849	2100	2102	2104	rBV2	2103	979	0.05%	0.006%
30	7.945	2128	2132	2135	rBV5	2264	2335	0.11%	0.015%
31	8.048	2160	2164	2165	rBV3	2314	1422	0.07%	0.009%
32	8.074	2170	2172	2174	rBV3	1313	696	0.03%	0.005%
33	8.116	2175	2185	2215	rBV2	468694	978326	48.16%	6.332%
34	8.508	2304	2307	2310	rBV5	1558	1315	0.06%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015208.D
 Acq On : 27 Mar 2020 13:00
 Operator : SY/MD
 Sample : L2045-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

35	8.543	2315	2318	2321	rBV5	1641	1011	0.05%	0.007%
36	8.627	2338	2344	2348	rBV7	2325	3013	0.15%	0.020%
37	8.650	2348	2351	2353	rBV4	1574	1040	0.05%	0.007%
38	8.685	2360	2362	2366	rBV4	1129	734	0.04%	0.005%
39	8.788	2391	2394	2398	rBV6	2509	1702	0.08%	0.011%
40	8.875	2409	2421	2447	rBV	1257348	2031494	100.00%	13.148%
41	9.219	2525	2528	2529	rBV3	1582	726	0.04%	0.005%
42	9.376	2575	2577	2578	rBV2	1873	726	0.04%	0.005%
43	9.556	2631	2633	2635	rBV3	1359	677	0.03%	0.004%
44	9.685	2669	2673	2676	rVB5	2115	1478	0.07%	0.010%
45	9.730	2681	2687	2689	rBV6	2003	1688	0.08%	0.011%
46	9.788	2703	2705	2709	rVB4	1857	981	0.05%	0.006%
47	9.862	2727	2728	2731	rVB3	2095	863	0.04%	0.006%
48	9.884	2731	2735	2736	rBV4	1515	1152	0.06%	0.007%
49	9.932	2748	2750	2752	rBV3	1495	805	0.04%	0.005%
50	10.068	2790	2792	2794	rBV3	1495	900	0.04%	0.006%
51	10.109	2803	2805	2806	rBV2	1559	759	0.04%	0.005%
52	10.132	2810	2812	2817	rVV5	2062	1591	0.08%	0.010%
53	10.167	2821	2823	2826	rBV3	1845	981	0.05%	0.006%
54	10.238	2834	2845	2867	rBV	573585	883927	43.51%	5.721%
55	10.511	2926	2930	2934	rVB7	2320	2060	0.10%	0.013%
56	10.531	2934	2936	2937	rBV2	1605	658	0.03%	0.004%
57	10.595	2953	2956	2958	rBV4	1267	765	0.04%	0.005%
58	10.624	2962	2965	2967	rBV4	2013	1306	0.06%	0.008%
59	10.698	2984	2988	2989	rBV4	2274	1367	0.07%	0.009%
60	10.762	3003	3008	3009	rBV5	1493	1180	0.06%	0.008%
61	10.810	3021	3023	3025	rVB2	1655	713	0.04%	0.005%
62	10.875	3039	3043	3045	rBV5	2564	2037	0.10%	0.013%
63	10.942	3061	3064	3067	rBV6	2326	1518	0.07%	0.010%
64	11.029	3088	3091	3093	rBV4	2239	1331	0.07%	0.009%
65	11.074	3103	3105	3107	rBV3	1739	817	0.04%	0.005%
66	11.093	3107	3111	3113	rBV5	899	655	0.03%	0.004%
67	11.119	3117	3119	3122	rBV3	2140	985	0.05%	0.006%
68	11.167	3128	3134	3137	rBV7	2616	3328	0.16%	0.022%
69	11.270	3155	3166	3189	rBV	1238662	1899750	93.51%	12.295%
70	11.646	3271	3283	3302	rVV	835511	1309938	64.48%	8.478%
71	11.900	3359	3362	3365	rBV3	2086	1279	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015208.D
 Acq On : 27 Mar 2020 13:00
 Operator : SY/MD
 Sample : L2045-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

72	11.974	3381	3385	3386	rBV3	3045	1775	0.09%	0.011%
73	12.019	3397	3399	3401	rBV3	1442	866	0.04%	0.006%
74	12.048	3406	3408	3412	rVB5	2216	1278	0.06%	0.008%
75	12.251	3470	3471	3473	rBV2	1795	949	0.05%	0.006%
76	12.312	3486	3490	3494	rBV7	1726	1873	0.09%	0.012%
77	12.370	3505	3508	3510	rBV3	2307	1173	0.06%	0.008%
78	12.463	3533	3537	3541	rBV5	1759	1582	0.08%	0.010%
79	12.537	3558	3560	3563	rBV4	1406	1005	0.05%	0.007%
80	12.749	3624	3626	3629	rBV4	1597	833	0.04%	0.005%
81	12.775	3629	3634	3637	rBV7	1239	1209	0.06%	0.008%
82	12.794	3637	3640	3641	rBV4	1645	823	0.04%	0.005%
83	12.936	3681	3684	3686	rBV4	2036	1361	0.07%	0.009%
84	13.006	3700	3706	3708	rBV7	1677	1795	0.09%	0.012%
85	13.016	3708	3709	3714	rVB4	1769	912	0.04%	0.006%
86	13.038	3714	3716	3717	rBV2	1792	675	0.03%	0.004%
87	13.109	3736	3738	3741	rVB4	2745	1190	0.06%	0.008%
88	13.129	3742	3744	3747	rVB3	2252	1110	0.05%	0.007%
89	13.283	3787	3792	3793	rBV5	3115	2685	0.13%	0.017%
90	13.347	3808	3812	3813	rBV3	1547	904	0.04%	0.006%
91	13.492	3854	3857	3860	rVB5	1647	1163	0.06%	0.008%
92	13.511	3860	3863	3866	rBV4	2082	1419	0.07%	0.009%
93	13.566	3877	3880	3883	rBV4	1673	1236	0.06%	0.008%
94	13.637	3897	3902	3904	rBV6	1900	1846	0.09%	0.012%
95	13.746	3934	3936	3938	rBV3	1368	742	0.04%	0.005%
96	14.193	4071	4075	4076	rBV4	2010	1645	0.08%	0.011%
97	14.238	4085	4089	4091	rBV4	2501	1555	0.08%	0.010%
98	14.251	4091	4093	4096	rBV4	2006	1204	0.06%	0.008%
99	14.749	4244	4248	4251	rBV5	2756	2433	0.12%	0.016%
100	15.054	4341	4343	4345	rBV3	2507	1648	0.08%	0.011%


Sum of corrected areas: 15450878

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015208.D
Acq On : 27 Mar 2020 13:00
Operator : SY/MD
Sample : L2045-04
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

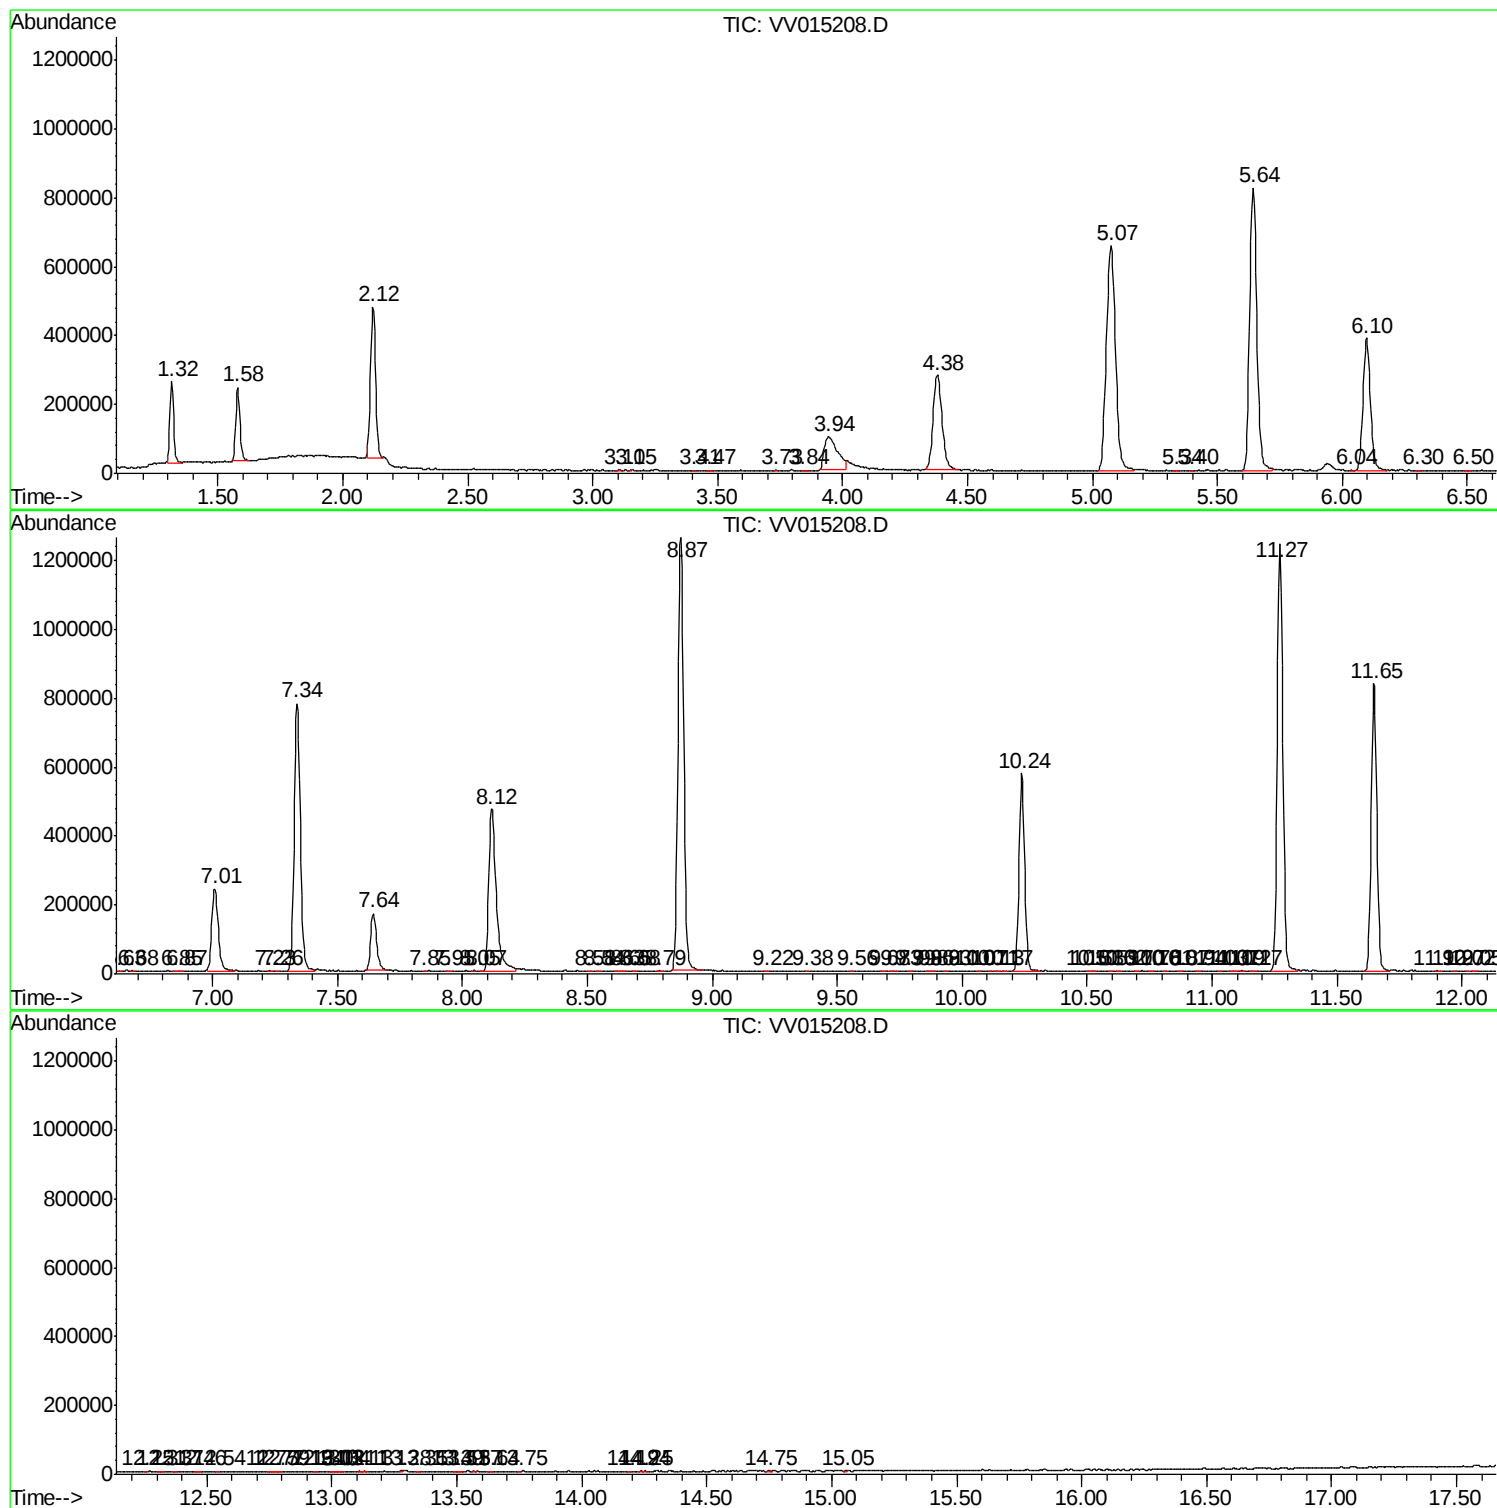

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032620\
Data File : VV015208.D
Acq On : 27 Mar 2020 13:00
Operator : SY/MD
Sample : L2045-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV032620\
Data File : VV015208.D
Acq On : 27 Mar 2020 13:00
Operator : SY/MD
Sample : L2045-04
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc