

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015209.D
 Acq On : 27 Mar 2020 13:24
 Operator : SY/MD
 Sample : L1941-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	65	70	81	rVB	244843	242426	12.08%	1.574%
2	1.579	146	152	163	rVB	208374	244546	12.19%	1.588%
3	2.119	314	320	344	rVB	462226	710255	35.40%	4.611%
4	2.746	513	515	517	rBV3	1750	901	0.04%	0.006%
5	2.936	572	574	576	rBV3	2181	1365	0.07%	0.009%
6	2.991	585	591	592	rBV5	2464	2316	0.12%	0.015%
7	3.071	613	616	619	rBV4	2436	1640	0.08%	0.011%
8	3.200	654	656	658	rBV3	2134	1177	0.06%	0.008%
9	3.376	709	711	716	rVB5	1991	1165	0.06%	0.008%
10	3.685	805	807	809	rBV2	1623	983	0.05%	0.006%
11	3.714	814	816	818	rVB3	2003	803	0.04%	0.005%
12	3.946	876	888	930	rBV2	92959	432991	21.58%	2.811%
13	4.380	1010	1023	1053	rVB2	271844	683299	34.06%	4.436%
14	4.833	1161	1164	1170	rVB7	1696	1496	0.07%	0.010%
15	4.865	1170	1174	1176	rBV4	1849	1225	0.06%	0.008%
16	4.884	1176	1180	1182	rVB4	1824	1374	0.07%	0.009%
17	4.958	1201	1203	1205	rBV3	2055	845	0.04%	0.005%
18	5.074	1222	1239	1262	rBV3	637377	1612834	80.38%	10.471%
19	5.508	1371	1374	1377	rVB5	3081	1846	0.09%	0.012%
20	5.531	1377	1381	1384	rBV5	1060	913	0.05%	0.006%
21	5.569	1391	1393	1396	rBV4	1366	829	0.04%	0.005%
22	5.640	1403	1415	1442	rBV	791406	1588165	79.15%	10.310%
23	5.868	1483	1486	1488	rBV3	2496	1442	0.07%	0.009%
24	5.939	1498	1508	1520	rBV9	16583	36383	1.81%	0.236%
25	6.097	1543	1557	1577	rBV	376698	770277	38.39%	5.001%
26	6.405	1649	1653	1655	rBV4	2676	2317	0.12%	0.015%
27	6.437	1661	1663	1665	rBV3	1654	842	0.04%	0.005%
28	6.682	1734	1739	1741	rBV5	1894	1571	0.08%	0.010%
29	6.720	1748	1751	1754	rBV5	2440	2179	0.11%	0.014%
30	6.839	1783	1788	1795	rVB10	1693	2375	0.12%	0.015%
31	6.875	1798	1799	1806	rBV7	1215	1179	0.06%	0.008%
32	7.010	1829	1841	1860	rBV	231840	421960	21.03%	2.739%
33	7.206	1900	1902	1905	rBV5	2916	1915	0.10%	0.012%
34	7.286	1924	1927	1928	rBV3	1677	1159	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015209.D
 Acq On : 27 Mar 2020 13:24
 Operator : SY/MD
 Sample : L1941-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

35	7.338	1932	1943	1960	rVV	739141	1274739	63.53%	8.276%
36	7.643	2028	2038	2058	rBV	162319	280698	13.99%	1.822%
37	7.904	2117	2119	2121	rBV3	1676	830	0.04%	0.005%
38	7.933	2125	2128	2132	rBV5	3203	3283	0.16%	0.021%
39	8.119	2175	2186	2217	rBV2	465207	965532	48.12%	6.268%
40	8.527	2310	2313	2314	rBV3	1566	1021	0.05%	0.007%
41	8.576	2323	2328	2329	rBV5	2032	1228	0.06%	0.008%
42	8.614	2337	2340	2344	rBV6	2495	1313	0.07%	0.009%
43	8.640	2344	2348	2354	rBV9	1500	1661	0.08%	0.011%
44	8.711	2366	2370	2371	rBV3	1499	1081	0.05%	0.007%
45	8.875	2406	2421	2440	rBV	1242395	2006452	100.00%	13.026%
46	9.238	2532	2534	2536	rBV3	1346	771	0.04%	0.005%
47	9.396	2577	2583	2586	rVB7	2033	1829	0.09%	0.012%
48	9.415	2586	2589	2590	rBV2	2111	1040	0.05%	0.007%
49	9.489	2609	2612	2615	rBV5	1363	789	0.04%	0.005%
50	9.502	2615	2616	2623	rVB6	1944	1616	0.08%	0.010%
51	9.534	2623	2626	2627	rBV3	1294	898	0.04%	0.006%
52	9.595	2642	2645	2648	rVB4	1633	1038	0.05%	0.007%
53	9.691	2673	2675	2679	rBV4	1327	715	0.04%	0.005%
54	9.849	2720	2724	2726	rBV5	1687	1510	0.08%	0.010%
55	9.887	2732	2736	2742	rVB8	2043	2285	0.11%	0.015%
56	10.170	2822	2824	2826	rBV3	1604	717	0.04%	0.005%
57	10.238	2833	2845	2866	rBV	568131	890423	44.38%	5.781%
58	10.460	2911	2914	2915	rBV3	1616	836	0.04%	0.005%
59	10.550	2939	2942	2943	rBV3	1408	716	0.04%	0.005%
60	10.637	2965	2969	2974	rVB7	2086	1767	0.09%	0.011%
61	10.688	2983	2985	2993	rBV8	2137	3388	0.17%	0.022%
62	10.762	3004	3008	3009	rBV4	1897	1253	0.06%	0.008%
63	10.932	3057	3061	3064	rBV6	1251	887	0.04%	0.006%
64	10.945	3064	3065	3067	rBV2	1604	761	0.04%	0.005%
65	10.977	3073	3075	3078	rBV3	1291	750	0.04%	0.005%
66	11.010	3082	3085	3091	rVB8	2828	2235	0.11%	0.015%
67	11.087	3107	3109	3113	rBV4	1635	1254	0.06%	0.008%
68	11.273	3153	3167	3191	rBV	1195243	1853121	92.36%	12.030%
69	11.575	3259	3261	3265	rVV4	2235	1365	0.07%	0.009%
70	11.649	3271	3284	3300	rBV	817270	1268929	63.24%	8.238%
71	11.907	3361	3364	3367	rBV5	2545	1446	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV032620\
 Data File : VV015209.D
 Acq On : 27 Mar 2020 13:24
 Operator : SY/MD
 Sample : L1941-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
 Title : VOC Analysis

72	11.936	3370	3373	3375	rBV4	1993	1108	0.06%	0.007%
73	11.945	3375	3376	3380	rVB4	1471	799	0.04%	0.005%
74	11.984	3387	3388	3393	rVB4	2185	1512	0.08%	0.010%
75	12.019	3393	3399	3403	rBV8	2932	3339	0.17%	0.022%
76	12.038	3403	3405	3408	rVB4	1587	900	0.04%	0.006%
77	12.064	3410	3413	3415	rBV4	1451	833	0.04%	0.005%
78	12.132	3431	3434	3437	rBV5	1422	1037	0.05%	0.007%
79	12.276	3476	3479	3482	rBV4	1877	1451	0.07%	0.009%
80	12.399	3512	3517	3519	rBV6	2376	2355	0.12%	0.015%
81	12.444	3529	3531	3535	rVB4	1334	910	0.05%	0.006%
82	12.466	3535	3538	3542	rVB6	1690	937	0.05%	0.006%
83	12.495	3545	3547	3548	rBV	1473	750	0.04%	0.005%
84	12.627	3585	3588	3592	rBV5	1918	1519	0.08%	0.010%
85	12.710	3611	3614	3618	rBV6	2007	1620	0.08%	0.011%
86	12.743	3622	3624	3631	rVB8	1773	1475	0.07%	0.010%
87	12.772	3631	3633	3636	rVB4	2246	1198	0.06%	0.008%
88	12.791	3636	3639	3641	rBV3	1714	1052	0.05%	0.007%
89	12.846	3652	3656	3659	rBV5	1485	1158	0.06%	0.008%
90	12.884	3664	3668	3673	rBV8	1723	1936	0.10%	0.013%
91	12.932	3681	3683	3684	rBV2	2198	1023	0.05%	0.007%
92	13.418	3832	3834	3837	rBV3	2018	1227	0.06%	0.008%
93	13.444	3840	3842	3844	rVB4	2030	822	0.04%	0.005%
94	13.463	3844	3848	3852	rBV7	2602	2507	0.12%	0.016%
95	13.675	3912	3914	3919	rBV5	1708	1747	0.09%	0.011%
96	13.887	3977	3980	3983	rBV5	2454	2274	0.11%	0.015%
97	13.942	3993	3997	4000	rBV6	1824	2070	0.10%	0.013%
98	14.238	4084	4089	4097	rVB6	3548	4577	0.23%	0.030%
99	14.276	4097	4101	4105	rBV6	3587	3523	0.18%	0.023%
100	14.296	4105	4107	4109	rBV3	1525	754	0.04%	0.005%


Sum of corrected areas: 15403583

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV032620\
Data File : VV015209.D
Acq On : 27 Mar 2020 13:24
Operator : SY/MD
Sample : L1941-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

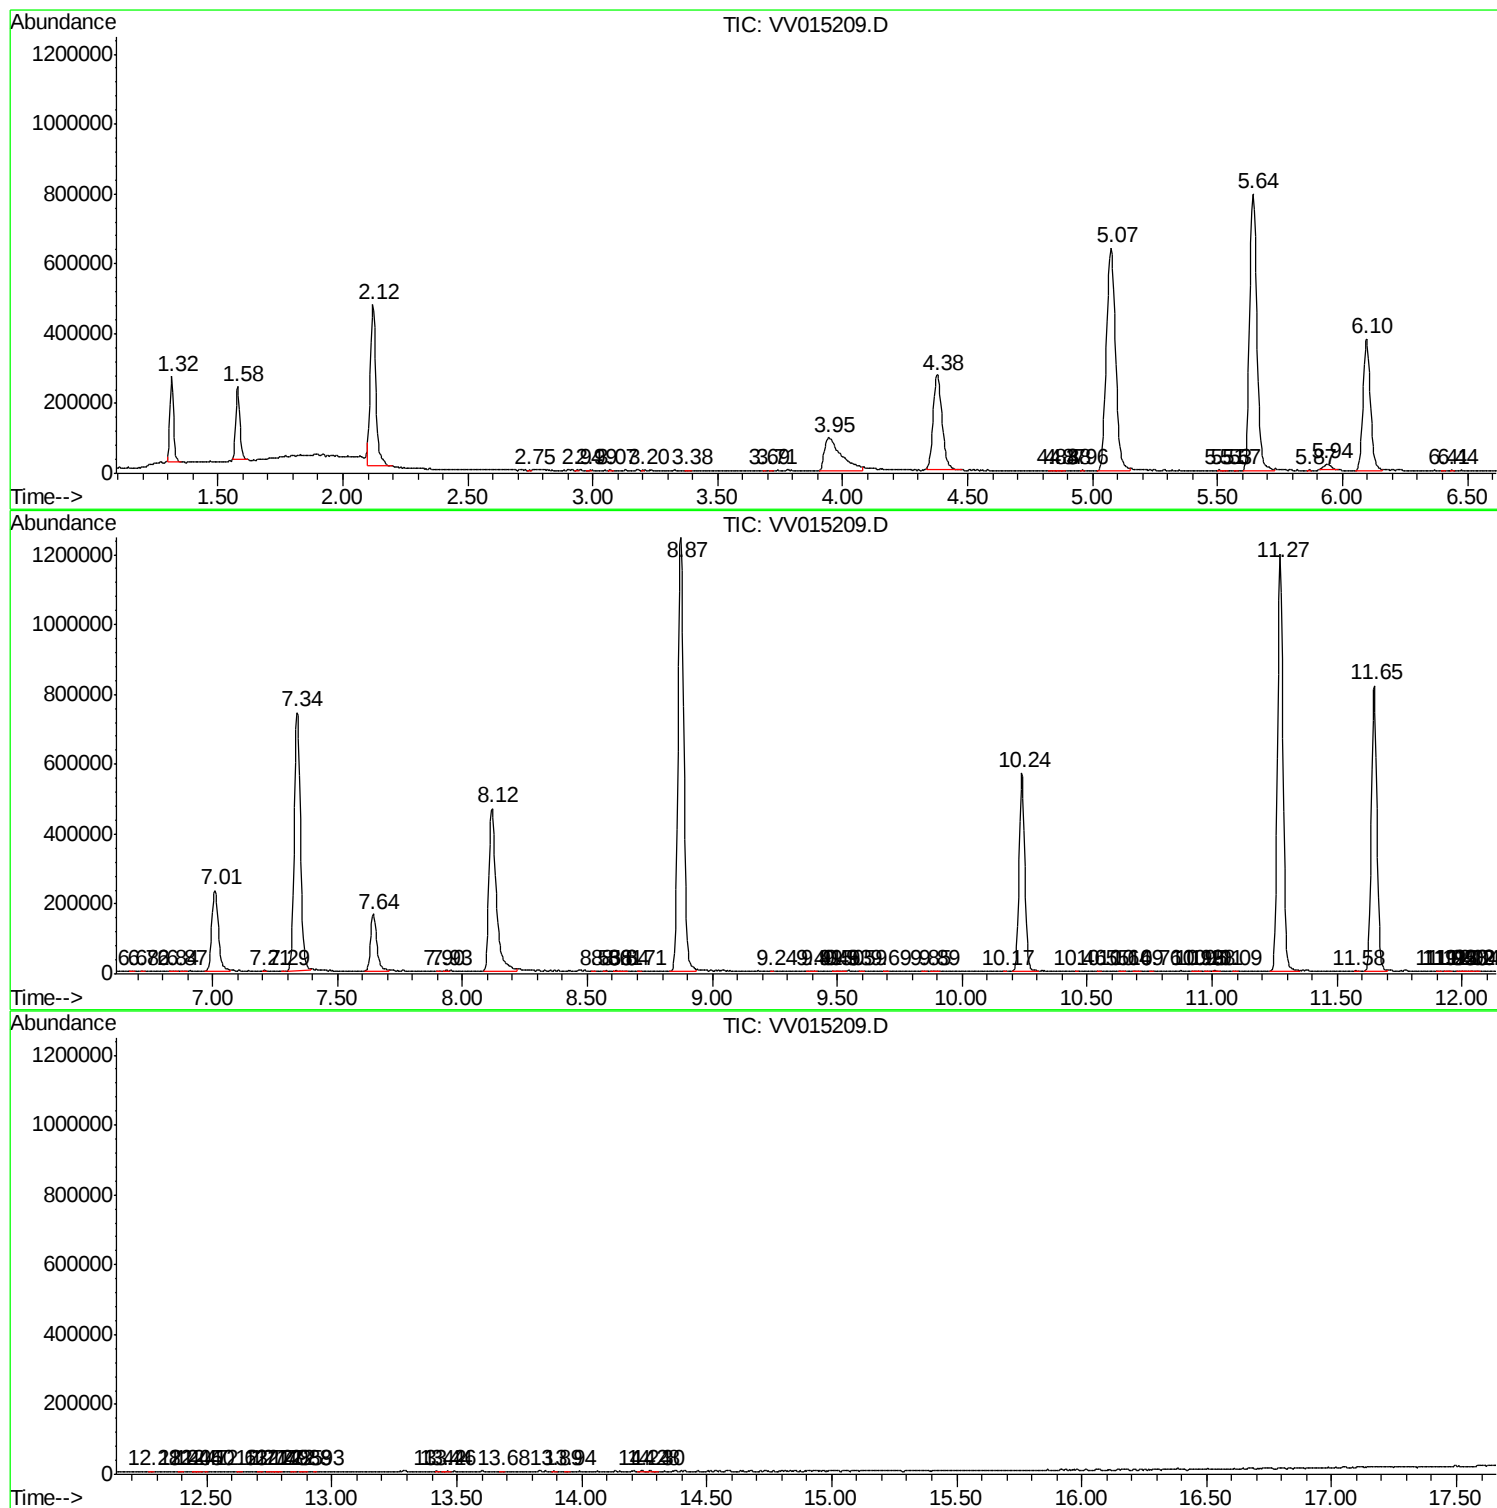

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV032620\
Data File : VV015209.D
Acq On : 27 Mar 2020 13:24
Operator : SY/MD
Sample : L1941-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV032620\
Data File : VV015209.D
Acq On : 27 Mar 2020 13:24
Operator : SY/MD
Sample : L1941-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM032620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc