


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV032620\
 Data File : VV015164.D
 Acq On : 26 Mar 2020 08:48
 Operator : SY/MD
 Sample : BFB73
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB73

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM0326620WMA.M
 Title : VOC Analysis
 Last Update : Wed Jan 29 12:34:48 2020

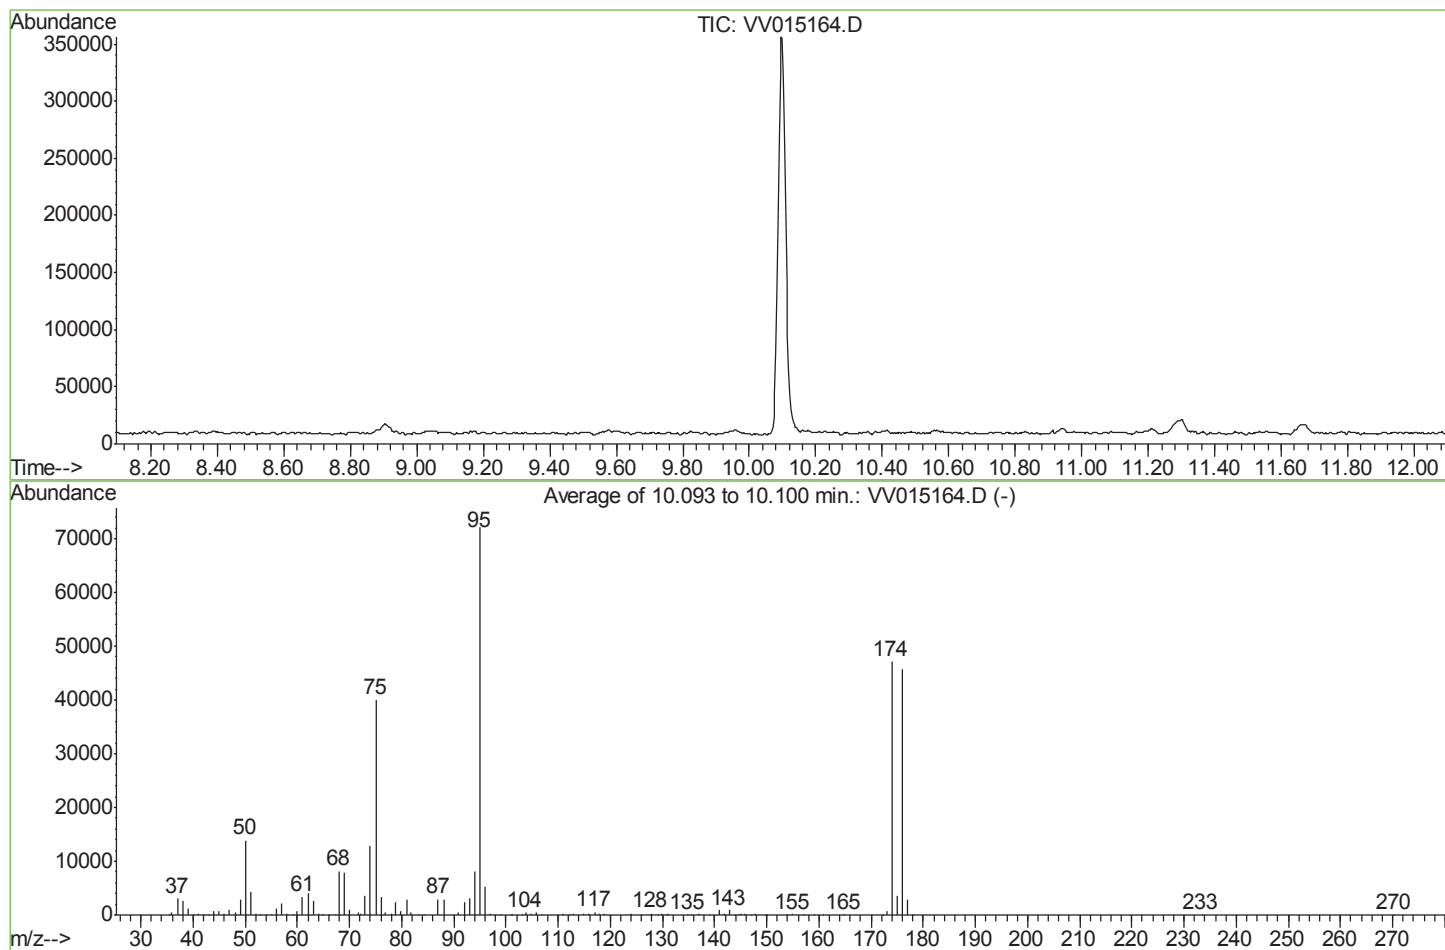

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.2	13855	PASS
75	95	30	80	55.6	40080	PASS
95	95	100	100	100.0	72081	PASS
96	95	5	9	7.3	5287	PASS
173	174	0.00	2	1.5	730	PASS
174	95	50	120	65.4	47106	PASS
175	174	5	9	7.8	3693	PASS
176	174	95	101	97.0	45712	PASS
177	176	5	9	6.4	2940	PASS

m/z	Abundance
35.90	681.0
37.00	3361.0
38.00	2922.0
38.90	1679.0
39.90	981.0
40.90	410.0
42.00	331.0
43.10	409.0
44.00	1655.0
45.00	870.0
45.90	244.0
47.00	1027.0
48.00	532.0
49.00	2864.0
50.00	13434.0
51.00	4020.0
51.90	256.0
52.70	151.0
53.20	123.0
54.00	200.0
54.90	536.0
56.00	1158.0
57.00	2522.0
58.00	184.0
59.90	714.0
61.00	3009.0
62.00	3846.0
63.00	2705.0
63.90	441.0
64.70	125.0
66.80	211.0
68.00	7748.0
69.00	7541.0
69.90	880.0
70.90	187.0
71.80	400.0
72.20	443.0
73.00	3521.0
74.00	12377.0
75.00	37168.0
76.00	3156.0
76.90	585.0
78.00	410.0
78.90	2436.0
79.90	711.0
80.90	2782.0
81.90	648.0
82.90	168.0
87.00	2645.0
88.00	3049.0
90.90	523.0
92.00	2309.0
93.00	2994.0
94.00	7874.0
95.00	67968.0
96.00	5177.0
97.10	288.0
101.10	107.0
103.70	361.0
104.70	198.0
105.80	367.0
106.70	118.0
111.00	203.0
112.80	175.0
114.80	119.0
115.90	298.0
116.90	561.0
117.80	191.0
118.90	308.0
123.80	117.0
127.90	304.0
129.80	218.0
130.70	126.0
131.00	137.0
134.80	133.0
135.40	102.0
137.00	200.0
138.90	124.0
140.80	793.0
141.70	180.0
142.80	874.0
144.60	104.0
145.10	141.0
145.90	130.0
147.80	226.0
150.00	122.0
155.00	138.0
164.80	118.0
173.00	701.0
174.00	42912.0
175.00	3233.0
175.90	42520.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73

176.90

2619.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73

m/z	Abundance
35.30	125.0
35.90	748.0
37.00	3371.0
38.00	3059.0
38.90	1746.0
39.90	922.0
41.00	463.0
42.00	310.0
43.10	382.0
44.00	1737.0
45.10	977.0
45.90	286.0
47.00	984.0
48.00	541.0
49.00	2981.0
50.00	14451.0
51.00	4285.0
52.00	266.0
53.10	170.0
54.00	255.0
54.90	523.0
56.00	1365.0
57.00	2476.0
57.90	186.0
59.90	708.0
61.00	3509.0
62.00	4230.0
63.00	2933.0
64.00	341.0
64.70	135.0
66.10	122.0
67.20	215.0
68.00	8450.0
69.00	8427.0
70.00	848.0
70.90	207.0
71.80	468.0
73.00	3680.0
74.00	13308.0
75.00	41640.0
76.00	3456.0
76.90	600.0
78.00	427.0
78.90	2661.0
79.90	837.0
80.90	2974.0
81.90	595.0
83.20	155.0
84.10	156.0
85.10	134.0
87.00	2978.0
88.00	2936.0
90.90	524.0
92.00	2516.0
93.00	3128.0
94.00	8359.0
95.00	74344.0
96.00	5407.0
97.10	278.0
99.00	136.0
100.80	150.0
103.80	397.0
104.80	212.0
105.80	416.0
106.70	123.0
111.00	192.0
112.10	114.0
112.80	213.0
114.80	201.0
115.90	382.0
117.00	545.0
117.80	213.0
118.80	329.0
123.80	171.0
127.90	294.0
129.00	118.0
129.80	239.0
131.00	160.0
134.80	115.0
136.90	202.0
139.00	133.0
140.80	936.0
141.70	181.0
142.90	927.0
144.90	179.0
145.90	167.0
147.80	236.0
149.70	120.0
153.90	106.0
155.00	180.0
157.00	103.0
159.10	122.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73

172.90	747.0
174.00	48752.0
175.00	3838.0
175.90	46968.0
176.90	2976.0
177.80	118.0
233.30	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73

m/z	Abundance
35.90	714.0
37.00	2996.0
38.00	2920.0
39.00	1691.0
39.90	784.0
41.00	489.0
41.90	295.0
42.90	408.0
44.00	1754.0
45.10	963.0
45.90	290.0
47.00	836.0
48.00	461.0
49.00	2813.0
50.00	13681.0
51.00	4275.0
52.00	324.0
53.10	240.0
54.00	215.0
55.00	541.0
56.00	1445.0
57.00	2369.0
57.80	184.0
59.20	134.0
59.90	695.0
61.00	3505.0
62.00	4073.0
63.00	2714.0
64.00	266.0
66.10	147.0
66.90	281.0
68.00	8615.0
69.00	8442.0
70.00	809.0
70.90	266.0
71.80	397.0
73.00	3456.0
74.00	12944.0
75.00	41432.0
76.00	3408.0
77.00	580.0
78.00	329.0
78.90	2761.0
79.90	845.0
80.90	2814.0
81.90	544.0
83.20	210.0
84.10	223.0
85.10	166.0
87.00	3108.0
88.00	2546.0
90.90	415.0
92.00	2314.0
93.00	3080.0
94.00	8135.0
95.00	74320.0
96.00	5279.0
96.90	269.0
98.00	109.0
99.00	127.0
100.80	160.0
103.00	103.0
103.80	444.0
104.90	217.0
105.80	344.0
106.80	129.0
110.90	139.0
112.10	156.0
112.80	204.0
114.80	225.0
115.90	385.0
117.10	469.0
117.80	222.0
118.80	339.0
123.90	207.0
126.00	124.0
127.80	225.0
129.00	136.0
129.80	216.0
131.00	137.0
136.80	141.0
140.80	972.0
141.80	155.0
142.90	949.0
143.90	112.0
144.90	206.0
145.90	120.0
147.10	116.0
147.70	255.0
149.60	156.0
153.90	126.0
154.90	176.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73

157.00	146.0
159.10	122.0
160.70	101.0
172.30	250.0
172.90	743.0
173.90	49656.0
174.90	4010.0
175.90	47648.0
176.90	3225.0
177.90	132.0
270.30	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73

m/z	Abundance
35.80	237.0
36.40	104.0
37.20	168.0
38.10	238.0
39.10	415.0
39.90	882.0
41.00	259.0
41.90	256.0
43.00	377.0
43.90	935.0
44.90	175.0
45.60	136.0
48.20	124.0
53.20	199.0
54.20	173.0
55.10	408.0
55.80	142.0
57.10	249.0
60.20	143.0
63.00	104.0
64.00	123.0
67.00	166.0
68.00	127.0
68.80	281.0
71.10	303.0
77.90	163.0
79.00	150.0
80.20	136.0
81.10	102.0
81.80	117.0
82.90	251.0
85.00	212.0
95.10	129.0
102.30	132.0
105.10	134.0
107.20	132.0
118.90	129.0
125.10	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73