

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020746.D
 Acq On : 26 Mar 2021 11:03
 Operator : SY/MD
 Sample : VV0326MBL01
 Misc : 5.0g/5mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK79

Quant Time: Mar 27 06:51:29 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 27 06:50:46 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	688805	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	671529	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	329069	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	222300	45.46	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	90.92%		
7) Chloroethane-d5	1.568	69	176130	47.64	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	95.28%		
11) 1,1-Dichloroethene-d2	2.108	63	342997	37.18	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	74.36%		
21) 2-Butanone-d5	3.886	46	289842	91.10	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	91.10%		
24) Chloroform-d	4.349	84	472761	48.64	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.28%		
26) 1,2-Dichloroethane-d4	5.031	65	321194	50.16	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.32%		
32) Benzene-d6	5.050	84	897555	50.14	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.28%		
36) 1,2-Dichloropropane-d6	6.072	67	272261	49.54	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	99.08%		
41) Toluene-d8	7.317	98	813202	48.81	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	97.62%		
43) trans-1,3-Dichloroprop...	7.622	79	137752	47.11	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	94.22%		
47) 2-Hexanone-d5	8.092	63	212155	92.08	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	92.08%		
57) 1,1,2,2-Tetrachloroeth...	10.220	84	370094	46.23	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	92.46%		
64) 1,2-Dichlorobenzene-d4	11.632	152	336762	52.73	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	105.46%		
Target Compounds						
10) 1,1,2-Trichloro-1,2,2-...	2.108	101	3504	0.81	ug/L #	27
48) 2-Hexanone	8.088	43	23945	4.82	ug/L #	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020746.D
Acq On : 26 Mar 2021 11:03
Operator : SY/MD
Sample : VV0326MBL01
Misc : 5.0g/5mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK79

Quant Time: Mar 27 06:51:29 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 27 06:50:46 2021
Response via : Initial Calibration




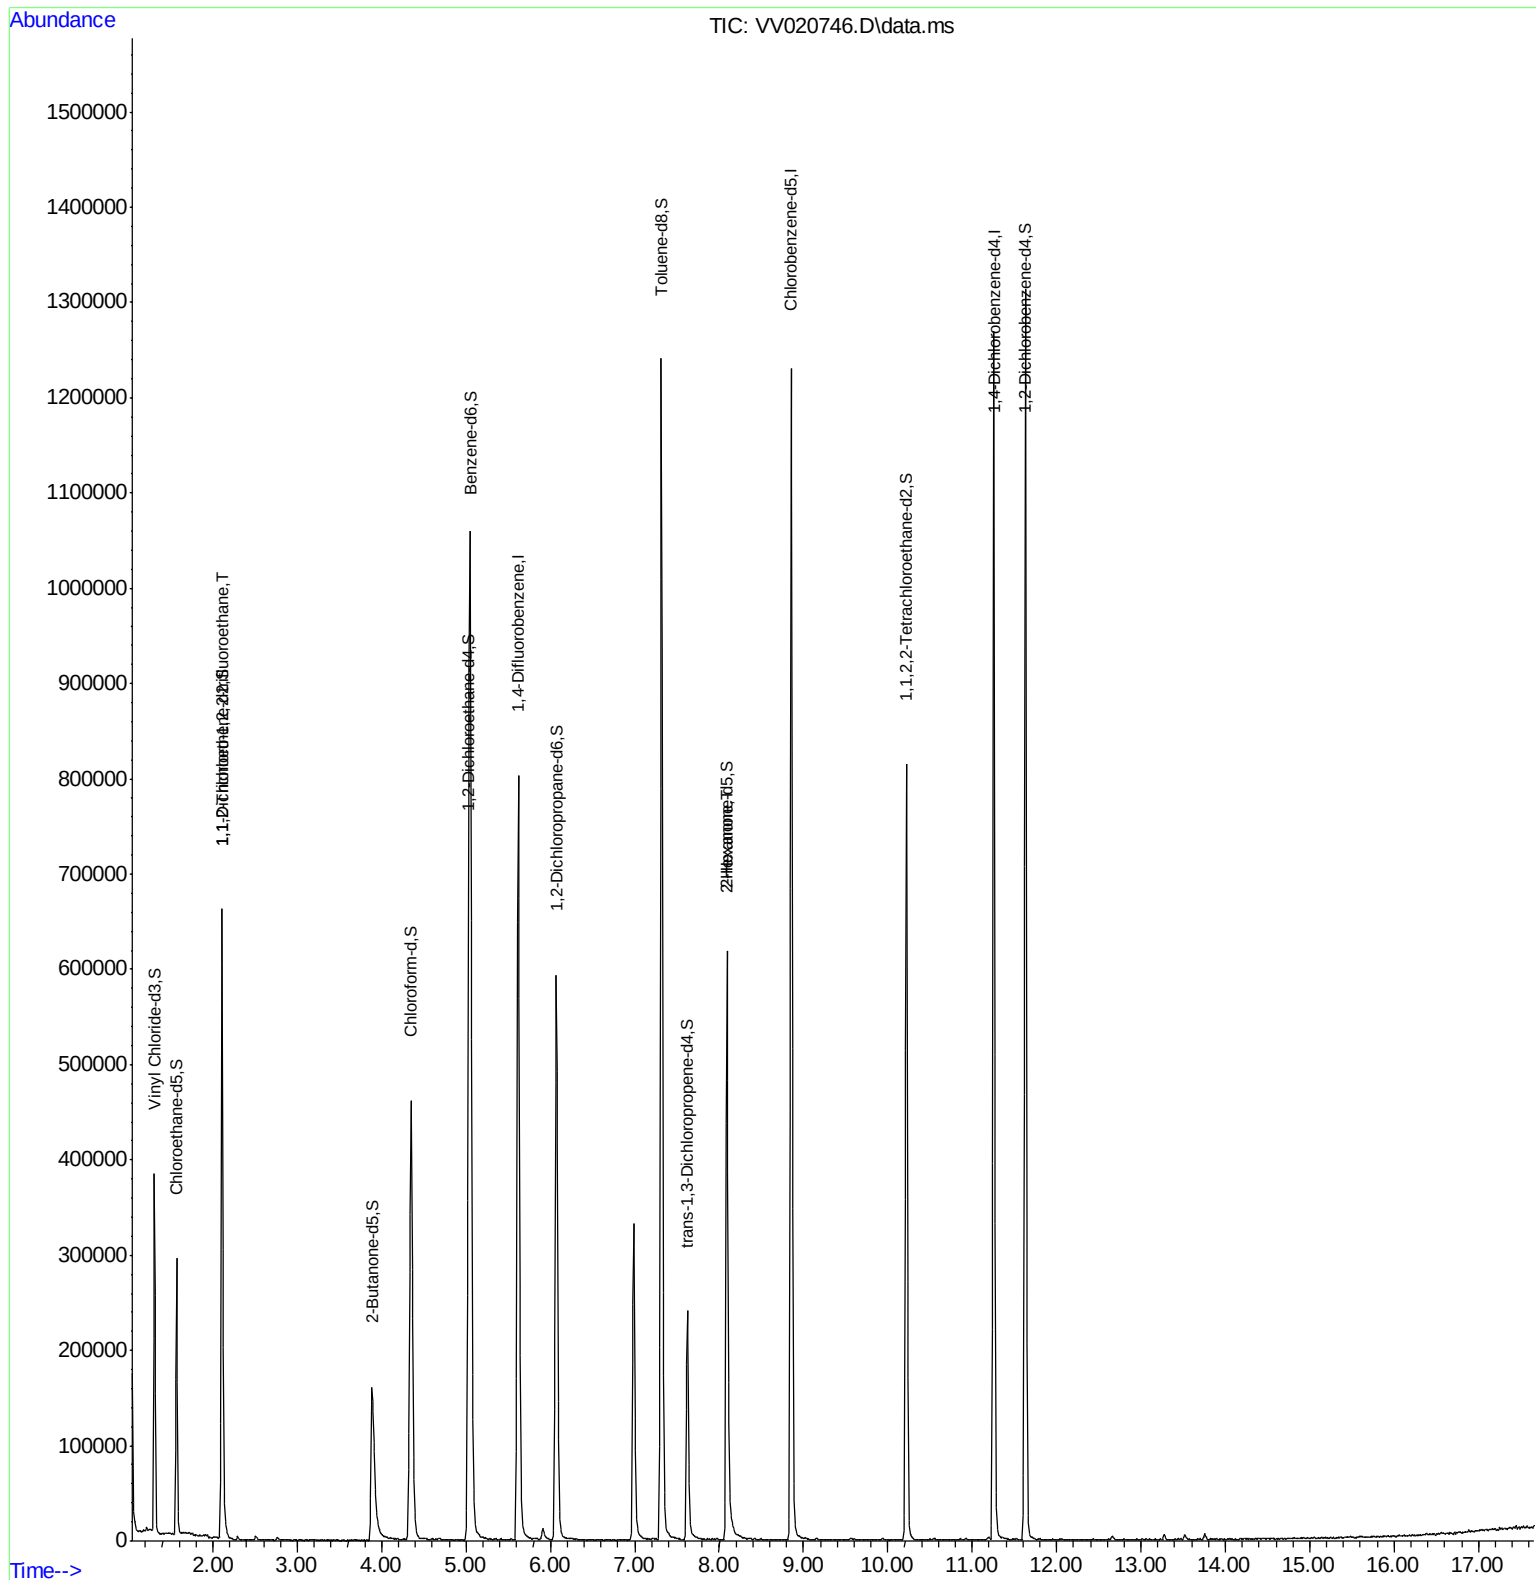


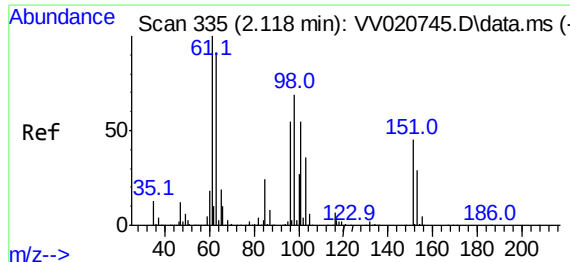

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.81 ug/L
 RT: 2.108 min Scan# 332
 Delta R.T. -0.010 min
 Lab File: VV020746.D
 Acq: 26 Mar 2021 11:03

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK79

Tgt Ion:101 Resp: 3504
 Ion Ratio Lower Upper
 101 100
 85 4.5 35.4 53.0#
 151 9.7 63.5 95.3#

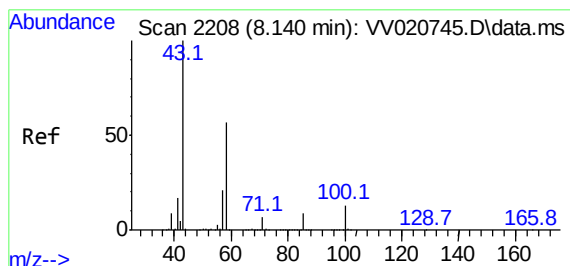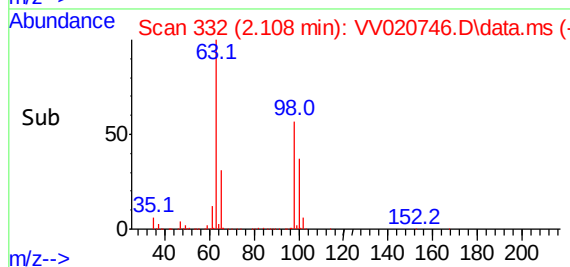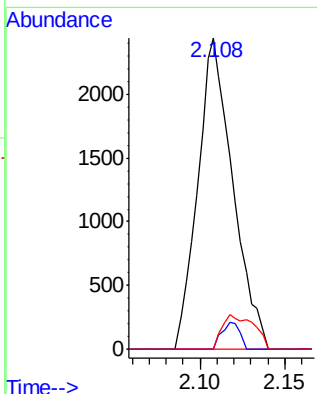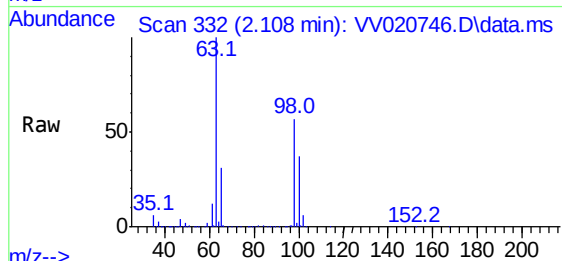

#48
 2-Hexanone
 Concen: 4.82 ug/L
 RT: 8.088 min Scan# 2192
 Delta R.T. -0.051 min
 Lab File: VV020746.D
 Acq: 26 Mar 2021 11:03

Tgt Ion: 43 Resp: 23945
 Ion Ratio Lower Upper
 43 100
 58 20.6 45.8 68.8#
 57 30.1 15.4 23.2#
 100 2.4 10.2 15.4#

