

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020747.D
 Acq On : 26 Mar 2021 11:26
 Operator : SY/MD
 Sample : VV0326WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK80

Quant Time: Mar 27 06:51:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 27 06:50:46 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	671092	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	662072	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	314146	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	213444	44.80	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	89.60%		
7) Chloroethane-d5	1.571	69	173177	48.08	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	96.16%		
11) 1,1-Dichloroethene-d2	2.111	63	334232	37.18	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	74.36%		
21) 2-Butanone-d5	3.892	46	304906	98.37	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	98.37%		
24) Chloroform-d	4.352	84	474070	50.06	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.12%		
26) 1,2-Dichloroethane-d4	5.037	65	319470	51.21	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	102.42%		
32) Benzene-d6	5.053	84	884419	50.12	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.24%		
36) 1,2-Dichloropropane-d6	6.072	67	269743	49.79	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	99.58%		
41) Toluene-d8	7.320	98	791573	48.19	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.38%		
43) trans-1,3-Dichloroprop...	7.625	79	139061	48.24	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	96.48%		
47) 2-Hexanone-d5	8.091	63	229345	100.96	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	100.96%		
57) 1,1,2,2-Tetrachloroeth...	10.220	84	378153	47.92	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	95.84%		
64) 1,2-Dichlorobenzene-d4	11.632	152	334079	54.79	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	109.58%		
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.108	101	3456	0.82	ug/L	# 28


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020747.D
Acq On : 26 Mar 2021 11:26
Operator : SY/MD
Sample : VV0326WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK80


Quant Time: Mar 27 06:51:43 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 27 06:50:46 2021
Response via : Initial Calibration

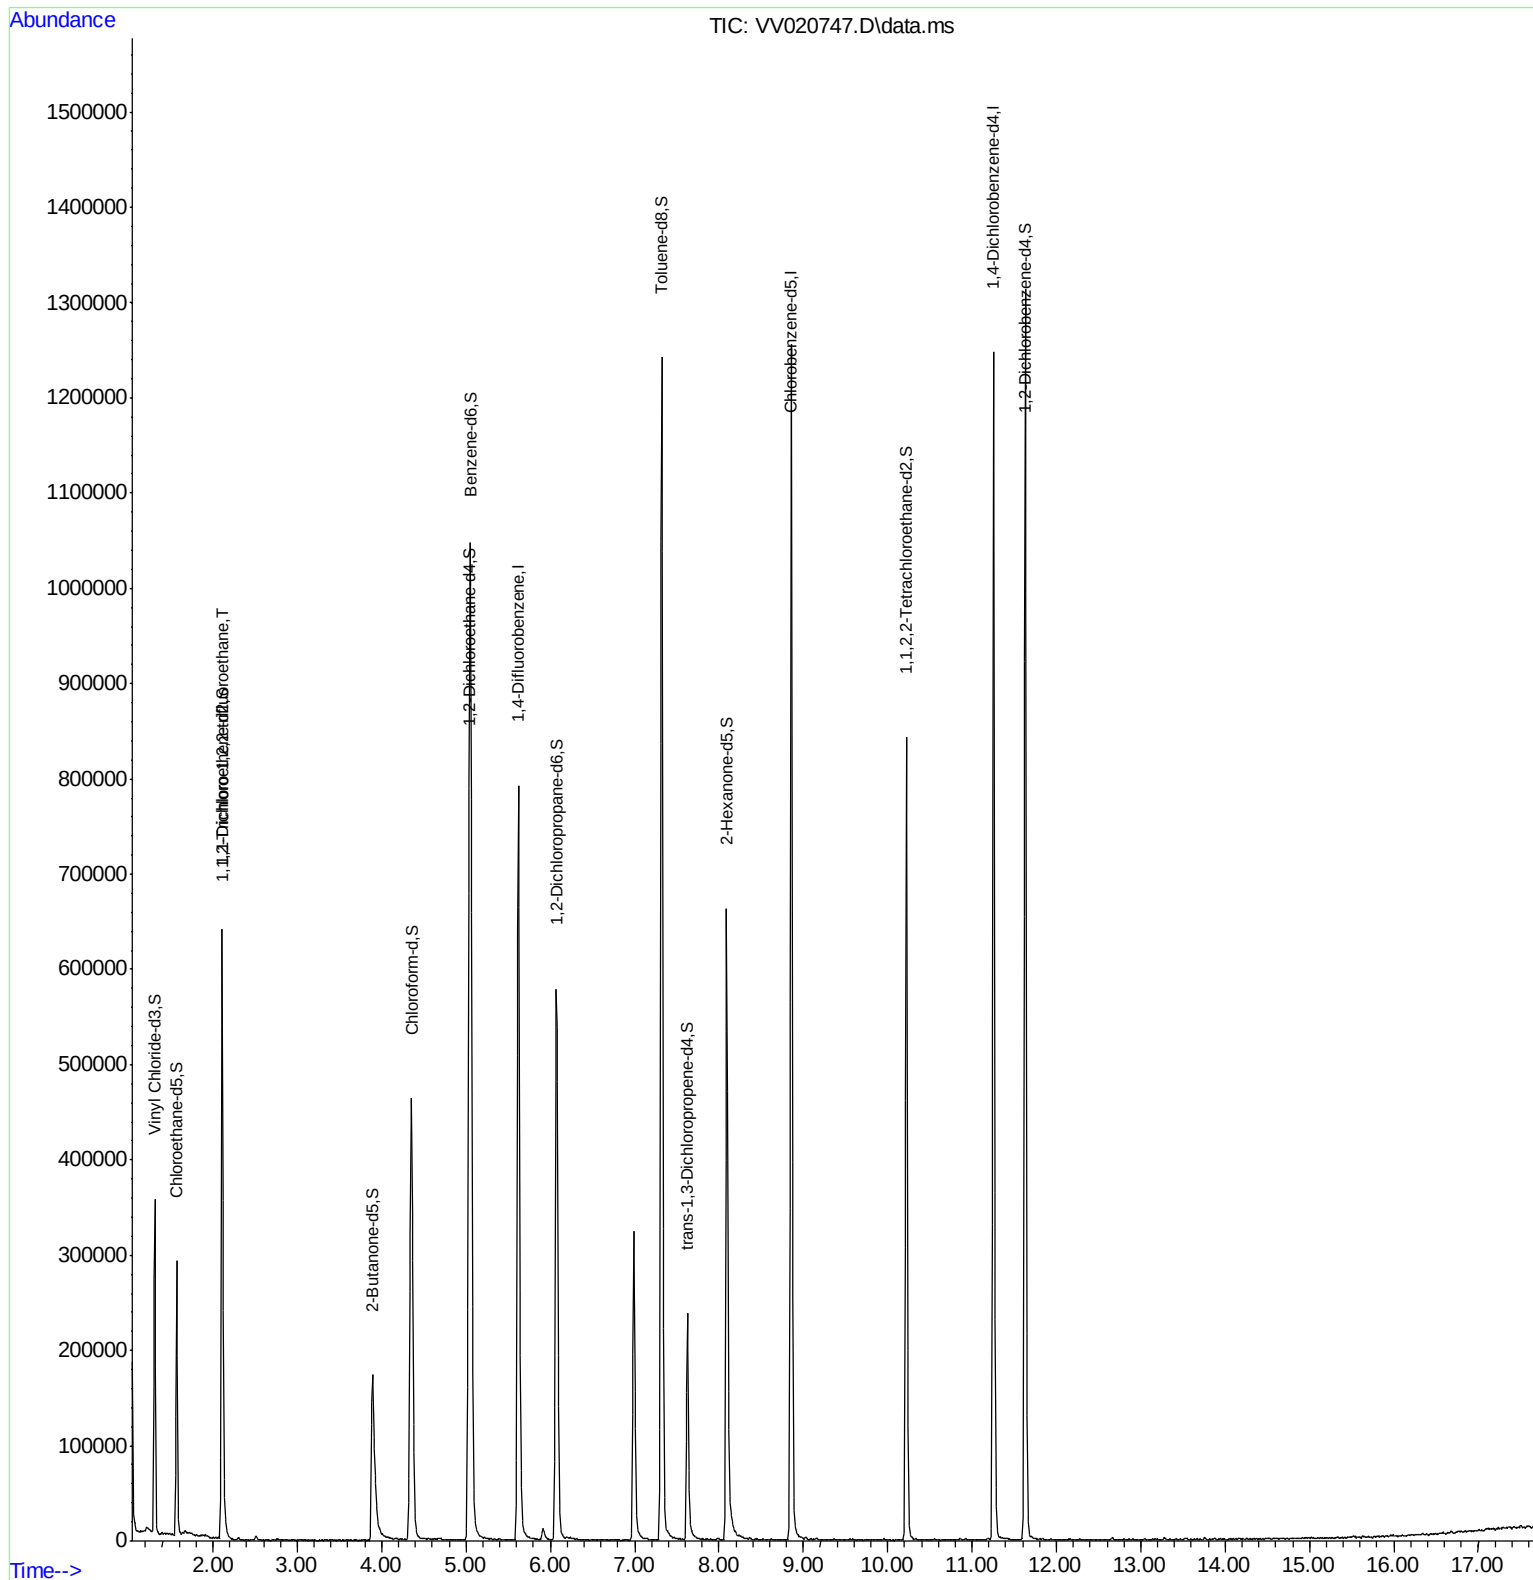

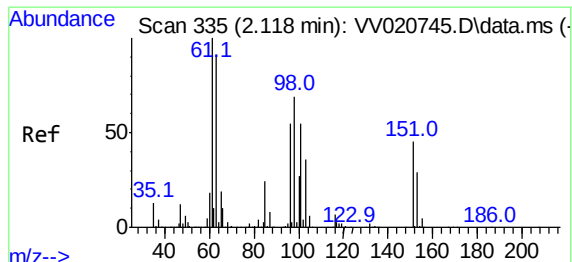

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.82 ug/L
 RT: 2.108 min Scan# 332
 Delta R.T. -0.010 min
 Lab File: VV020747.D
 Acq: 26 Mar 2021 11:26

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK80

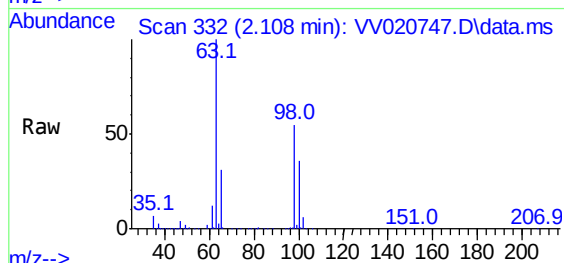

Tgt Ion:101 Resp: 3456
 Ion Ratio Lower Upper
 101 100
 85 4.0 35.4 53.0#
 151 11.3 63.5 95.3#

