

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032621\
 Data File : VW020751.D
 Acq On : 26 Mar 2021 13:00
 Operator : SY/MD
 Sample : M1816-05 10X
 Misc : 5.54g/5mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3L3

Quant Time: Mar 27 06:52:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 27 06:50:46 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	672408	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	654901	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.256	152	320228	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	170531	35.72	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	71.44%		
7) Chloroethane-d5	1.571	69	147672	40.92	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	81.84%		
11) 1,1-Dichloroethene-d2	2.108	63	279443	31.03	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	62.06%		
21) 2-Butanone-d5	3.892	46	301266	97.00	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	97.00%		
24) Chloroform-d	4.352	84	437715	46.13	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.26%		
26) 1,2-Dichloroethane-d4	5.037	65	302165	48.34	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.68%		
32) Benzene-d6	5.053	84	788852	45.19	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.38%		
36) 1,2-Dichloropropane-d6	6.072	67	255257	47.63	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	95.26%		
41) Toluene-d8	7.320	98	703280	43.28	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	86.56%		
43) trans-1,3-Dichloroprop...	7.625	79	127467	44.70	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	89.40%		
47) 2-Hexanone-d5	8.092	63	228792	101.82	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	101.82%		
57) 1,1,2,2-Tetrachloroeth...	10.220	84	365965	46.88	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	93.76%		
64) 1,2-Dichlorobenzene-d4	11.632	152	320515	51.57	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	103.14%		
Target Compounds						Qvalue
59) 1,2,3-Trichloropropane	11.252	75	34798	5.63	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020751.D
Acq On : 26 Mar 2021 13:00
Operator : SY/MD
Sample : M1816-05 10X
Misc : 5.54g/5mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3L3

Quant Time: Mar 27 06:52:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 27 06:50:46 2021
Response via : Initial Calibration

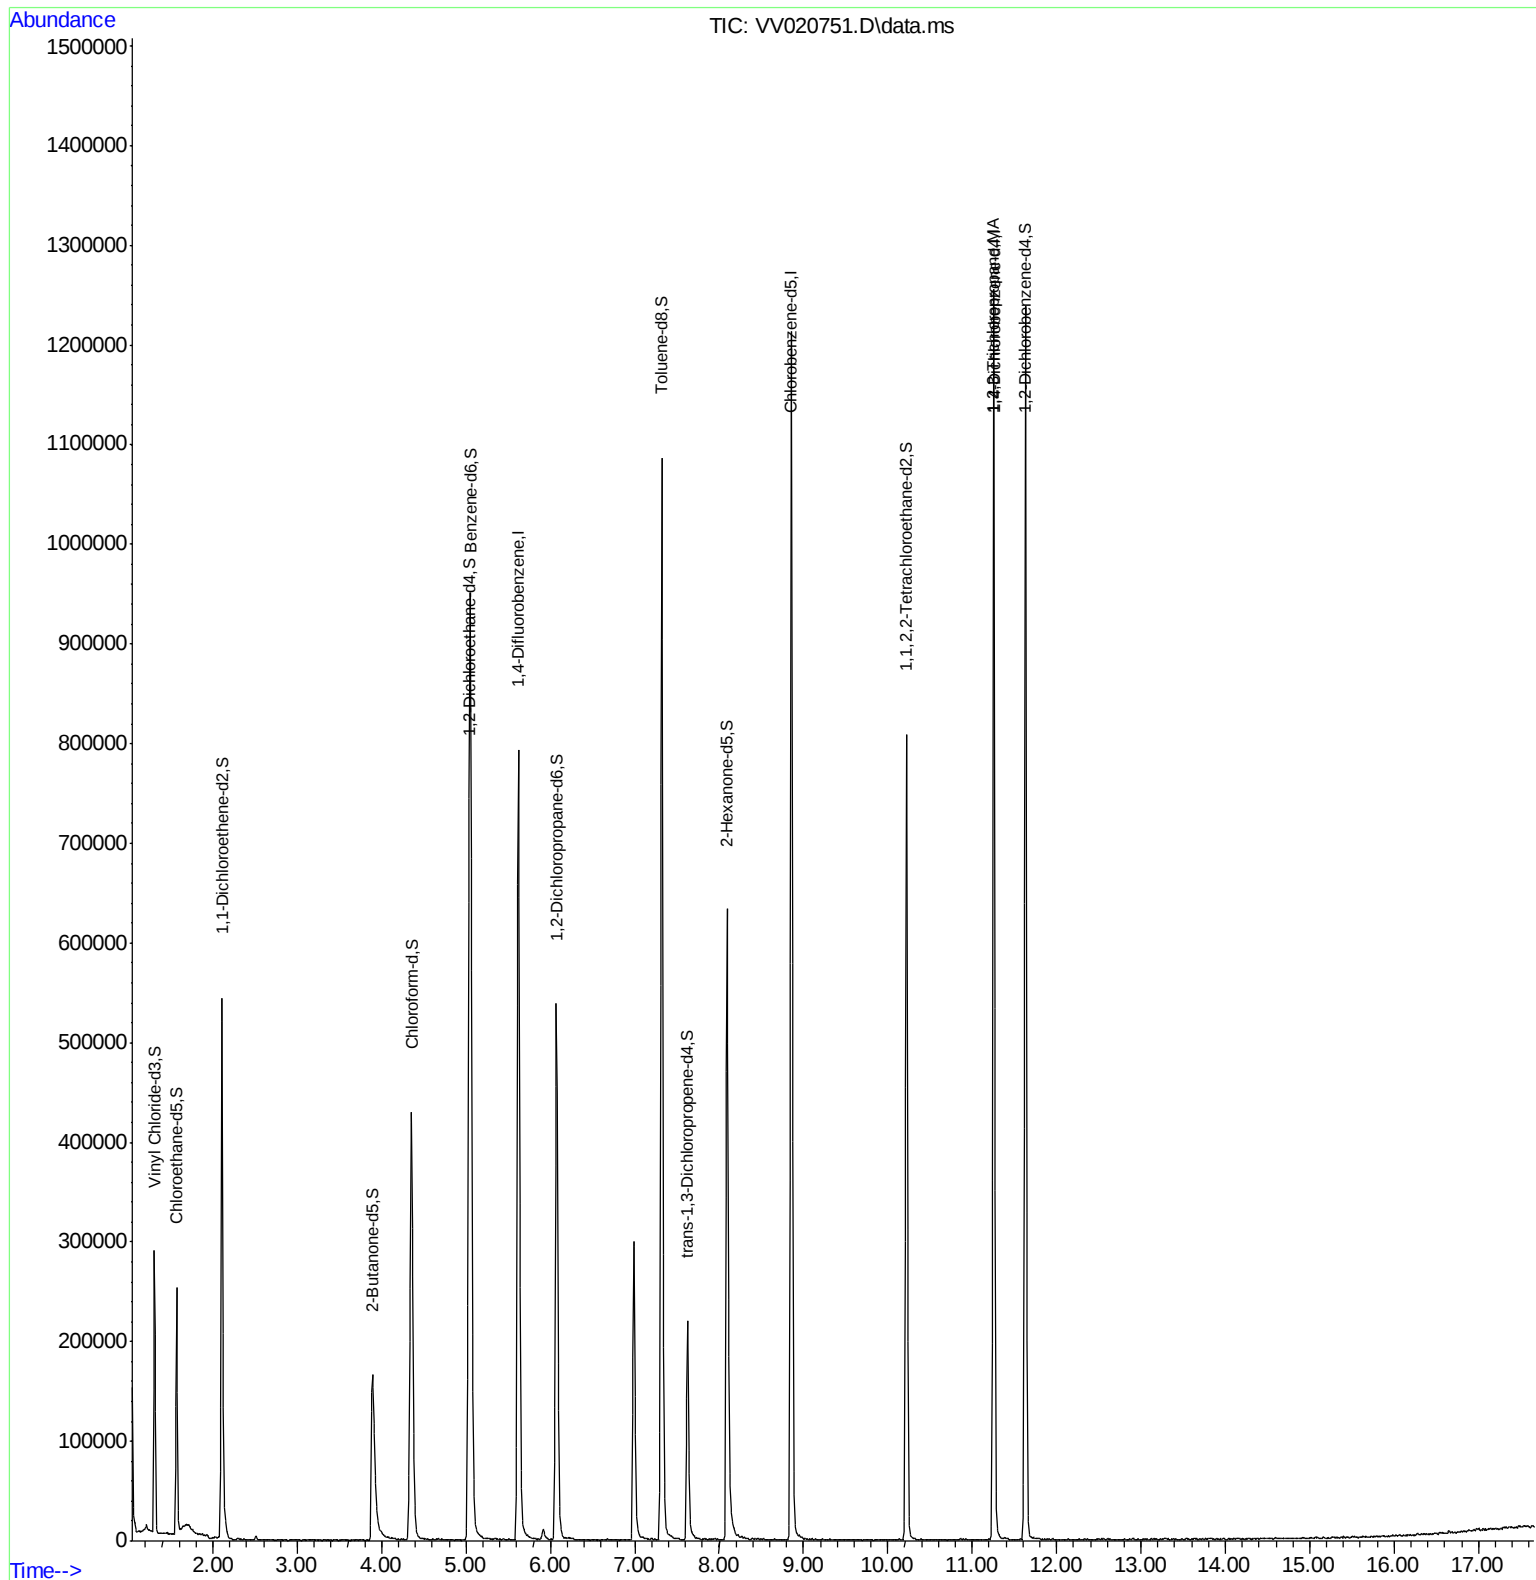

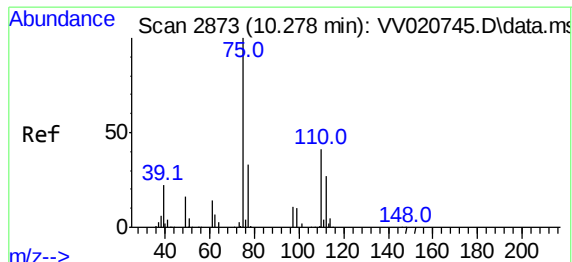

#59
 1,2,3-Trichloropropane
 Concen: 5.63 ug/L
 RT: 11.252 min Scan# 3176
 Delta R.T. 0.974 min
 Lab File: VV020751.D
 Acq: 26 Mar 2021 13:00

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3L3

Tgt Ion: 75 Resp: 34798
 Ion Ratio Lower Upper
 75 100
 77 36.9 25.3 37.9

