

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032621\
 Data File : VW020756.D
 Acq On : 26 Mar 2021 14:58
 Operator : SY/MD
 Sample : M1781-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Quant Time: Mar 27 06:53:21 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 27 06:50:46 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	716127	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	701891	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.256	152	341043	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	207913	40.89	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	81.78%		
7) Chloroethane-d5	1.571	69	171087	44.51	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	89.02%		
11) 1,1-Dichloroethene-d2	2.111	63	332820	34.70	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	69.40%		
21) 2-Butanone-d5	3.889	46	304300	92.00	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	92.00%		
24) Chloroform-d	4.352	84	470803	46.59	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.18%		
26) 1,2-Dichloroethane-d4	5.037	65	322367	48.43	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.86%		
32) Benzene-d6	5.053	84	875691	46.81	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.62%		
36) 1,2-Dichloropropane-d6	6.076	67	268971	46.83	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	93.66%		
41) Toluene-d8	7.320	98	799562	45.91	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	91.82%		
43) trans-1,3-Dichloroprop...	7.625	79	136433	44.64	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	89.28%		
47) 2-Hexanone-d5	8.092	63	223520	92.82	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	92.82%		
57) 1,1,2,2-Tetrachloroeth...	10.220	84	370152	44.24	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	88.48%		
64) 1,2-Dichlorobenzene-d4	11.632	152	334037	50.47	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	100.94%		


Target Compounds					Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.108	101	3083	0.69 ug/L	# 19


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020756.D
Acq On : 26 Mar 2021 14:58
Operator : SY/MD
Sample : M1781-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02


Quant Time: Mar 27 06:53:21 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 27 06:50:46 2021
Response via : Initial Calibration

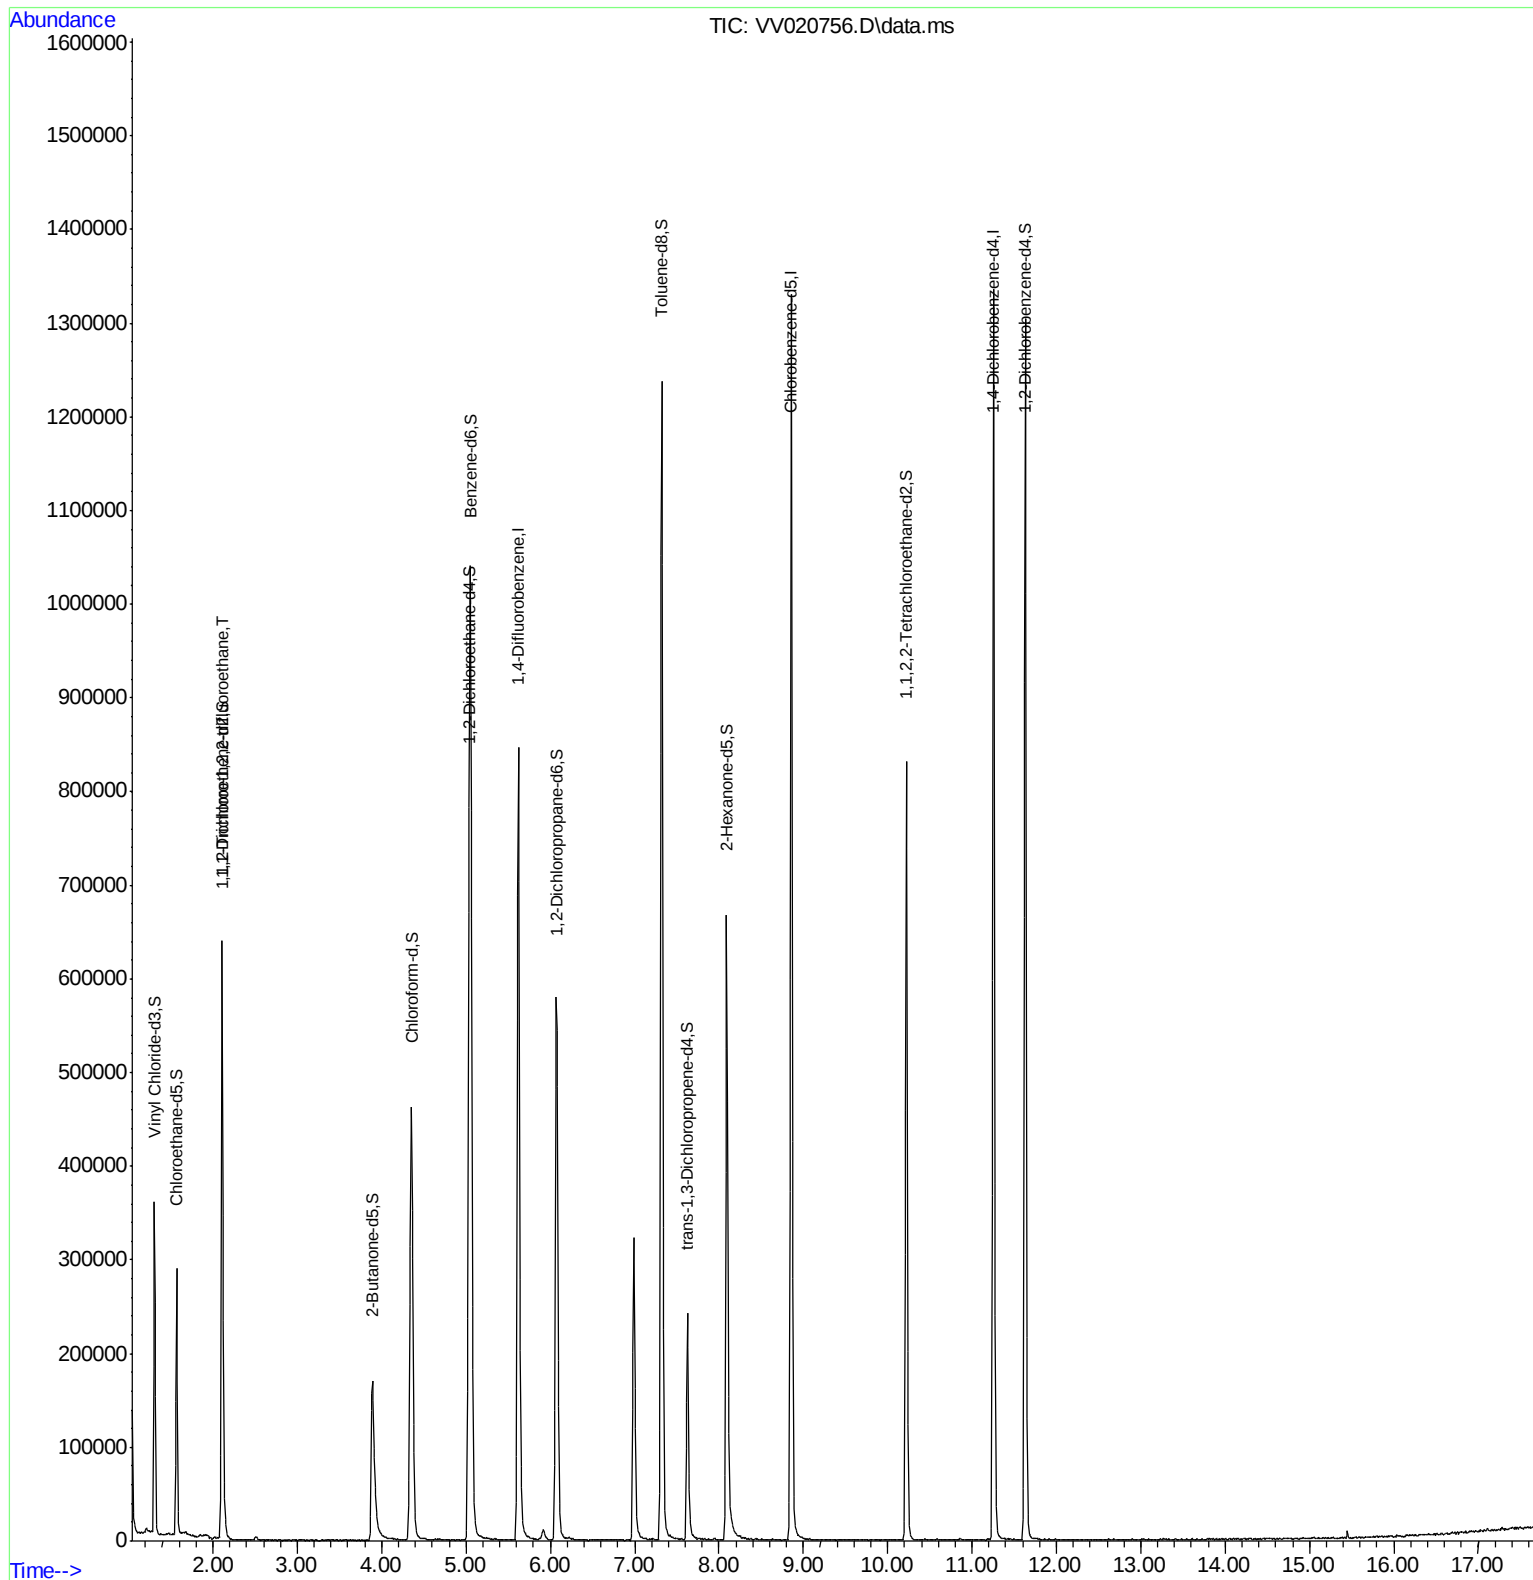

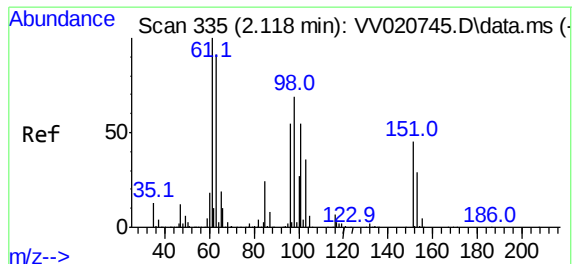

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.69 ug/L
 RT: 2.108 min Scan# 332
 Delta R.T. -0.010 min
 Lab File: VV020756.D
 Acq: 26 Mar 2021 14:58

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

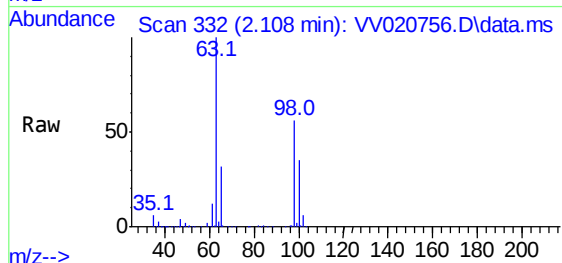

Tgt Ion:101 Resp: 3083
 Ion Ratio Lower Upper
 101 100
 85 0.0 35.4 53.0#
 151 2.3 63.5 95.3#

