

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032621\
 Data File : VW020759.D
 Acq On : 26 Mar 2021 16:09
 Operator : SY/MD
 Sample : M1784-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4W5

Quant Time: Mar 27 06:53:58 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 27 06:50:46 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	540681	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	532203	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	257713	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	154733	40.31	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	80.62%
7) Chloroethane-d5	1.571	69	133582	46.03	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	92.06%
11) 1,1-Dichloroethene-d2	2.111	63	250655	34.61	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	69.22%
21) 2-Butanone-d5	3.892	46	264710	106.00	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	106.00%
24) Chloroform-d	4.352	84	393847	51.62	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.24%
26) 1,2-Dichloroethane-d4	5.037	65	274513	54.62	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	109.24%
32) Benzene-d6	5.053	84	708813	49.97	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.94%
36) 1,2-Dichloropropane-d6	6.075	67	223271	51.27	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	102.54%
41) Toluene-d8	7.320	98	622176	47.12	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.24%
43) trans-1,3-Dichloroprop...	7.625	79	112729	48.65	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	97.30%
47) 2-Hexanone-d5	8.091	63	194447	106.49	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	106.49%
57) 1,1,2,2-Tetrachloroeth...	10.223	84	318995	50.28	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	100.56%
64) 1,2-Dichlorobenzene-d4	11.632	152	279676	55.92	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	111.84%
Target Compounds						
39) cis-1,3-Dichloropropene	6.992	75	6863	1.15	ug/L	Qvalue # 54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020759.D
Acq On : 26 Mar 2021 16:09
Operator : SY/MD
Sample : M1784-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4W5

Quant Time: Mar 27 06:53:58 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 27 06:50:46 2021
Response via : Initial Calibration

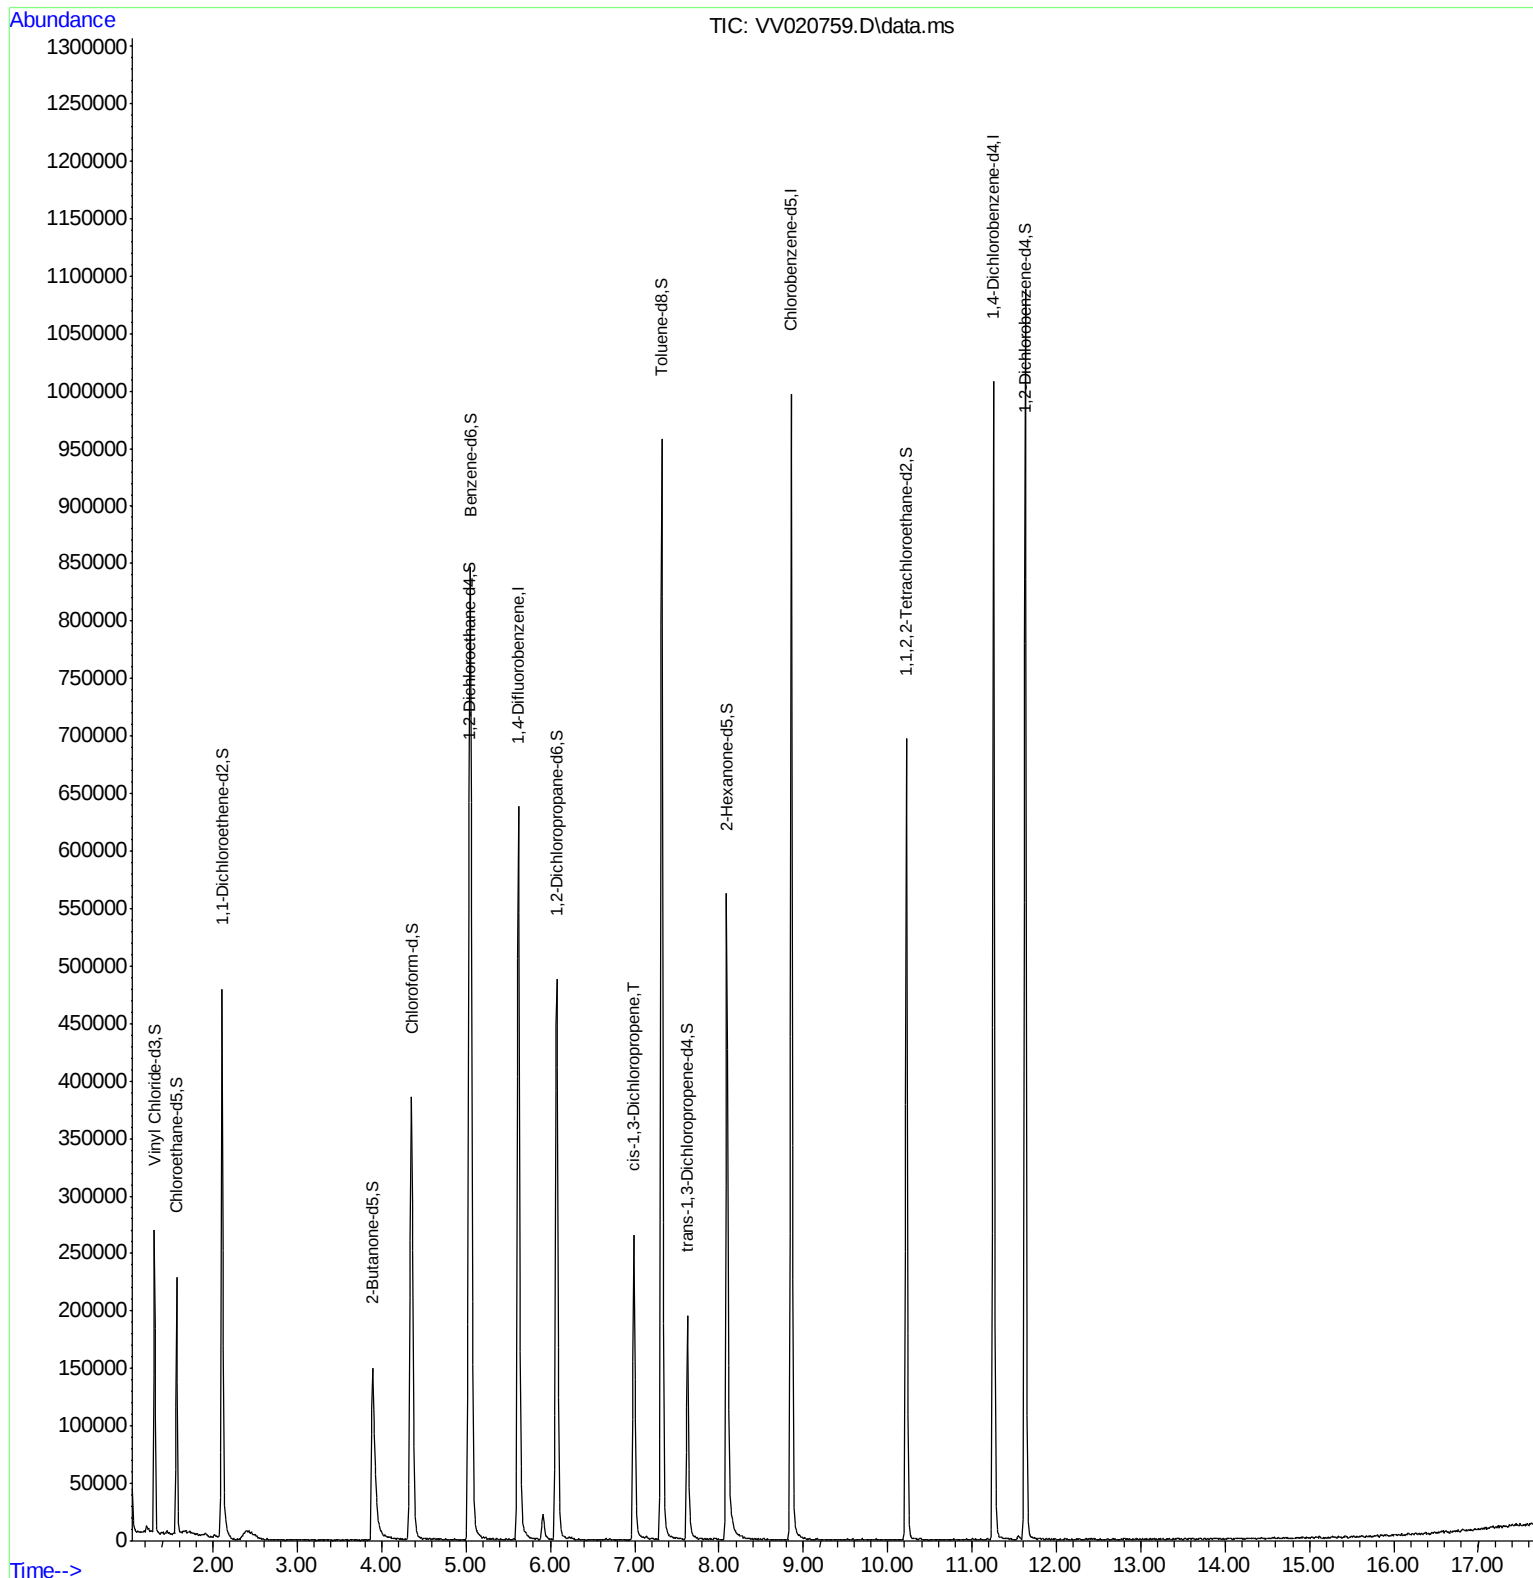

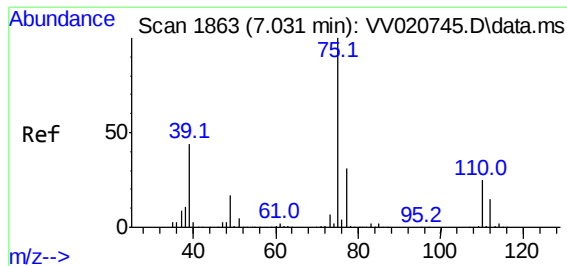

#39
 cis-1,3-Dichloropropene
 Concen: 1.15 ug/L
 RT: 6.992 min Scan# 1851
 Delta R.T. -0.039 min
 Lab File: VV020759.D
 Acq: 26 Mar 2021 16:09

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4W5

Tgt Ion: 75 Resp: 6863
 Ion Ratio Lower Upper
 75 100
 77 56.1 21.7 40.3#

