

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032621\
 Data File : VW020776.D
 Acq On : 26 Mar 2021 23:15
 Operator : SY/MD
 Sample : M1824-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4T1

Quant Time: Mar 27 08:23:42 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 27 08:21:41 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	644651	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	638305	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	310229	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	150809	32.95	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	65.90%		
7) Chloroethane-d5	1.571	69	130474	37.71	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	75.42%		
11) 1,1-Dichloroethene-d2	2.111	63	246636	28.56	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	57.12%#		
21) 2-Butanone-d5	3.892	46	260476	87.48	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	87.48%		
24) Chloroform-d	4.352	84	411642	45.25	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.50%		
26) 1,2-Dichloroethane-d4	5.037	65	282349	47.12	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.24%		
32) Benzene-d6	5.053	84	723225	42.51	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.02%		
36) 1,2-Dichloropropane-d6	6.075	67	233580	44.72	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	89.44%		
41) Toluene-d8	7.320	98	651687	41.15	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	82.30%		
43) trans-1,3-Dichloroprop...	7.625	79	114925	41.35	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	82.70%		
47) 2-Hexanone-d5	8.091	63	190803	87.13	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	87.13%		
57) 1,1,2,2-Tetrachloroeth...	10.220	84	329536	43.31	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	86.62%		
64) 1,2-Dichlorobenzene-d4	11.631	152	296830	49.30	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.60%		
Target Compounds					Qvalue	
48) 2-Hexanone	8.091	43	22150	4.69	ug/L #	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020776.D
Acq On : 26 Mar 2021 23:15
Operator : SY/MD
Sample : M1824-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4T1


Quant Time: Mar 27 08:23:42 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 27 08:21:41 2021
Response via : Initial Calibration

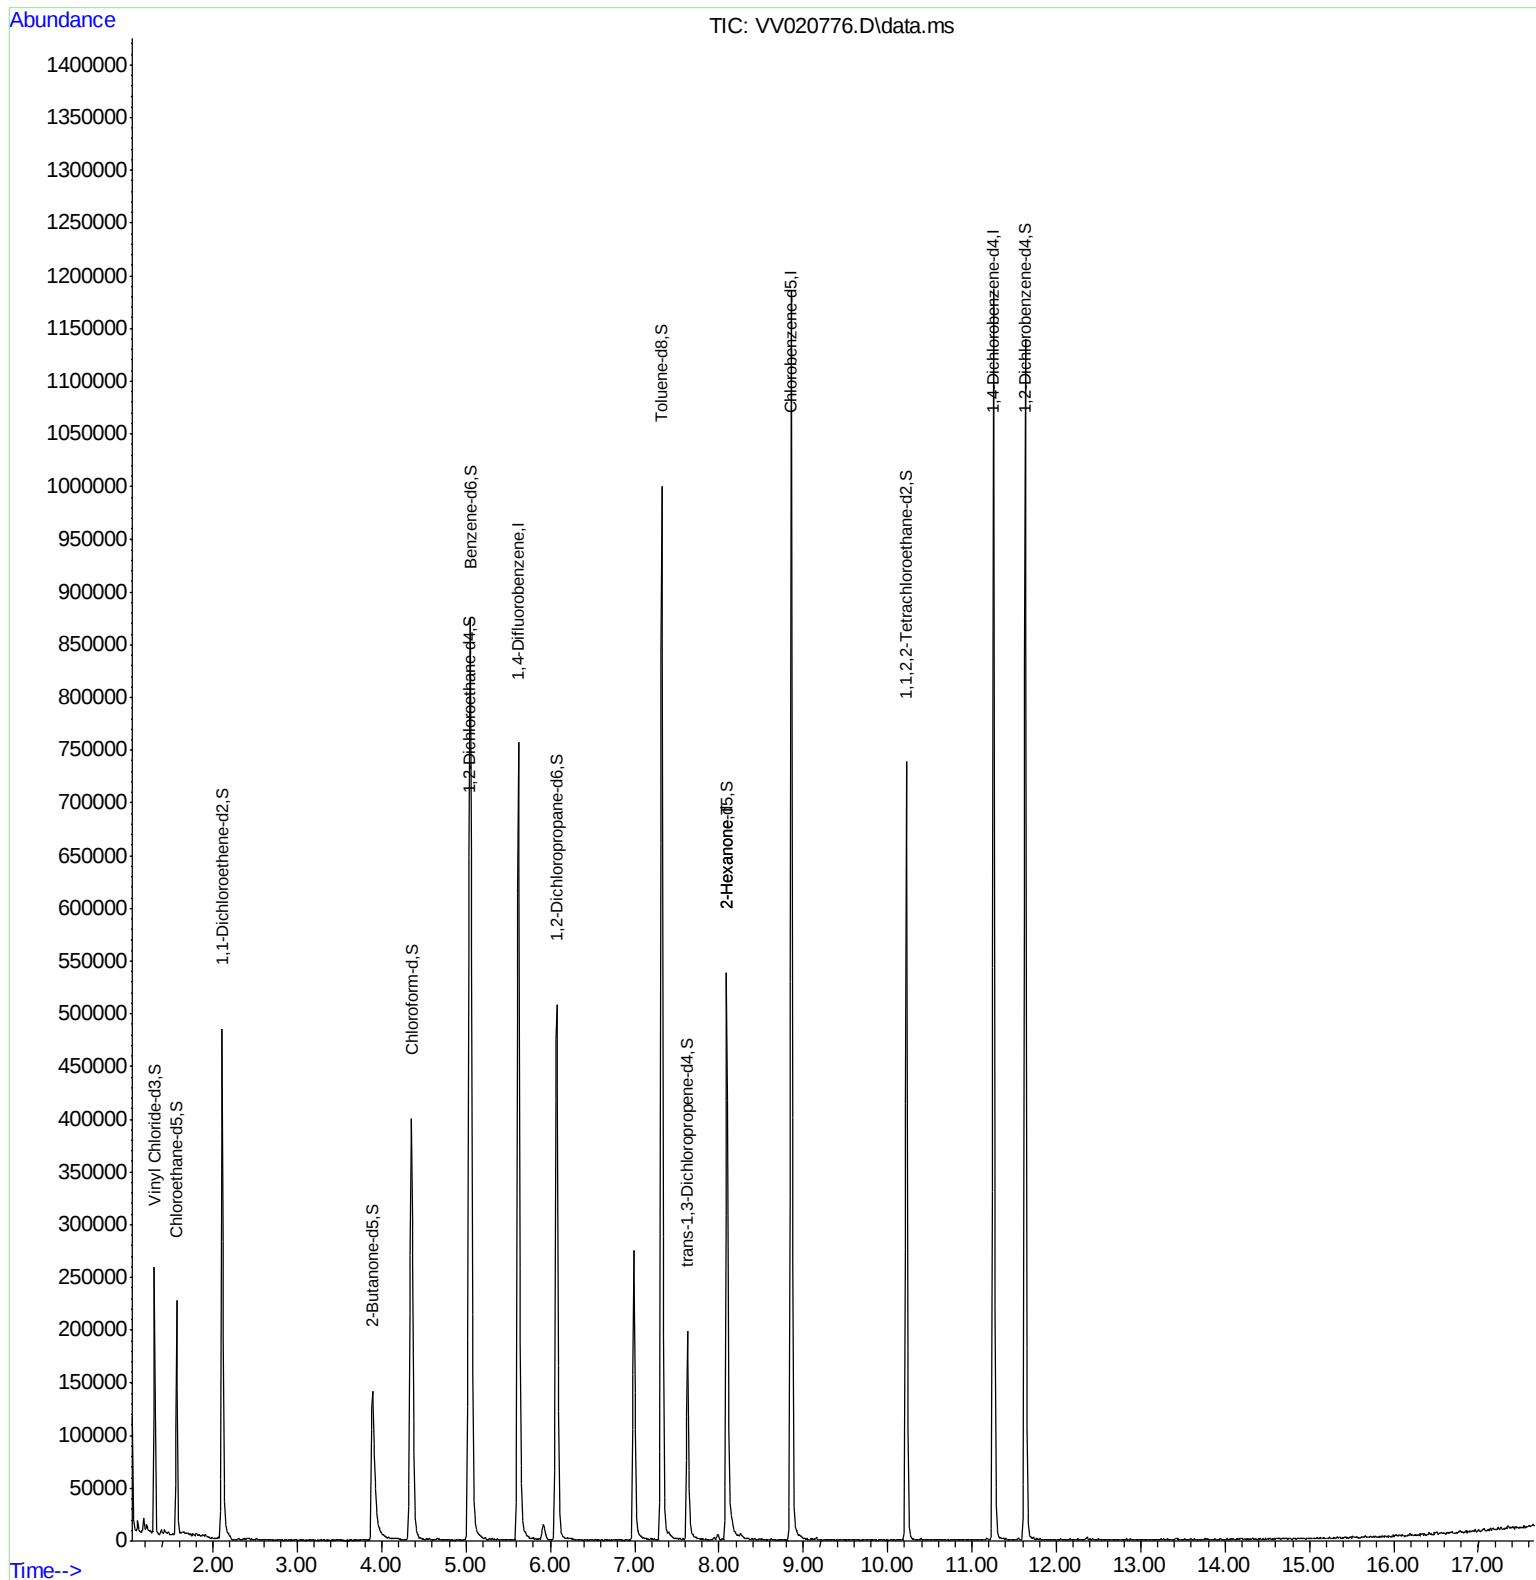

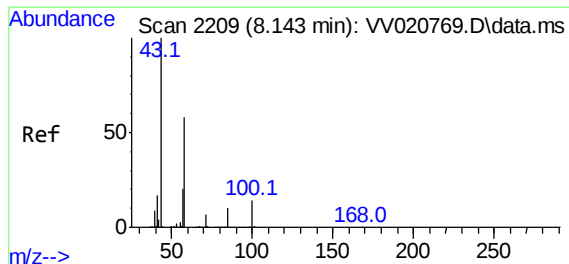

#48
 2-Hexanone
 Concen: 4.69 ug/L
 RT: 8.091 min Scan# 2193
 Delta R.T. -0.052 min
 Lab File: VV020776.D
 Acq: 26 Mar 2021 23:15

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4T1

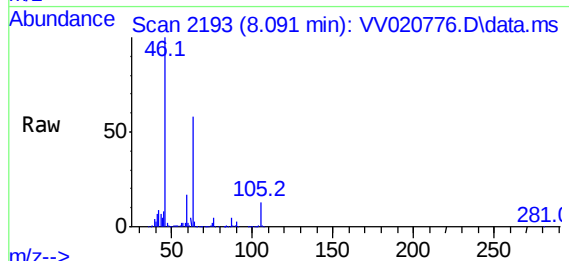

Tgt Ion: 43 Resp: 22150

Ion	Ratio	Lower	Upper
43	100		
58	31.1	45.8	68.8#
57	30.1	15.4	23.2#
100	2.2	10.2	15.4#

