

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020748.D
 Acq On : 26 Mar 2021 11:50
 Operator : SY/MD
 Sample : M1816-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3G1

Quant Time: Mar 27 06:51:55 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 27 06:50:46 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	614840	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	603659	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	296616	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	175054	40.10	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	80.20%		
7) Chloroethane-d5	1.571	69	145736	44.16	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	88.32%		
11) 1,1-Dichloroethene-d2	2.111	63	276655	33.59	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	67.18%		
21) 2-Butanone-d5	3.889	46	280772	98.87	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	98.87%		
24) Chloroform-d	4.352	84	437021	50.37	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.74%		
26) 1,2-Dichloroethane-d4	5.034	65	297533	52.06	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	104.12%		
32) Benzene-d6	5.053	84	773911	48.10	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.20%		
36) 1,2-Dichloropropane-d6	6.072	67	247225	50.05	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	100.10%		
41) Toluene-d8	7.320	98	678416	45.30	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	90.60%		
43) trans-1,3-Dichloroprop...	7.625	79	122127	46.46	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	92.92%		
47) 2-Hexanone-d5	8.091	63	208506	100.67	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	100.67%		
57) 1,1,2,2-Tetrachloroeth...	10.220	84	342879	47.65	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	95.30%		
64) 1,2-Dichlorobenzene-d4	11.631	152	307001	53.33	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	106.66%		
Target Compounds					Qvalue	
13) Acetone	2.185	43	26977	13.32	ug/L	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020748.D
Acq On : 26 Mar 2021 11:50
Operator : SY/MD
Sample : M1816-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3G1

Quant Time: Mar 27 06:51:55 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 27 06:50:46 2021
Response via : Initial Calibration

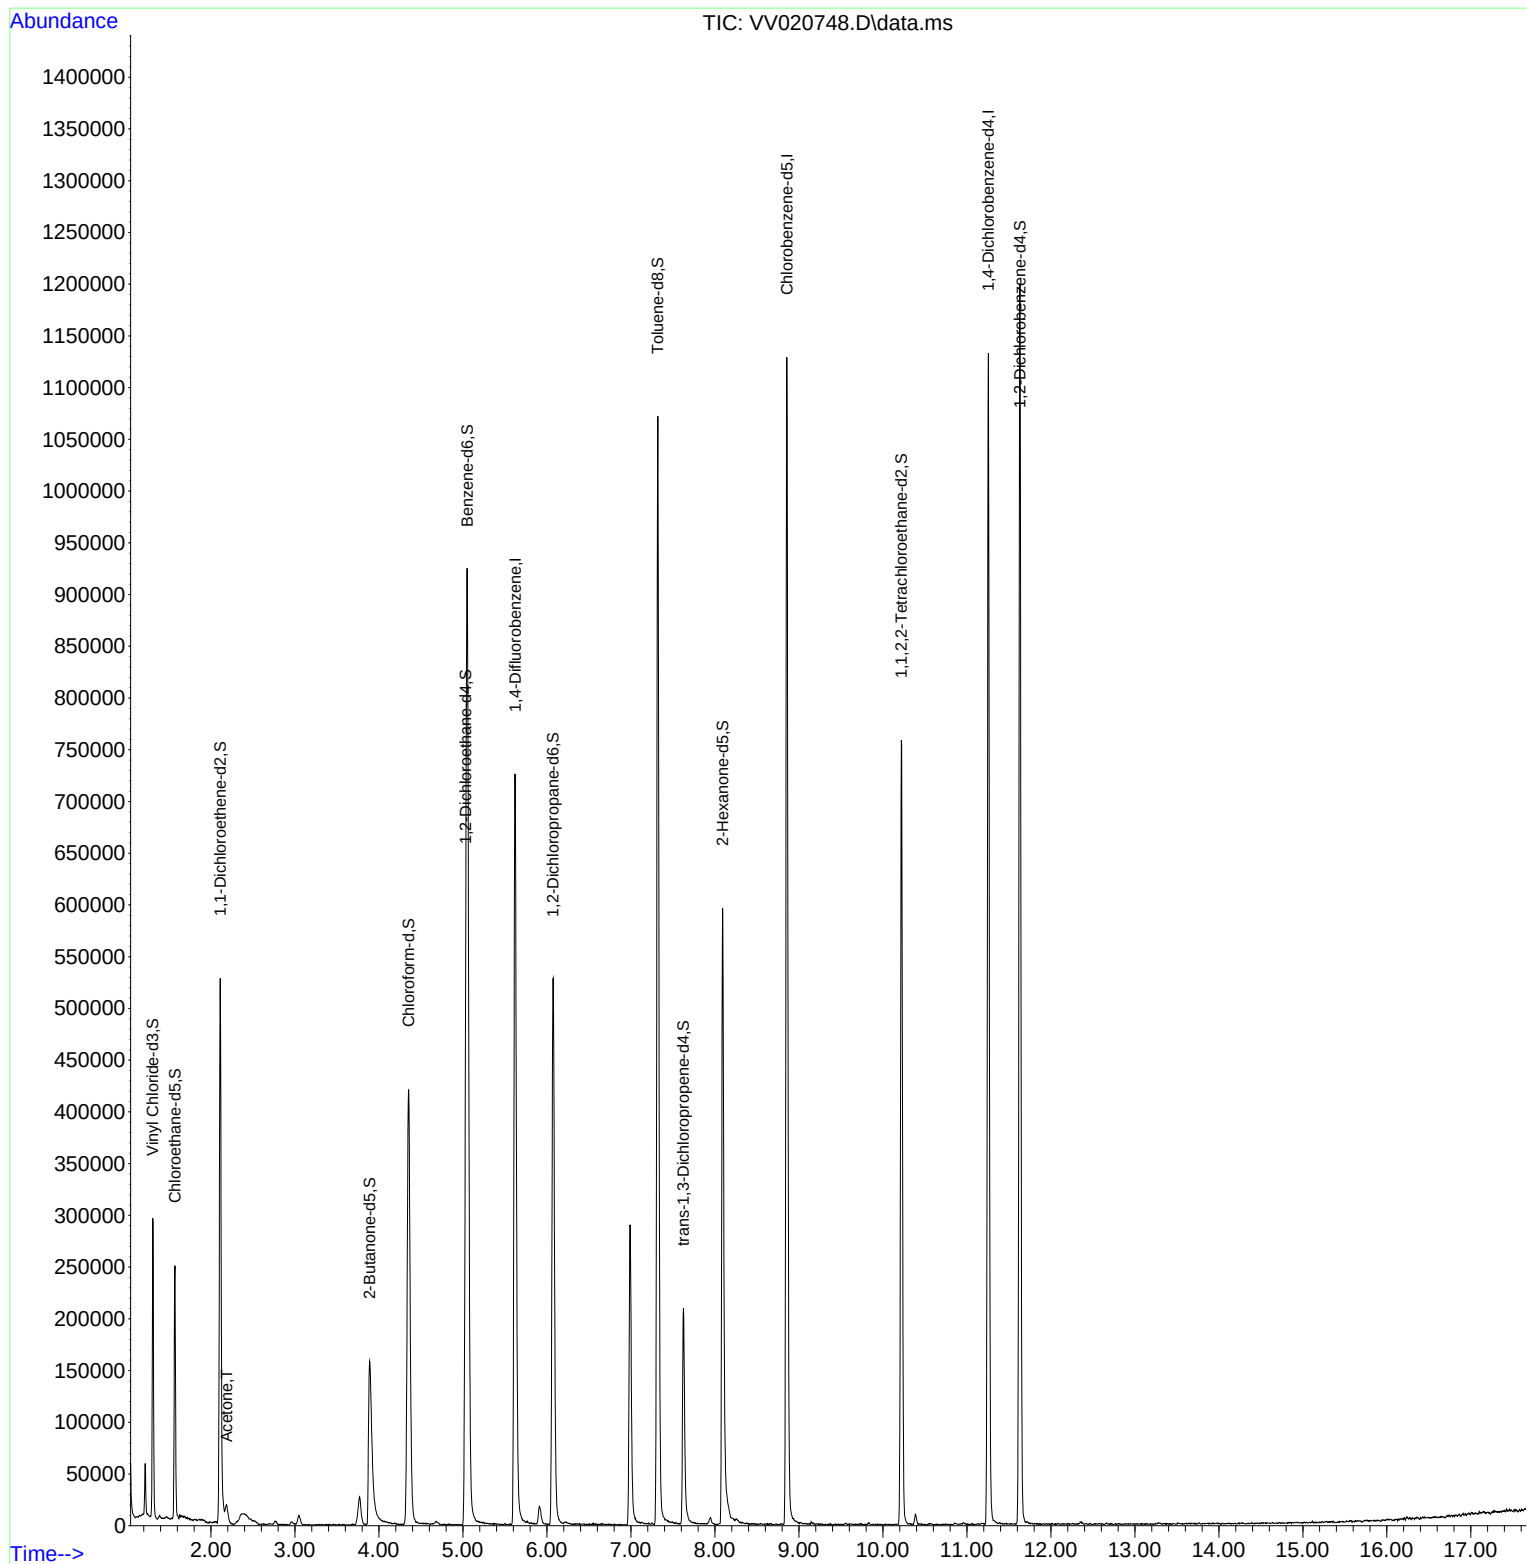

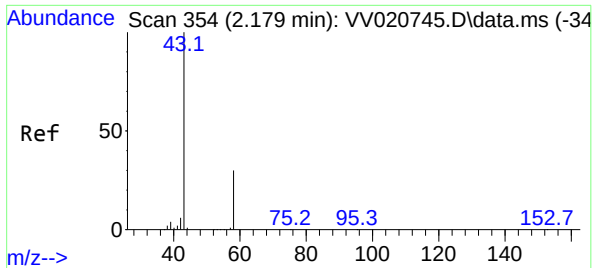

#13
Acetone
Concen: 13.32 ug/L
RT: 2.185 min Scan# 356
Delta R.T. 0.006 min
Lab File: VV020748.D
Acq: 26 Mar 2021 11:50

Instrument :
MSVOA_V
ClientSampleId :
BG3G1

Tgt Ion: 43 Resp: 26977
Ion Ratio Lower Upper
43 100
58 19.4 0.0 60.8

