

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032621\
 Data File : VW020749.D
 Acq On : 26 Mar 2021 12:13
 Operator : SY/MD
 Sample : M1816-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3H6

Quant Time: Mar 27 06:52:08 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 27 06:50:46 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	651479	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	637585	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	308989	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	171818	37.15	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 74.30%			
7) Chloroethane-d5	1.571	69	147828	42.28	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 84.56%			
11) 1,1-Dichloroethene-d2	2.111	63	274955	31.51	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 63.02%			
21) 2-Butanone-d5	3.892	46	274452	91.21	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 91.21%			
24) Chloroform-d	4.352	84	429725	46.74	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 93.48%			
26) 1,2-Dichloroethane-d4	5.037	65	293166	48.41	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 96.82%			
32) Benzene-d6	5.053	84	769597	45.28	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 90.56%			
36) 1,2-Dichloropropane-d6	6.072	67	243925	46.75	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 93.50%			
41) Toluene-d8	7.320	98	676160	42.74	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 85.48%			
43) trans-1,3-Dichloroprop...	7.625	79	122464	44.11	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 88.22%			
47) 2-Hexanone-d5	8.091	63	196695	89.92	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 89.92%			
57) 1,1,2,2-Tetrachloroeth...	10.220	84	336417	44.26	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 88.52%			
64) 1,2-Dichlorobenzene-d4	11.632	152	305968	51.02	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 102.04%			
Target Compounds					Qvalue	
13) Acetone	2.185	43	25077	11.69	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020749.D
Acq On : 26 Mar 2021 12:13
Operator : SY/MD
Sample : M1816-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3H6

Quant Time: Mar 27 06:52:08 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 27 06:50:46 2021
Response via : Initial Calibration

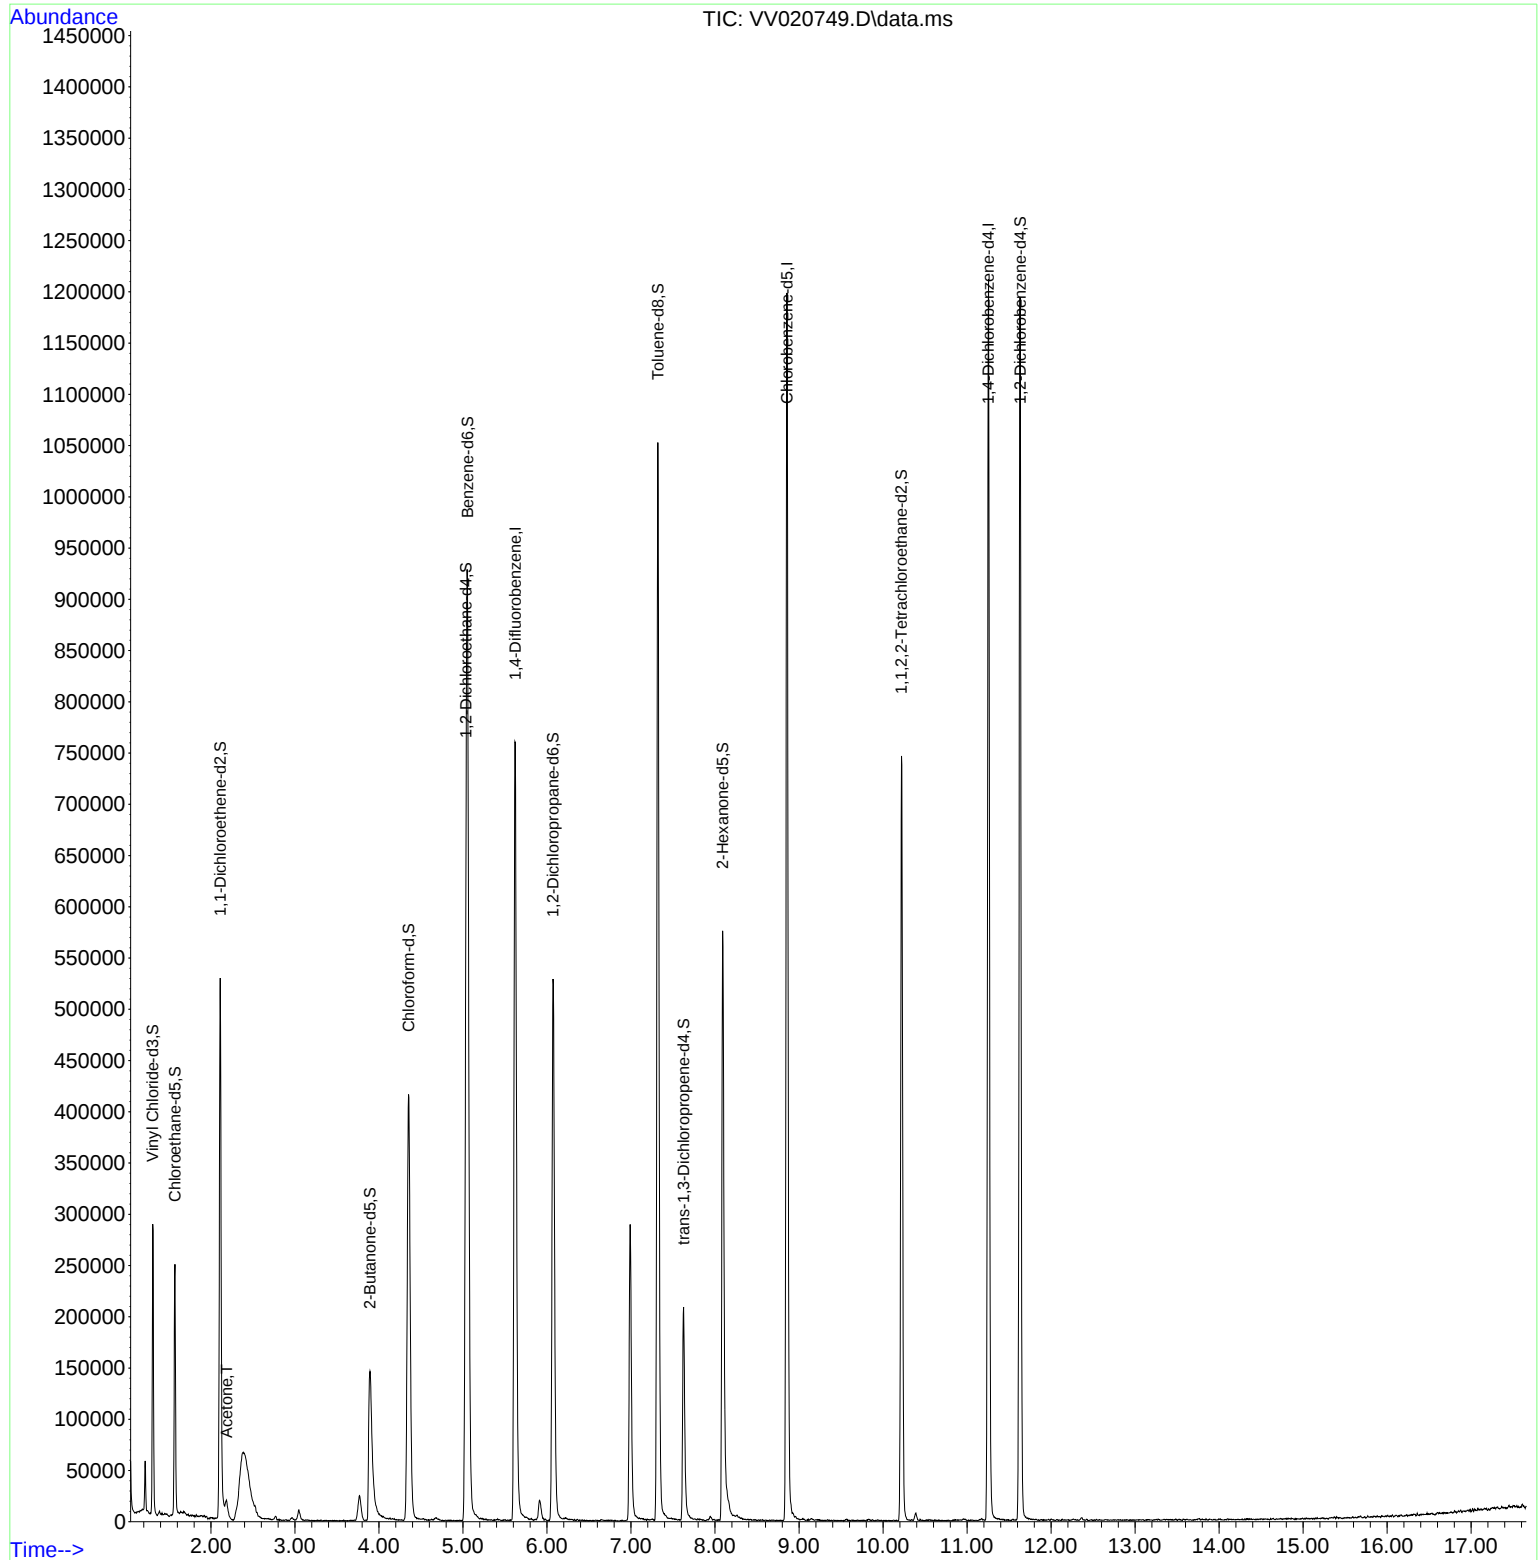

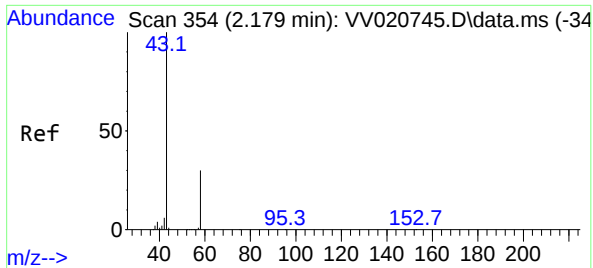

#13
Acetone
Concen: 11.69 ug/L
RT: 2.185 min Scan# 356
Delta R.T. 0.006 min
Lab File: VV020749.D
Acq: 26 Mar 2021 12:13

Instrument :
MSVOA_V
ClientSampleId :
BG3H6

Tgt Ion: 43 Resp: 25077
Ion Ratio Lower Upper
43 100
58 33.8 0.0 60.8

