

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032621\
 Data File : VW020752.D
 Acq On : 26 Mar 2021 13:24
 Operator : SY/MD
 Sample : M1781-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3F9

Quant Time: Mar 27 06:52:45 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 27 06:50:46 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	661314	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	656060	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	317106	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	164436	35.02	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	70.04%	
7) Chloroethane-d5	1.571	69	141005	39.72	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	79.44%	
11) 1,1-Dichloroethene-d2	2.111	63	262700	29.66	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	59.32%#	
21) 2-Butanone-d5	3.892	46	282467	92.48	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	92.48%	
24) Chloroform-d	4.352	84	421739	45.19	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	90.38%	
26) 1,2-Dichloroethane-d4	5.037	65	294724	47.94	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	95.88%	
32) Benzene-d6	5.053	84	756670	43.27	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	86.54%	
36) 1,2-Dichloropropane-d6	6.075	67	241618	45.00	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	90.00%	
41) Toluene-d8	7.320	98	672807	41.33	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	82.66%	
43) trans-1,3-Dichloroprop...	7.625	79	122503	42.89	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	85.78%	
47) 2-Hexanone-d5	8.091	63	203252	90.30	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	90.30%	
57) 1,1,2,2-Tetrachloroeth...	10.220	84	338139	43.24	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	86.48%	
64) 1,2-Dichlorobenzene-d4	11.632	152	307790	50.01	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	100.02%	
Target Compounds						
13) Acetone	2.188	43	26869	12.34	ug/L	Qvalue 76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020752.D
Acq On : 26 Mar 2021 13:24
Operator : SY/MD
Sample : M1781-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3F9

Quant Time: Mar 27 06:52:45 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 27 06:50:46 2021
Response via : Initial Calibration

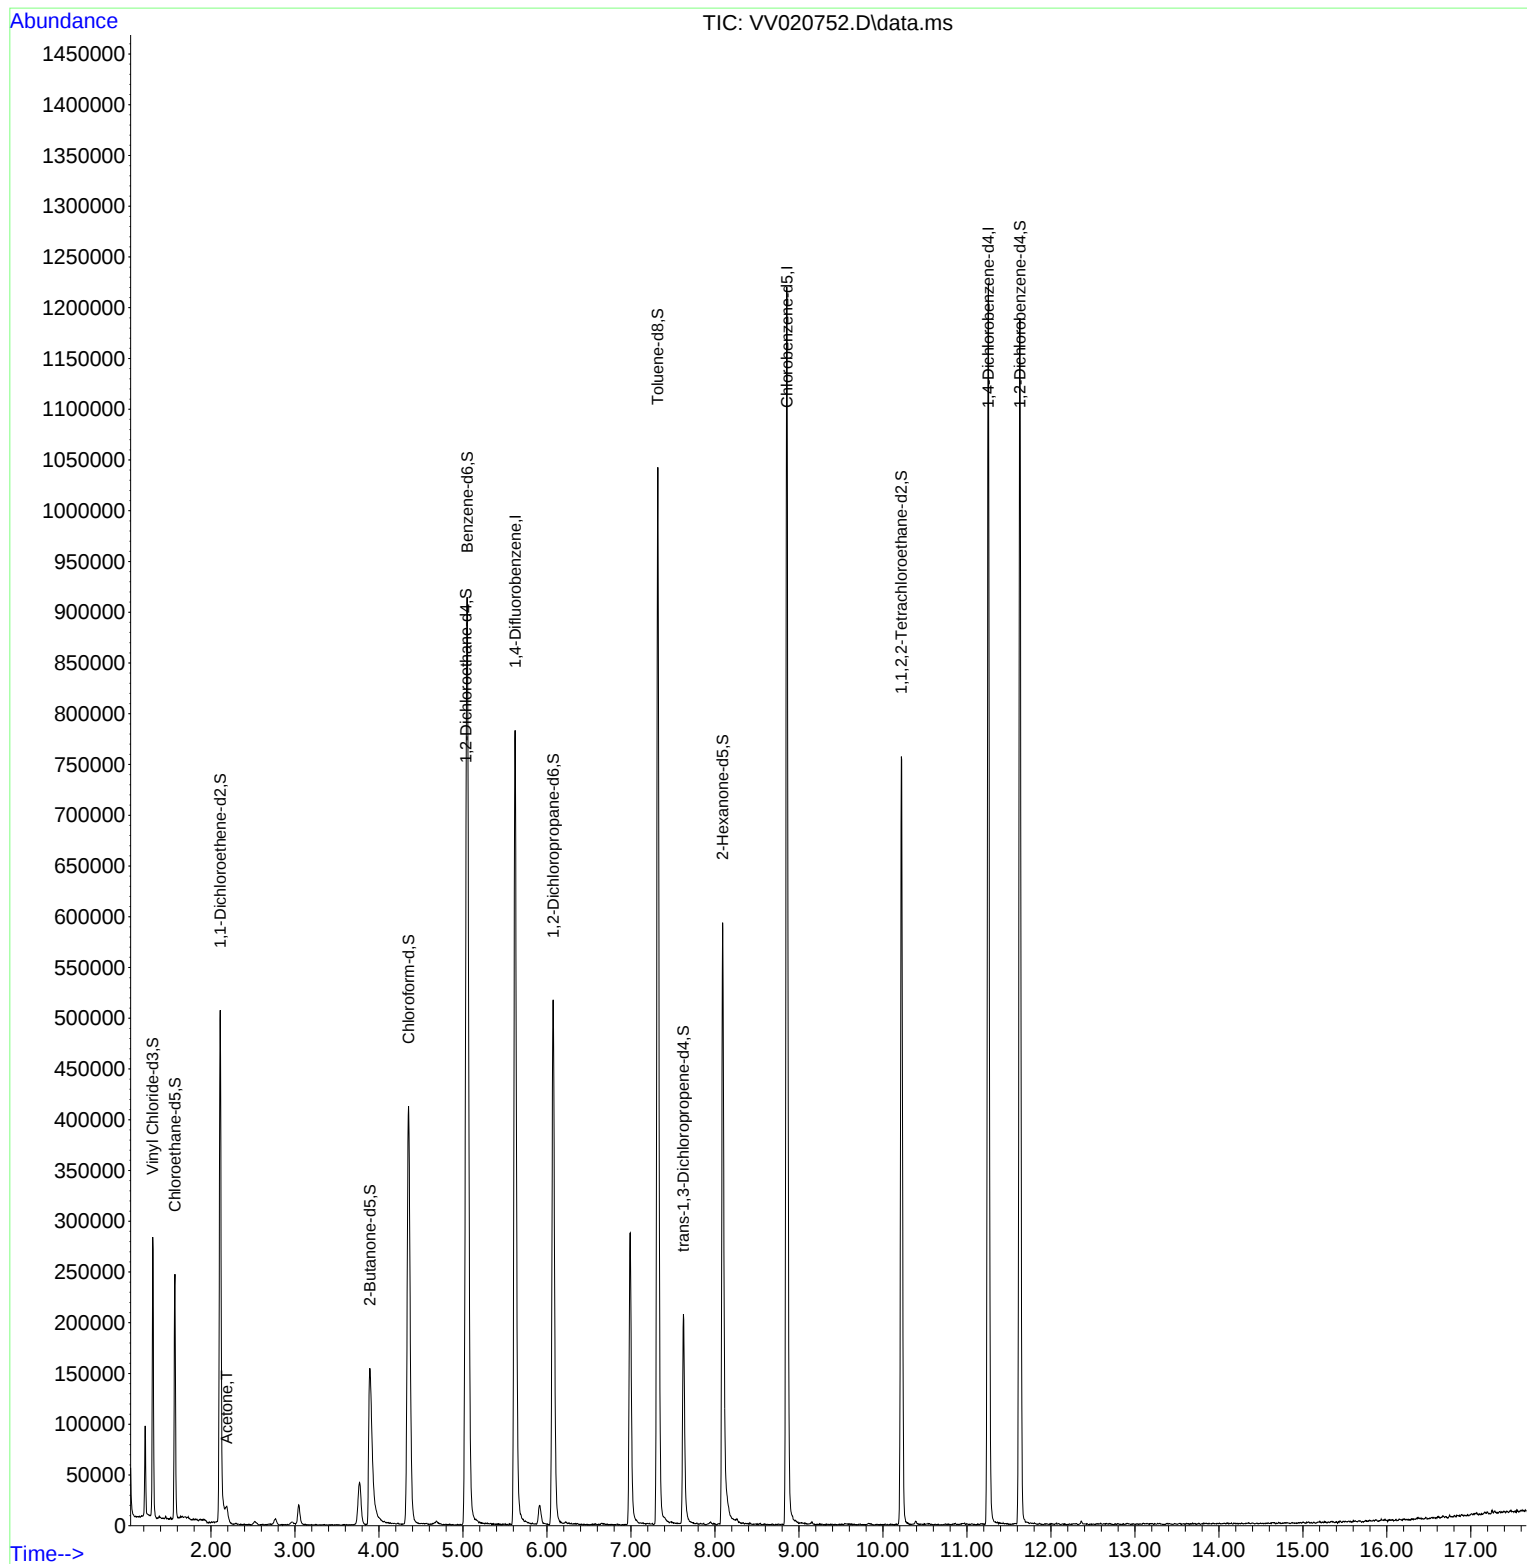

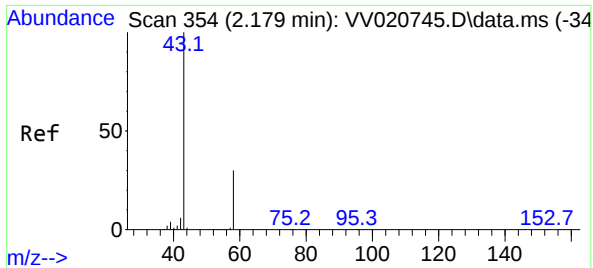

#13
Acetone
Concen: 12.34 ug/L
RT: 2.188 min Scan# 357
Delta R.T. 0.010 min
Lab File: VV020752.D
Acq: 26 Mar 2021 13:24

Instrument :
MSVOA_V
ClientSampleId :
BG3F9

Tgt Ion: 43 Resp: 26869
Ion Ratio Lower Upper
43 100
58 17.4 0.0 60.8

