

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032621\
 Data File : VW020755.D
 Acq On : 26 Mar 2021 14:35
 Operator : SY/MD
 Sample : M1781-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3H5

Quant Time: Mar 27 06:53:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 27 06:50:46 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	639682	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	627227	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	307728	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	156442	34.45	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	68.90%		
7) Chloroethane-d5	1.568	69	133166	38.78	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	77.56%		
11) 1,1-Dichloroethene-d2	2.111	63	252554	29.48	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	58.96%#		
21) 2-Butanone-d5	3.886	46	283131	95.83	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	95.83%		
24) Chloroform-d	4.352	84	405911	44.97	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.94%		
26) 1,2-Dichloroethane-d4	5.037	65	280893	47.24	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.48%		
32) Benzene-d6	5.053	84	723426	43.27	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.54%		
36) 1,2-Dichloropropane-d6	6.076	67	234835	45.75	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	91.50%		
41) Toluene-d8	7.320	98	642330	41.28	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	82.56%		
43) trans-1,3-Dichloroprop...	7.625	79	115741	42.38	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.76%		
47) 2-Hexanone-d5	8.092	63	200753	93.29	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	93.29%		
57) 1,1,2,2-Tetrachloroeth...	10.223	84	327728	43.83	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	87.66%		
64) 1,2-Dichlorobenzene-d4	11.632	152	293920	49.21	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.42%		
Target Compounds					Qvalue	
13) Acetone	2.179	43	27653	13.12	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020755.D
Acq On : 26 Mar 2021 14:35
Operator : SY/MD
Sample : M1781-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3H5

Quant Time: Mar 27 06:53:09 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 27 06:50:46 2021
Response via : Initial Calibration

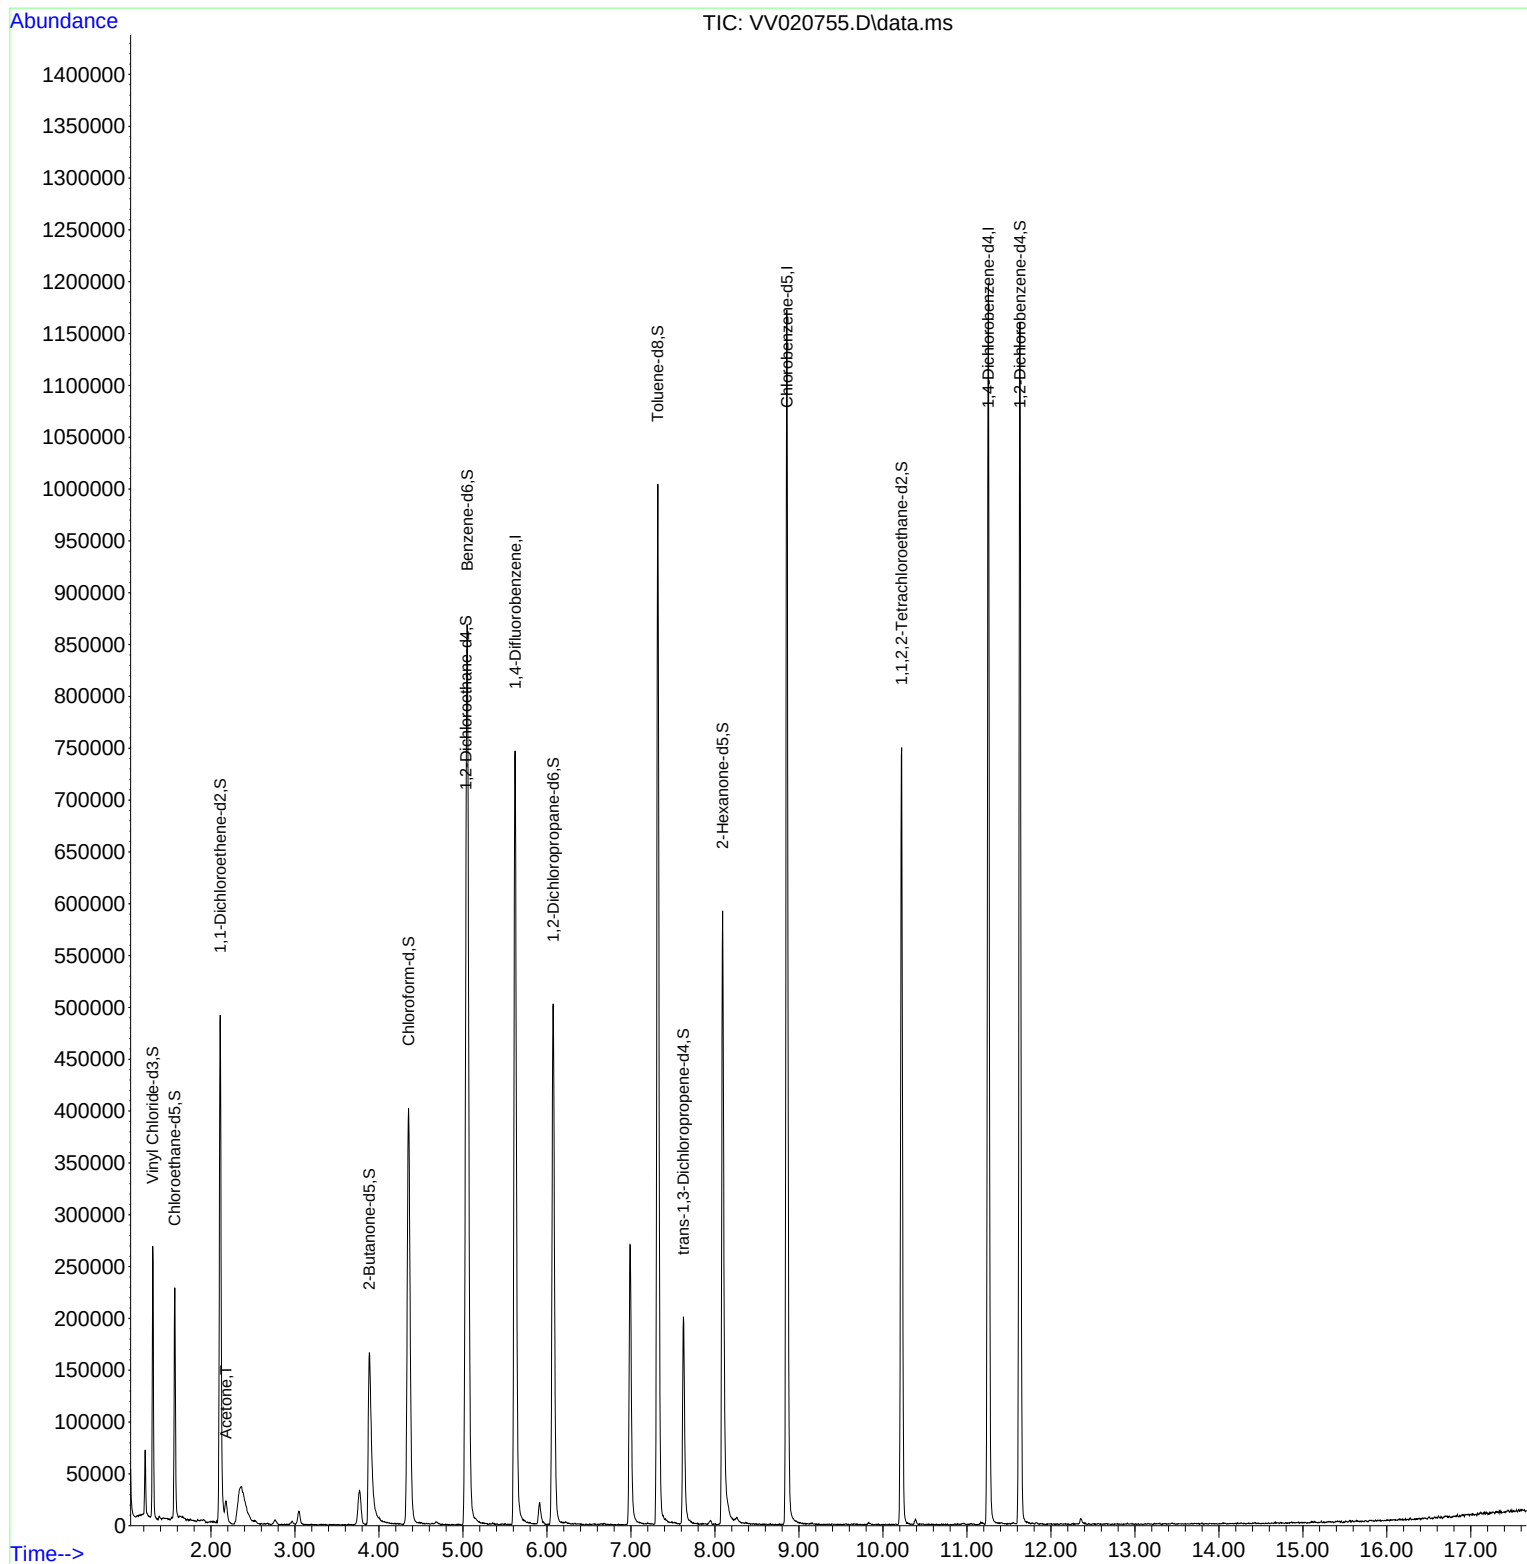

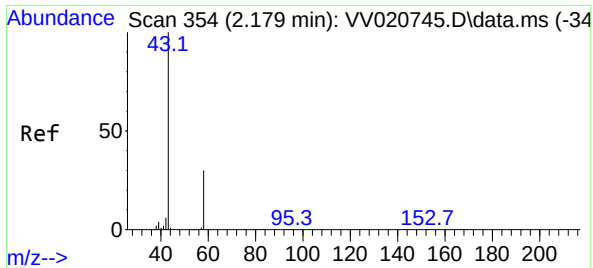

#13
Acetone
Concen: 13.12 ug/L
RT: 2.179 min Scan# 354
Delta R.T. -0.000 min
Lab File: VV020755.D
Acq: 26 Mar 2021 14:35

Instrument :
MSVOA_V
ClientSampleId :
BG3H5

Tgt Ion: 43 Resp: 27653
Ion Ratio Lower Upper
43 100
58 30.1 0.0 60.8

