

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032621\
 Data File : VW020780.D
 Acq On : 27 Mar 2021 00:49
 Operator : SY/MD
 Sample : M1824-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4T5

Quant Time: Mar 27 08:24:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 27 08:21:41 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	645472	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	637368	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	312216	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	142374	31.07	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 62.14%			
7) Chloroethane-d5	1.568	69	127718	36.86	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 73.72%			
11) 1,1-Dichloroethene-d2	2.111	63	240542	27.82	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 55.64%#			
21) 2-Butanone-d5	3.886	46	257691	86.43	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 86.43%			
24) Chloroform-d	4.352	84	396877	43.57	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 87.14%			
26) 1,2-Dichloroethane-d4	5.037	65	273894	45.65	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 91.30%			
32) Benzene-d6	5.053	84	711656	41.89	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 83.78%			
36) 1,2-Dichloropropane-d6	6.072	67	224746	43.09	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 86.18%			
41) Toluene-d8	7.320	98	631621	39.94	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 79.88%#			
43) trans-1,3-Dichloroprop...	7.625	79	110662	39.88	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 79.76%			
47) 2-Hexanone-d5	8.091	63	188297	86.11	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 86.11%			
57) 1,1,2,2-Tetrachloroeth...	10.220	84	319802	42.09	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 84.18%			
64) 1,2-Dichlorobenzene-d4	11.632	152	287901	47.51	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 95.02%			
Target Compounds					Qvalue	
13) Acetone	2.182	43	7375	3.47	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020780.D
Acq On : 27 Mar 2021 00:49
Operator : SY/MD
Sample : M1824-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4T5

Quant Time: Mar 27 08:24:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 27 08:21:41 2021
Response via : Initial Calibration

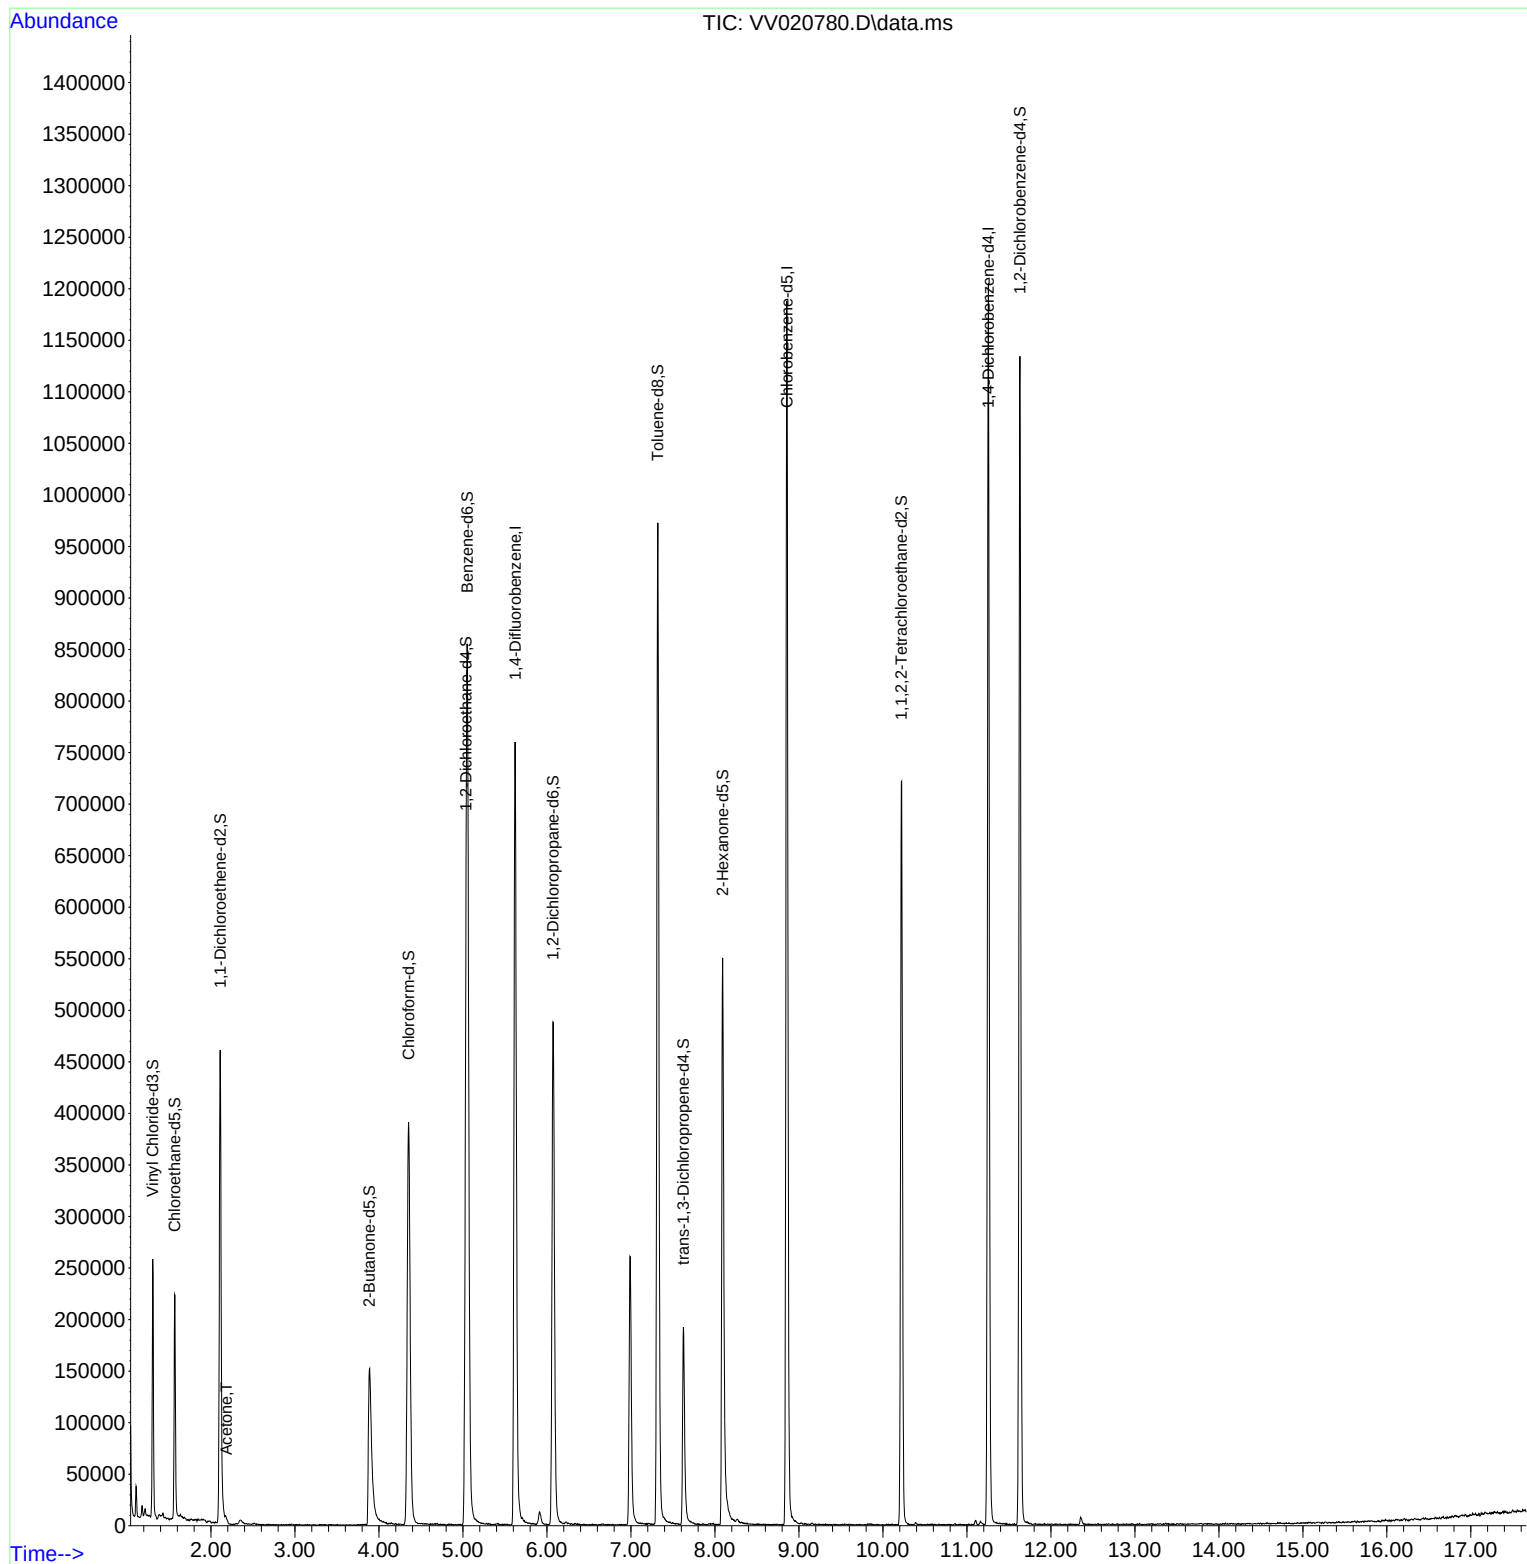

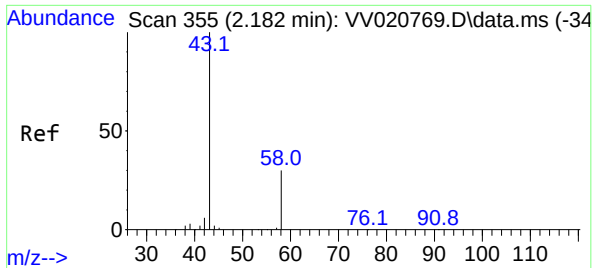

#13
 Acetone
 Concen: 3.47 ug/L
 RT: 2.182 min Scan# 355
 Delta R.T. 0.000 min
 Lab File: VV020780.D
 Acq: 27 Mar 2021 00:49

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4T5

Tgt Ion: 43 Resp: 7375
 Ion Ratio Lower Upper
 43 100
 58 30.5 0.0 60.8

