

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020747.D
 Acq On : 26 Mar 2021 11:26
 Operator : SY/MD
 Sample : VV0326WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020747.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	101	rVB	352158	360776	13.35%	1.767%
2	1.571	158	165	176	rBV	285585	315859	11.69%	1.547%
3	2.111	322	333	361	rVB	639774	966786	35.78%	4.736%
4	2.352	406	408	412	rVB2	869	508	0.02%	0.002%
5	2.375	412	415	416	rBV	879	525	0.02%	0.003%
6	2.436	431	434	436	rBV2	913	719	0.03%	0.004%
7	2.478	445	447	449	rBV3	608	245	0.01%	0.001%
8	2.574	475	477	480	rVB2	563	326	0.01%	0.002%
9	2.597	480	484	488	rVB5	766	534	0.02%	0.003%
10	2.696	511	515	518	rBV3	520	368	0.01%	0.002%
11	2.715	518	521	522	rBV	354	171	0.01%	0.001%
12	2.757	530	534	535	rBV2	1632	1024	0.04%	0.005%
13	2.806	547	549	552	rBV	453	259	0.01%	0.001%
14	2.822	552	554	557	rVB3	887	518	0.02%	0.003%
15	2.854	557	564	566	rBV2	927	881	0.03%	0.004%
16	2.908	579	581	583	rVB2	622	292	0.01%	0.001%
17	2.931	583	588	593	rBV4	829	1181	0.04%	0.006%
18	2.998	606	609	611	rVB2	506	231	0.01%	0.001%
19	3.108	641	643	647	rVB2	388	235	0.01%	0.001%
20	3.156	656	658	660	rVB	619	260	0.01%	0.001%
21	3.175	660	664	667	rBV2	420	435	0.02%	0.002%
22	3.198	667	671	673	rBV4	803	506	0.02%	0.002%
23	3.262	689	691	693	rBV4	486	235	0.01%	0.001%
24	3.275	693	695	697	rBV	522	242	0.01%	0.001%
25	3.317	706	708	711	rBV2	404	220	0.01%	0.001%
26	3.375	722	726	727	rBV2	644	397	0.01%	0.002%
27	3.436	743	745	749	rBV2	540	464	0.02%	0.002%
28	3.468	753	755	758	rBV	473	220	0.01%	0.001%
29	3.484	758	760	762	rBV	448	261	0.01%	0.001%
30	3.535	773	776	781	rBV2	802	753	0.03%	0.004%
31	3.619	799	802	805	rBV2	744	465	0.02%	0.002%
32	3.641	807	809	813	rVB2	507	285	0.01%	0.001%
33	3.664	813	816	817	rBV	691	304	0.01%	0.001%
34	3.693	822	825	830	rVB2	888	608	0.02%	0.003%
35	3.735	835	838	839	rBV	301	171	0.01%	0.001%
36	3.789	853	855	857	rBV	510	187	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020747.D
 Acq On : 26 Mar 2021 11:26
 Operator : SY/MD
 Sample : VV0326WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	3.838	867	870	871	rVB2	322	171	0.01%	0.001%
38	3.892	876	887	920	rBV	173813	517599	19.15%	2.535%
39	4.352	1014	1030	1057	rBV	462678	1133847	41.96%	5.554%
40	4.805	1168	1171	1173	rBV3	858	497	0.02%	0.002%
41	4.899	1198	1200	1201	rBV2	642	219	0.01%	0.001%
42	4.940	1211	1213	1215	rBV3	670	255	0.01%	0.001%
43	5.050	1228	1247	1282	rBV2	1047571	2702325	100.00%	13.237%
44	5.542	1397	1400	1404	rBV3	864	827	0.03%	0.004%
45	5.561	1404	1406	1411	rVB2	571	265	0.01%	0.001%
46	5.622	1411	1425	1459	rBV	792205	1593144	58.95%	7.804%
47	5.979	1534	1536	1539	rVB3	876	351	0.01%	0.002%
48	6.072	1550	1565	1597	rBV	578192	1187420	43.94%	5.817%
49	6.394	1663	1665	1668	rBV2	663	446	0.02%	0.002%
50	6.420	1671	1673	1674	rBV2	593	201	0.01%	0.001%
51	6.477	1687	1691	1692	rBV2	547	421	0.02%	0.002%
52	6.558	1714	1716	1719	rBV2	586	326	0.01%	0.002%
53	6.603	1728	1730	1733	rBV	434	285	0.01%	0.001%
54	6.664	1747	1749	1750	rBV	784	315	0.01%	0.002%
55	6.709	1761	1763	1766	rBV2	862	574	0.02%	0.003%
56	6.735	1768	1771	1772	rBV2	596	308	0.01%	0.002%
57	6.844	1802	1805	1806	rBV2	438	245	0.01%	0.001%
58	6.863	1809	1811	1812	rBV	721	290	0.01%	0.001%
59	6.918	1826	1828	1831	rVB	474	182	0.01%	0.001%
60	6.934	1831	1833	1836	rVB2	396	159	0.01%	0.001%
61	6.989	1836	1850	1879	rBV	324254	600637	22.23%	2.942%
62	7.320	1940	1953	1976	rBV	1241098	2119998	78.45%	10.385%
63	7.625	2038	2048	2079	rBV	237157	420073	15.54%	2.058%
64	7.899	2130	2133	2136	rBV3	931	702	0.03%	0.003%
65	8.040	2175	2177	2180	rBV3	414	292	0.01%	0.001%
66	8.091	2182	2193	2222	rBV	663247	1185458	43.87%	5.807%
67	8.561	2337	2339	2342	rBV2	824	543	0.02%	0.003%
68	8.603	2349	2352	2353	rBV2	877	456	0.02%	0.002%
69	8.622	2353	2358	2361	rVB6	1184	978	0.04%	0.005%
70	8.699	2378	2382	2387	rBV3	925	1105	0.04%	0.005%
71	8.857	2418	2431	2452	rBV	1254928	1995315	73.84%	9.774%
72	9.275	2557	2561	2564	rBV3	1215	881	0.03%	0.004%
73	9.294	2565	2567	2568	rBV2	539	183	0.01%	0.001%
74	9.310	2571	2572	2573	rBV	763	291	0.01%	0.001%
75	9.387	2592	2596	2597	rBV2	774	487	0.02%	0.002%
76	9.635	2670	2673	2674	rBV	651	312	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020747.D
 Acq On : 26 Mar 2021 11:26
 Operator : SY/MD
 Sample : VV0326WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

77	10.011	2787	2790	2792	rBV	540	292	0.01%	0.001%
78	10.088	2810	2814	2817	rBV4	715	746	0.03%	0.004%
79	10.152	2831	2834	2836	rVB5	726	291	0.01%	0.001%
80	10.165	2836	2838	2841	rBV	531	286	0.01%	0.001%
81	10.223	2843	2856	2881	rVV	842796	1324410	49.01%	6.488%
82	10.448	2925	2926	2928	rBV	365	190	0.01%	0.001%
83	10.493	2938	2940	2942	rBV2	530	268	0.01%	0.001%
84	10.551	2955	2958	2961	rBV3	1324	926	0.03%	0.005%
85	10.628	2980	2982	2985	rBV	676	498	0.02%	0.002%
86	10.802	3031	3036	3037	rBV2	728	596	0.02%	0.003%
87	10.847	3048	3050	3051	rBV	1043	369	0.01%	0.002%
88	10.921	3070	3073	3075	rBV2	1233	856	0.03%	0.004%
89	11.172	3147	3151	3152	rBV3	809	542	0.02%	0.003%
90	11.255	3165	3177	3200	rBV	1246744	1914938	70.86%	9.380%
91	11.632	3282	3294	3312	rBV	1312323	2038861	75.45%	9.987%
92	11.934	3386	3388	3391	rBV2	960	625	0.02%	0.003%
93	12.056	3422	3426	3432	rBV5	942	1085	0.04%	0.005%
94	12.149	3453	3455	3457	rBV2	838	314	0.01%	0.002%
95	12.638	3605	3607	3608	rBV	612	330	0.01%	0.002%
96	13.024	3724	3727	3728	rBV	652	303	0.01%	0.001%
97	13.117	3754	3756	3757	rBV	681	237	0.01%	0.001%
98	13.230	3789	3791	3796	rBV4	850	871	0.03%	0.004%
99	13.400	3843	3844	3847	rBV	622	224	0.01%	0.001%
100	13.493	3870	3873	3875	rBV2	911	673	0.02%	0.003%




Sum of corrected areas: 20414565

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020747.D
Acq On : 26 Mar 2021 11:26
Operator : SY/MD
Sample : VV0326WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

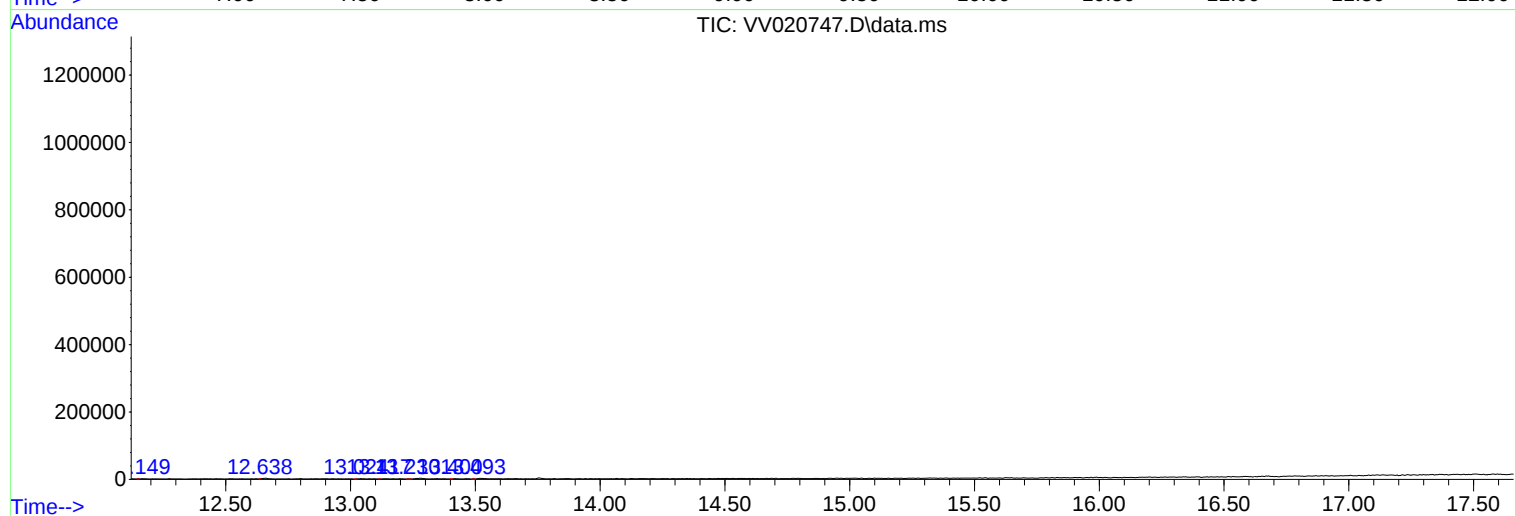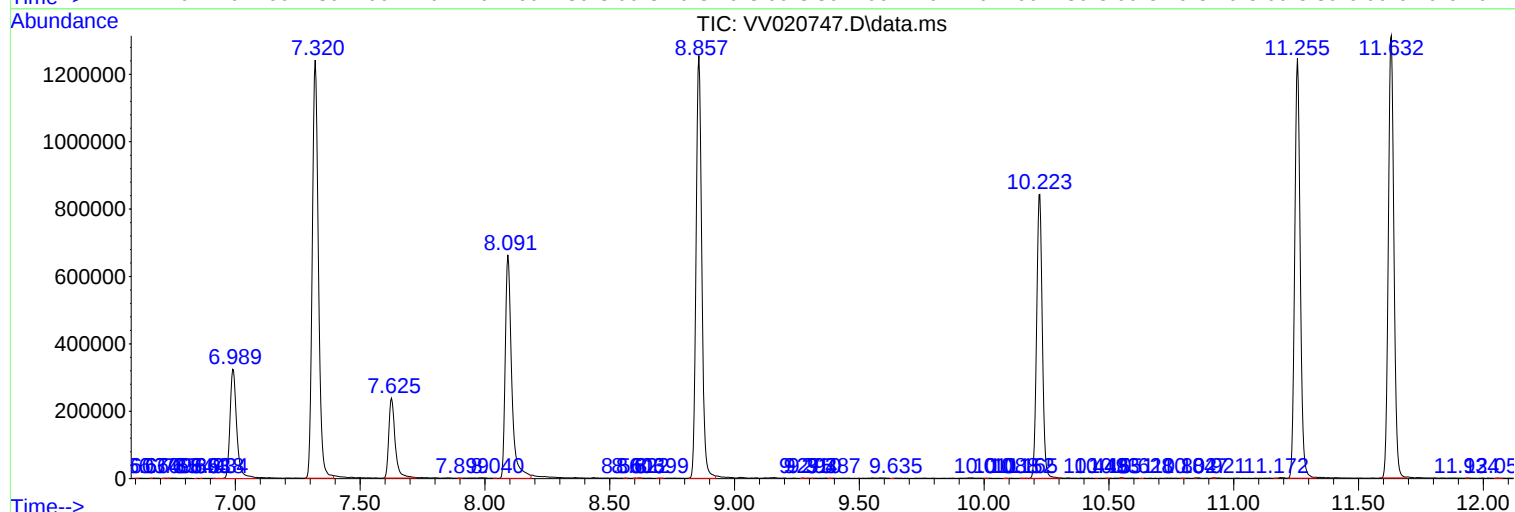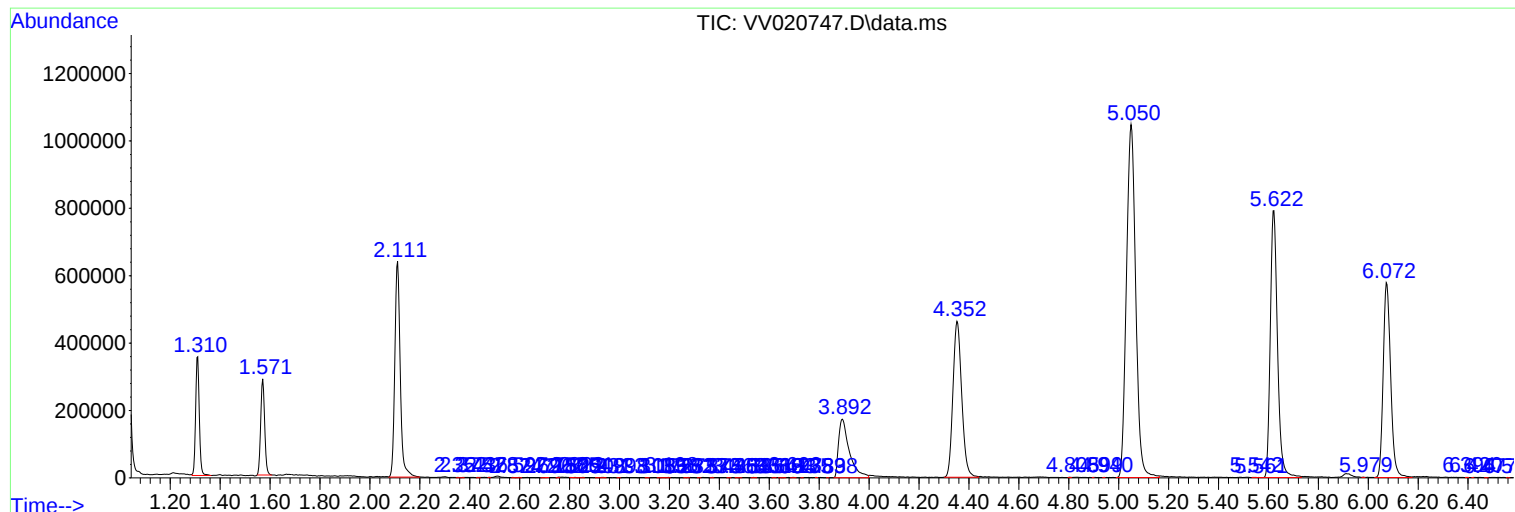

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020747.D
Acq On : 26 Mar 2021 11:26
Operator : SY/MD
Sample : VV0326WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020747.D
Acq On : 26 Mar 2021 11:26
Operator : SY/MD
Sample : VV0326WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
