

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020749.D
 Acq On : 26 Mar 2021 12:13
 Operator : SY/MD
 Sample : M1816-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3H6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020749.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	51	55	61	rVB	48612	41441	1.73%	0.222%
2	1.307	77	83	99	rVB	284432	291794	12.19%	1.565%
3	1.571	158	165	177	rVB	242441	265362	11.09%	1.423%
4	2.111	323	333	349	rBV	525580	776914	32.46%	4.167%
5	2.825	553	555	560	rBV4	896	778	0.03%	0.004%
6	2.966	590	599	604	rBV6	2533	4442	0.19%	0.024%
7	3.236	681	683	685	rBV2	562	318	0.01%	0.002%
8	3.336	712	714	715	rBV	297	138	0.01%	0.001%
9	3.420	737	740	742	rBV3	336	204	0.01%	0.001%
10	3.471	754	756	760	rVB3	627	406	0.02%	0.002%
11	3.490	760	762	766	rBV3	461	283	0.01%	0.002%
12	3.510	766	768	769	rBV	373	139	0.01%	0.001%
13	3.535	774	776	778	rBV2	742	392	0.02%	0.002%
14	3.580	788	790	793	rVB3	962	444	0.02%	0.002%
15	3.616	799	801	803	rVB2	840	325	0.01%	0.002%
16	3.629	803	805	808	rBV	561	336	0.01%	0.002%
17	3.683	820	822	824	rBV3	349	142	0.01%	0.001%
18	3.767	834	848	867	rVB5	24255	62350	2.60%	0.334%
19	3.892	876	887	921	rBV2	145154	448109	18.72%	2.403%
20	4.352	1015	1030	1060	rBV	413881	1017298	42.50%	5.456%
21	4.757	1153	1156	1160	rBV2	836	649	0.03%	0.003%
22	4.796	1163	1168	1171	rVB3	737	660	0.03%	0.004%
23	4.818	1173	1175	1178	rBV4	721	489	0.02%	0.003%
24	4.847	1181	1184	1186	rBV4	909	430	0.02%	0.002%
25	4.928	1207	1209	1212	rBV2	676	351	0.01%	0.002%
26	4.989	1226	1228	1230	rBV3	575	267	0.01%	0.001%
27	5.050	1230	1247	1279	rBV2	928146	2393592	100.00%	12.838%
28	5.368	1344	1346	1348	rBV3	707	330	0.01%	0.002%
29	5.413	1358	1360	1362	rVB3	1205	411	0.02%	0.002%
30	5.471	1376	1378	1379	rBV2	489	194	0.01%	0.001%
31	5.487	1379	1383	1384	rBV3	925	529	0.02%	0.003%
32	5.558	1401	1405	1407	rBV3	1188	851	0.04%	0.005%
33	5.619	1412	1424	1461	rVV	759500	1542805	64.46%	8.275%
34	5.912	1503	1515	1527	rBV5	19028	41581	1.74%	0.223%
35	5.979	1532	1536	1540	rVB6	1256	1115	0.05%	0.006%
36	6.021	1546	1549	1551	rBV3	612	320	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020749.D
 Acq On : 26 Mar 2021 12:13
 Operator : SY/MD
 Sample : M1816-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3H6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	6.072	1551	1565	1588	rBV	528466	1075899	44.95%	5.770%
38	6.358	1651	1654	1660	rVB6	1474	1665	0.07%	0.009%
39	6.391	1660	1664	1665	rBV3	1032	615	0.03%	0.003%
40	6.445	1679	1681	1686	rVB3	724	337	0.01%	0.002%
41	6.474	1686	1690	1693	rBV3	758	498	0.02%	0.003%
42	6.513	1699	1702	1707	rVB4	666	648	0.03%	0.003%
43	6.548	1710	1713	1715	rVB	761	347	0.01%	0.002%
44	6.564	1716	1718	1719	rBV	373	156	0.01%	0.001%
45	6.574	1719	1721	1723	rBV2	474	248	0.01%	0.001%
46	6.641	1738	1742	1743	rBV2	1249	810	0.03%	0.004%
47	6.738	1768	1772	1775	rBV5	655	473	0.02%	0.003%
48	6.809	1791	1794	1797	rBV3	787	489	0.02%	0.003%
49	6.879	1809	1816	1817	rBV2	608	472	0.02%	0.003%
50	6.989	1839	1850	1870	rBV2	288572	525892	21.97%	2.821%
51	7.191	1910	1913	1915	rBV3	1322	813	0.03%	0.004%
52	7.320	1941	1953	1988	rBV	1051601	1820424	76.05%	9.764%
53	7.625	2038	2048	2069	rBV	207700	367277	15.34%	1.970%
54	7.908	2129	2136	2137	rBV3	1239	1268	0.05%	0.007%
55	8.040	2175	2177	2180	rBV2	919	686	0.03%	0.004%
56	8.091	2183	2193	2230	rBV	575274	1064894	44.49%	5.711%
57	8.670	2370	2373	2375	rBV3	763	561	0.02%	0.003%
58	8.731	2389	2392	2393	rBV2	784	431	0.02%	0.002%
59	8.776	2405	2406	2410	rVB2	580	325	0.01%	0.002%
60	8.796	2410	2412	2416	rVB2	696	371	0.02%	0.002%
61	8.857	2416	2431	2450	rBV	1198157	1925982	80.46%	10.330%
62	9.114	2509	2511	2514	rBV3	1419	730	0.03%	0.004%
63	9.146	2514	2521	2527	rVV6	1677	2689	0.11%	0.014%
64	9.439	2608	2612	2616	rVB3	571	510	0.02%	0.003%
65	9.461	2616	2619	2622	rBV2	561	407	0.02%	0.002%
66	9.500	2629	2631	2634	rBV3	425	223	0.01%	0.001%
67	9.551	2641	2647	2648	rBV3	1290	985	0.04%	0.005%
68	9.593	2658	2660	2663	rVB3	639	290	0.01%	0.002%
69	9.632	2666	2672	2674	rBV5	1108	1019	0.04%	0.005%
70	9.693	2689	2691	2693	rBV2	549	253	0.01%	0.001%
71	9.767	2712	2714	2717	rBV	686	468	0.02%	0.003%
72	9.805	2722	2726	2727	rBV2	936	631	0.03%	0.003%
73	9.873	2744	2747	2751	rBV4	1076	818	0.03%	0.004%
74	9.911	2756	2759	2761	rBV2	668	350	0.01%	0.002%
75	9.979	2778	2780	2787	rVB5	890	713	0.03%	0.004%
76	10.011	2787	2790	2791	rBV	715	370	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020749.D
 Acq On : 26 Mar 2021 12:13
 Operator : SY/MD
 Sample : M1816-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3H6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

77	10.034	2795	2797	2799	rBV	665	358	0.01%	0.002%
78	10.127	2820	2826	2830	rBV5	798	923	0.04%	0.005%
79	10.156	2832	2835	2836	rBV	493	287	0.01%	0.002%
80	10.220	2843	2855	2876	rBV	746098	1184651	49.49%	6.354%
81	10.390	2898	2908	2921	rVB5	7504	12735	0.53%	0.068%
82	10.442	2921	2924	2926	rBV2	1231	592	0.02%	0.003%
83	10.516	2945	2947	2954	rVB4	882	826	0.03%	0.004%
84	10.545	2954	2956	2958	rBV2	1034	595	0.02%	0.003%
85	10.667	2989	2994	2997	rVB3	756	603	0.03%	0.003%
86	10.763	3021	3024	3026	rBV2	477	305	0.01%	0.002%
87	10.834	3043	3046	3047	rBV	872	502	0.02%	0.003%
88	10.857	3051	3053	3055	rBV3	868	416	0.02%	0.002%
89	11.255	3165	3177	3198	rBV	1210709	1871373	78.18%	10.037%
90	11.548	3262	3268	3272	rBV6	1382	1741	0.07%	0.009%
91	11.583	3277	3279	3281	rBV3	691	284	0.01%	0.002%
92	11.632	3282	3294	3314	rBV	1192634	1863184	77.84%	9.993%
93	12.133	3447	3450	3453	rBV4	1187	686	0.03%	0.004%
94	12.513	3565	3568	3571	rBV2	867	521	0.02%	0.003%
95	12.943	3700	3702	3705	rBV3	746	424	0.02%	0.002%
96	13.149	3764	3766	3770	rBV2	885	791	0.03%	0.004%
97	13.275	3802	3805	3809	rBV3	1348	1115	0.05%	0.006%
98	13.525	3877	3883	3885	rBV4	1306	1352	0.06%	0.007%
99	13.570	3894	3897	3904	rBV3	1390	1843	0.08%	0.010%
100	13.844	3980	3982	3986	rVB	1293	661	0.03%	0.004%




Sum of corrected areas: 18644994

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020749.D
Acq On : 26 Mar 2021 12:13
Operator : SY/MD
Sample : M1816-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3H6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

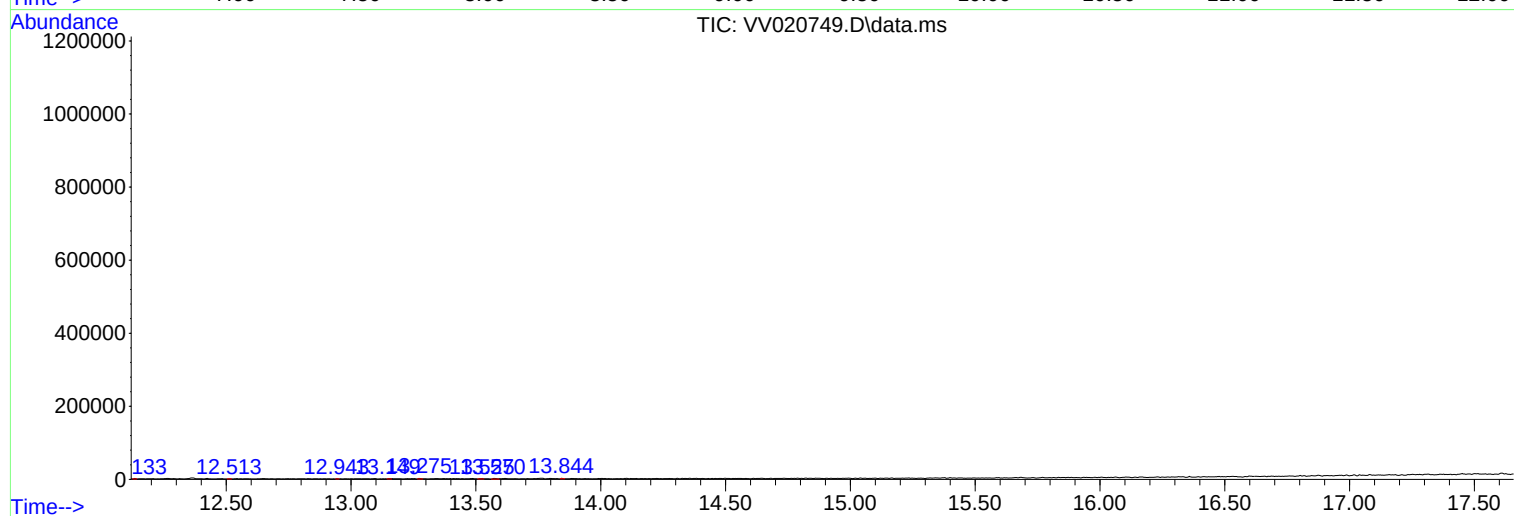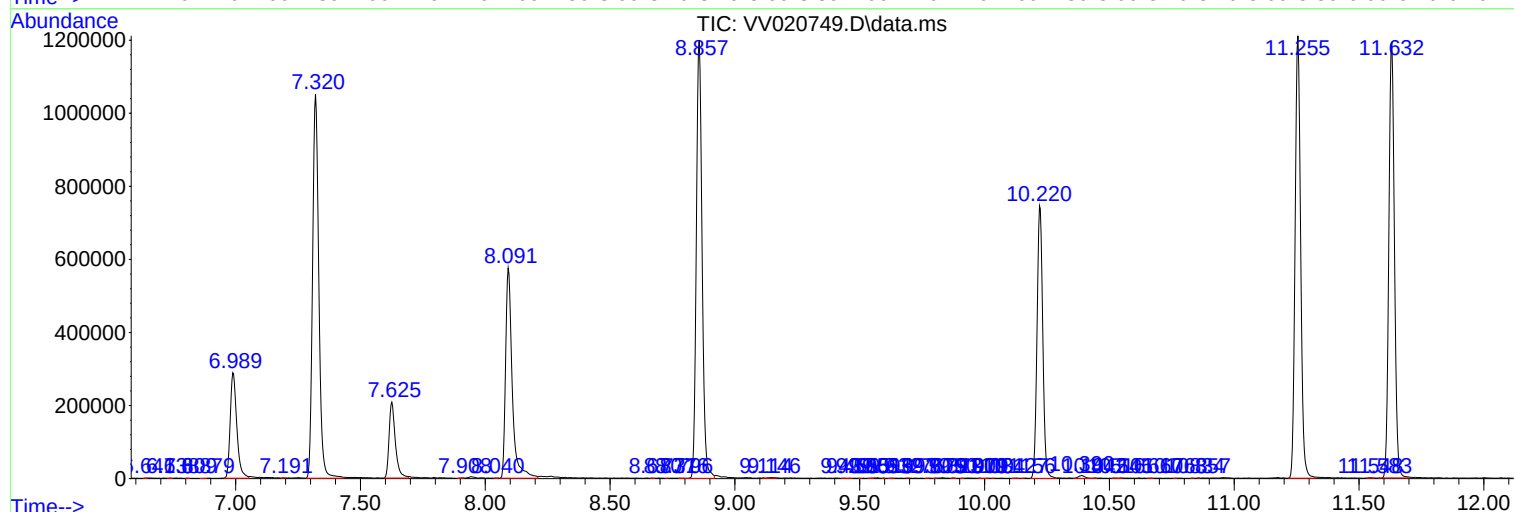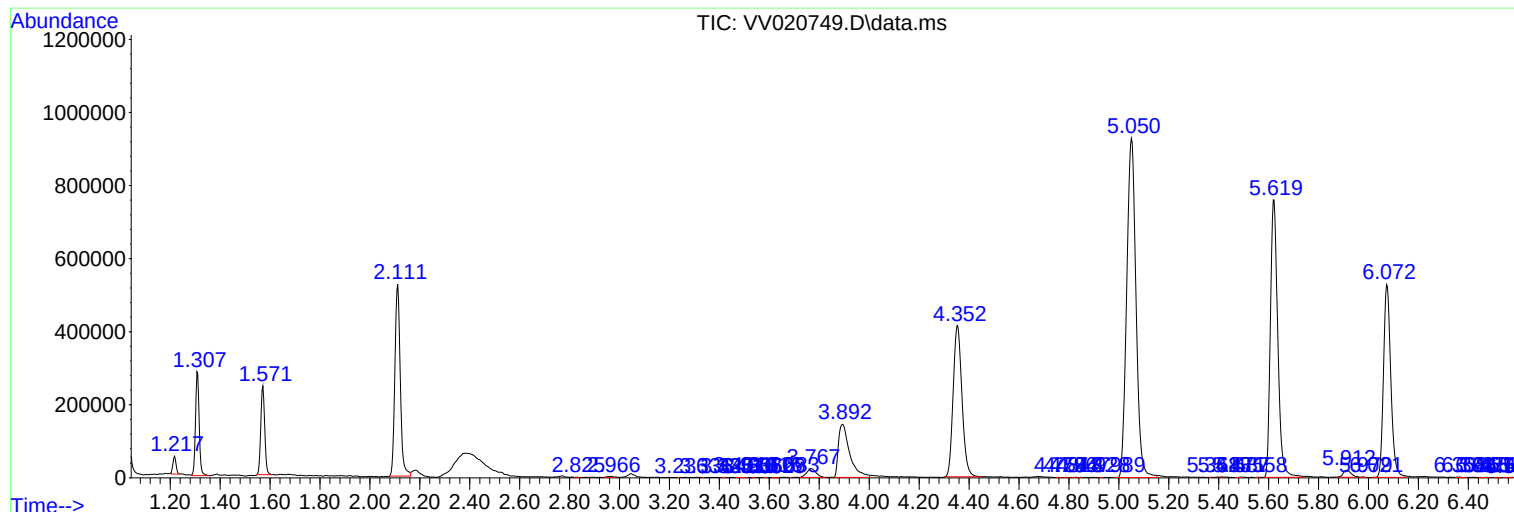

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020749.D
Acq On : 26 Mar 2021 12:13
Operator : SY/MD
Sample : M1816-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3H6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020749.D
Acq On : 26 Mar 2021 12:13
Operator : SY/MD
Sample : M1816-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3H6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------