

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020756.D
 Acq On : 26 Mar 2021 14:58
 Operator : SY/MD
 Sample : M1781-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020756.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	100	rVB	355911	355319	13.23%	1.713%
2	1.571	158	165	180	rVB	283220	314966	11.73%	1.519%
3	2.111	322	333	354	rBV	636409	950743	35.41%	4.585%
4	2.266	377	381	386	rVB4	932	720	0.03%	0.003%
5	2.291	386	389	390	rBV2	574	333	0.01%	0.002%
6	2.349	401	407	411	rVB2	924	765	0.03%	0.004%
7	2.446	435	437	439	rBV2	578	314	0.01%	0.002%
8	2.513	447	458	467	rBV9	3697	7005	0.26%	0.034%
9	2.667	504	506	511	rVV2	657	426	0.02%	0.002%
10	2.687	511	512	515	rVB2	609	274	0.01%	0.001%
11	2.767	535	537	540	rBV2	660	399	0.01%	0.002%
12	2.806	547	549	553	rVB2	559	317	0.01%	0.002%
13	2.831	553	557	558	rBV	670	392	0.01%	0.002%
14	2.873	566	570	571	rBV3	564	365	0.01%	0.002%
15	2.902	574	579	581	rBV	889	621	0.02%	0.003%
16	2.941	587	591	593	rBV	417	336	0.01%	0.002%
17	3.008	608	612	613	rBV2	494	437	0.02%	0.002%
18	3.069	629	631	634	rBV2	628	295	0.01%	0.001%
19	3.102	638	641	646	rVB3	503	360	0.01%	0.002%
20	3.127	646	649	652	rBV2	485	308	0.01%	0.001%
21	3.156	656	658	660	rBV2	483	255	0.01%	0.001%
22	3.233	681	682	687	rVB	564	379	0.01%	0.002%
23	3.291	697	700	702	rVV	532	276	0.01%	0.001%
24	3.497	761	764	766	rBV	569	261	0.01%	0.001%
25	3.548	777	780	782	rBV	755	469	0.02%	0.002%
26	3.674	817	819	823	rBV2	550	395	0.01%	0.002%
27	3.729	833	836	838	rBV	512	330	0.01%	0.002%
28	3.757	842	845	850	rBV3	849	730	0.03%	0.004%
29	3.819	861	864	867	rVV3	545	346	0.01%	0.002%
30	3.889	874	886	927	rBV	170792	504760	18.80%	2.434%
31	4.253	997	999	1001	rVB2	774	300	0.01%	0.001%
32	4.352	1014	1030	1061	rBV	461876	1135226	42.28%	5.474%
33	4.828	1175	1178	1179	rBV	898	495	0.02%	0.002%
34	4.864	1187	1189	1192	rVB	637	300	0.01%	0.001%
35	4.963	1218	1220	1221	rBV	570	289	0.01%	0.001%
36	5.050	1229	1247	1276	rBV2	1039681	2684955	100.00%	12.948%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020756.D
 Acq On : 26 Mar 2021 14:58
 Operator : SY/MD
 Sample : M1781-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

37	5.471	1376	1378	1380	rBV2	532	263	0.01%	0.001%
38	5.519	1391	1393	1396	rVB2	923	368	0.01%	0.002%
39	5.539	1397	1399	1401	rVV3	736	267	0.01%	0.001%
40	5.619	1411	1424	1458	rBV	846091	1701107	63.36%	8.203%
41	6.072	1551	1565	1596	rBV	578858	1186083	44.18%	5.720%
42	6.320	1637	1642	1650	rBV6	1046	1251	0.05%	0.006%
43	6.378	1658	1660	1662	rBV2	807	471	0.02%	0.002%
44	6.410	1668	1670	1674	rVB4	663	441	0.02%	0.002%
45	6.471	1684	1689	1690	rBV2	641	530	0.02%	0.003%
46	6.490	1694	1695	1699	rVB2	835	325	0.01%	0.002%
47	6.683	1752	1755	1759	rBV3	629	609	0.02%	0.003%
48	6.777	1781	1784	1786	rBV2	496	273	0.01%	0.001%
49	6.806	1791	1793	1797	rVB2	680	402	0.01%	0.002%
50	6.838	1799	1803	1808	rVB4	516	481	0.02%	0.002%
51	6.860	1808	1810	1813	rBV4	400	251	0.01%	0.001%
52	6.902	1819	1823	1824	rBV	611	404	0.02%	0.002%
53	6.989	1836	1850	1875	rBV	323963	605843	22.56%	2.922%
54	7.259	1932	1934	1936	rBV3	728	373	0.01%	0.002%
55	7.320	1941	1953	1982	rBV	1236816	2133452	79.46%	10.288%
56	7.571	2029	2031	2033	rBV2	716	408	0.02%	0.002%
57	7.625	2038	2048	2066	rBV	240774	409684	15.26%	1.976%
58	8.092	2183	2193	2230	rBV	666766	1179535	43.93%	5.688%
59	8.452	2303	2305	2310	rBV5	956	703	0.03%	0.003%
60	8.506	2319	2322	2326	rVB3	1038	705	0.03%	0.003%
61	8.674	2370	2374	2375	rBV3	814	580	0.02%	0.003%
62	8.751	2396	2398	2401	rBV3	868	442	0.02%	0.002%
63	8.786	2407	2409	2413	rBV5	851	555	0.02%	0.003%
64	8.857	2419	2431	2456	rBV	1329185	2113609	78.72%	10.193%
65	9.394	2596	2598	2600	rBV	391	241	0.01%	0.001%
66	9.484	2622	2626	2628	rBV3	900	607	0.02%	0.003%
67	9.555	2644	2648	2651	rBV2	1097	778	0.03%	0.004%
68	9.622	2667	2669	2672	rBV3	602	323	0.01%	0.002%
69	9.667	2678	2683	2684	rBV4	537	451	0.02%	0.002%
70	9.712	2693	2697	2699	rBV	536	421	0.02%	0.002%
71	9.783	2717	2719	2721	rBV2	595	327	0.01%	0.002%
72	9.796	2721	2723	2726	rVV2	595	347	0.01%	0.002%
73	9.844	2736	2738	2741	rBV2	507	285	0.01%	0.001%
74	9.928	2759	2764	2767	rBV3	818	762	0.03%	0.004%
75	10.220	2843	2855	2878	rBV	830793	1308056	48.72%	6.308%
76	10.420	2914	2917	2921	rBV2	583	422	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020756.D
 Acq On : 26 Mar 2021 14:58
 Operator : SY/MD
 Sample : M1781-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

77	10.439	2921	2923	2927	rBV3	1055	740	0.03%	0.004%
78	10.506	2942	2944	2948	rBV3	648	436	0.02%	0.002%
79	10.529	2948	2951	2953	rBV2	551	272	0.01%	0.001%
80	10.584	2965	2968	2973	rBV3	1166	1014	0.04%	0.005%
81	10.674	2993	2996	2998	rBV3	742	409	0.02%	0.002%
82	10.686	2998	3000	3003	rVB3	666	255	0.01%	0.001%
83	10.715	3007	3009	3013	rVB3	523	292	0.01%	0.001%
84	11.101	3126	3129	3130	rVB	541	244	0.01%	0.001%
85	11.117	3130	3134	3138	rBV3	771	649	0.02%	0.003%
86	11.169	3147	3150	3153	rBV2	1115	956	0.04%	0.005%
87	11.182	3153	3154	3156	rVV	726	310	0.01%	0.001%
88	11.256	3165	3177	3207	rBV	1335360	2057795	76.64%	9.923%
89	11.532	3261	3263	3268	rVB3	935	500	0.02%	0.002%
90	11.632	3281	3294	3314	rBV	1302790	2045668	76.19%	9.865%
91	12.120	3443	3446	3450	rVB3	589	416	0.02%	0.002%
92	12.288	3496	3498	3502	rBV3	738	489	0.02%	0.002%
93	12.320	3506	3508	3511	rBV	687	250	0.01%	0.001%
94	12.445	3545	3547	3549	rBV2	817	438	0.02%	0.002%
95	12.616	3596	3600	3601	rBV2	893	661	0.02%	0.003%
96	13.095	3748	3749	3750	rBV	955	242	0.01%	0.001%
97	13.207	3783	3784	3787	rBV2	670	288	0.01%	0.001%
98	13.329	3819	3822	3825	rBV3	1035	709	0.03%	0.003%
99	13.577	3896	3899	3903	rBV4	784	739	0.03%	0.004%
100	15.448	4478	4481	4490	rVB	8024	6136	0.23%	0.030%




Sum of corrected areas: 20736804

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020756.D
Acq On : 26 Mar 2021 14:58
Operator : SY/MD
Sample : M1781-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

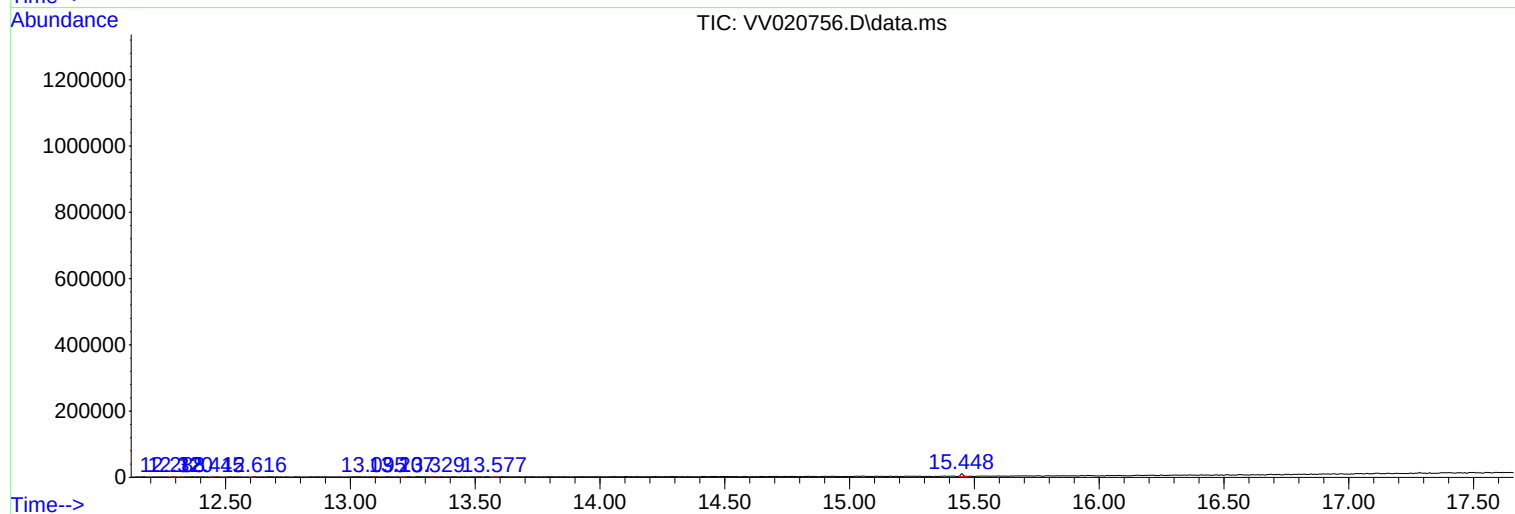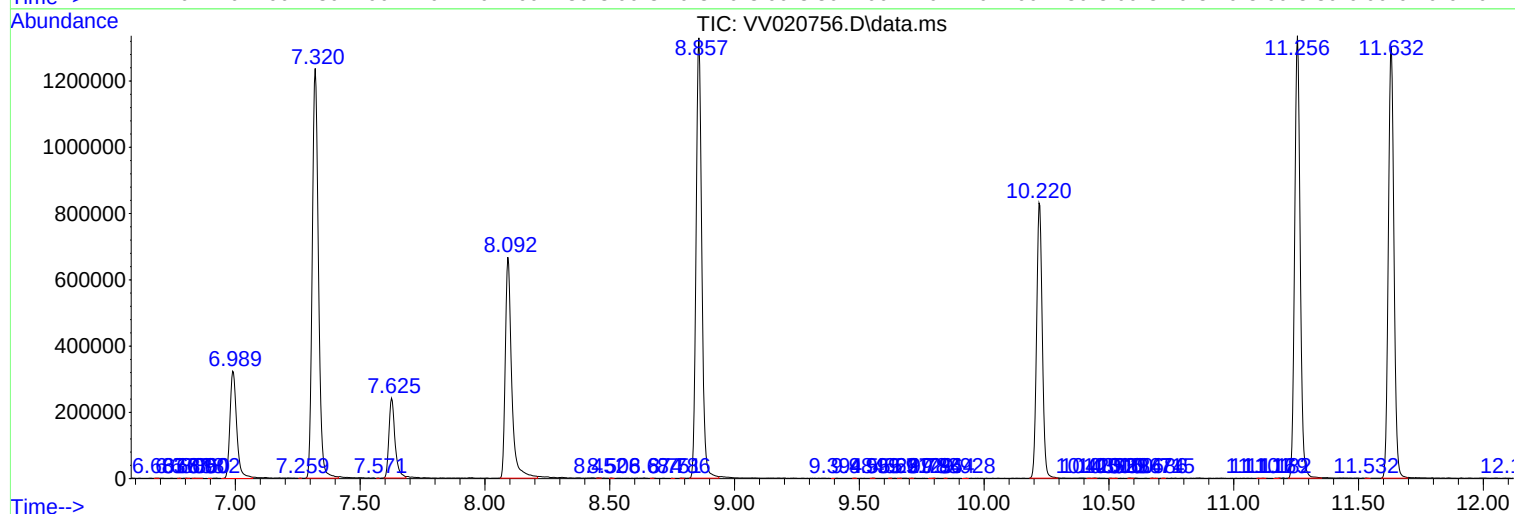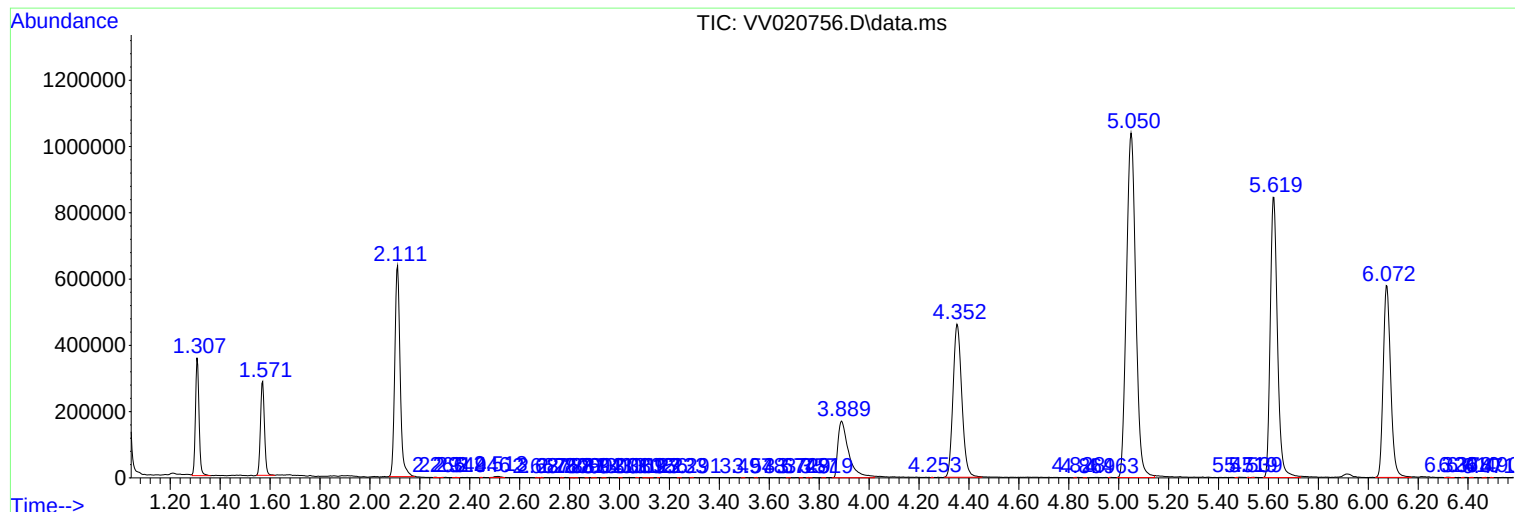

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020756.D
Acq On : 26 Mar 2021 14:58
Operator : SY/MD
Sample : M1781-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020756.D
Acq On : 26 Mar 2021 14:58
Operator : SY/MD
Sample : M1781-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
