

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020757.D
 Acq On : 26 Mar 2021 15:22
 Operator : SY/MD
 Sample : M1784-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4W4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020757.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	98	rVB	282727	282302	11.98%	1.537%
2	1.571	157	165	176	rBV	237536	266672	11.32%	1.452%
3	2.108	323	332	366	rVB	517037	794445	33.73%	4.325%
4	2.574	475	477	480	rBV2	847	531	0.02%	0.003%
5	2.590	480	482	485	rVV3	737	388	0.02%	0.002%
6	2.671	505	507	508	rBV2	674	228	0.01%	0.001%
7	2.719	519	522	524	rVB2	429	192	0.01%	0.001%
8	2.745	527	530	532	rBV3	607	337	0.01%	0.002%
9	2.793	543	545	548	rBV2	464	266	0.01%	0.001%
10	2.835	556	558	560	rBV2	649	364	0.02%	0.002%
11	2.905	578	580	582	rBV	432	194	0.01%	0.001%
12	2.915	582	583	585	rVV	573	221	0.01%	0.001%
13	3.005	609	611	613	rBV	495	225	0.01%	0.001%
14	3.066	628	630	635	rBV3	352	278	0.01%	0.002%
15	3.098	638	640	641	rBV	471	151	0.01%	0.001%
16	3.108	641	643	650	rVB5	532	340	0.01%	0.002%
17	3.140	650	653	654	rBV	476	251	0.01%	0.001%
18	3.198	668	671	675	rBV2	639	546	0.02%	0.003%
19	3.237	678	683	687	rBV2	596	627	0.03%	0.003%
20	3.259	687	690	697	rBV3	316	398	0.02%	0.002%
21	3.288	697	699	701	rBV2	382	163	0.01%	0.001%
22	3.323	706	710	711	rBV3	572	356	0.02%	0.002%
23	3.349	715	718	719	rBV	291	156	0.01%	0.001%
24	3.381	726	728	731	rBV	221	120	0.01%	0.001%
25	3.468	752	755	757	rBV3	466	327	0.01%	0.002%
26	3.510	762	768	774	rVB3	481	636	0.03%	0.003%
27	3.539	774	777	778	rBV2	336	218	0.01%	0.001%
28	3.548	778	780	783	rBV	327	238	0.01%	0.001%
29	3.574	787	788	792	rBV2	439	279	0.01%	0.002%
30	3.712	830	831	835	rVB	441	193	0.01%	0.001%
31	3.738	835	839	842	rBV	484	325	0.01%	0.002%
32	3.793	854	856	858	rBV	246	110	0.00%	0.001%
33	3.806	858	860	861	rVV	292	102	0.00%	0.001%
34	3.892	875	887	924	rBV2	167163	522847	22.20%	2.846%
35	4.352	1012	1030	1053	rBV	411880	1019011	43.26%	5.547%
36	4.786	1161	1165	1167	rBV3	750	464	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020757.D
 Acq On : 26 Mar 2021 15:22
 Operator : SY/MD
 Sample : M1784-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4W4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	4.815	1171	1174	1178	rBV3	394	349	0.01%	0.002%
38	4.835	1178	1180	1183	rBV3	590	381	0.02%	0.002%
39	4.899	1198	1200	1203	rVB2	693	338	0.01%	0.002%
40	4.915	1203	1205	1207	rBV	864	420	0.02%	0.002%
41	4.989	1226	1228	1230	rBV2	511	314	0.01%	0.002%
42	5.050	1230	1247	1279	rVV2	905248	2355495	100.00%	12.822%
43	5.478	1377	1380	1382	rBV3	898	622	0.03%	0.003%
44	5.622	1411	1425	1450	rBV	734369	1476866	62.70%	8.039%
45	5.912	1506	1515	1530	rVB4	20534	41167	1.75%	0.224%
46	6.024	1546	1550	1552	rBV3	1106	748	0.03%	0.004%
47	6.072	1552	1565	1588	rBV	527118	1068635	45.37%	5.817%
48	6.278	1627	1629	1635	rVB4	1211	810	0.03%	0.004%
49	6.426	1671	1675	1676	rBV	1112	672	0.03%	0.004%
50	6.516	1700	1703	1707	rVB2	653	431	0.02%	0.002%
51	6.539	1707	1710	1713	rBV3	581	390	0.02%	0.002%
52	6.558	1713	1716	1718	rBV2	550	364	0.02%	0.002%
53	6.773	1778	1783	1786	rBV5	829	776	0.03%	0.004%
54	6.796	1788	1790	1793	rBV4	870	493	0.02%	0.003%
55	6.838	1799	1803	1804	rBV3	804	466	0.02%	0.003%
56	6.924	1828	1830	1834	rVB3	691	325	0.01%	0.002%
57	6.989	1837	1850	1880	rBV	286466	534049	22.67%	2.907%
58	7.320	1941	1953	1983	rBV	1037320	1809044	76.80%	9.847%
59	7.625	2038	2048	2064	rBV	209437	361570	15.35%	1.968%
60	8.037	2171	2176	2182	rVB5	864	1006	0.04%	0.005%
61	8.092	2182	2193	2231	rBV	621715	1132408	48.08%	6.164%
62	8.616	2352	2356	2359	rBV4	855	590	0.03%	0.003%
63	8.731	2388	2392	2394	rBV2	1060	692	0.03%	0.004%
64	8.857	2418	2431	2460	rBV	1146978	1843450	78.26%	10.035%
65	9.108	2505	2509	2513	rBV4	1174	1029	0.04%	0.006%
66	9.133	2515	2517	2520	rVV	805	349	0.01%	0.002%
67	9.220	2542	2544	2546	rBV2	728	378	0.02%	0.002%
68	9.313	2571	2573	2576	rBV2	490	287	0.01%	0.002%
69	9.365	2585	2589	2593	rBV4	922	749	0.03%	0.004%
70	9.394	2596	2598	2599	rBV	393	130	0.01%	0.001%
71	9.567	2650	2652	2653	rBV	773	351	0.01%	0.002%
72	9.593	2658	2660	2662	rBV	401	220	0.01%	0.001%
73	9.612	2663	2666	2668	rVB2	790	388	0.02%	0.002%
74	9.783	2717	2719	2724	rBV3	663	632	0.03%	0.003%
75	9.828	2732	2733	2735	rBV3	311	107	0.00%	0.001%
76	9.844	2735	2738	2739	rBV3	666	382	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020757.D
 Acq On : 26 Mar 2021 15:22
 Operator : SY/MD
 Sample : M1784-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4W4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

77	9.895	2751	2754	2760	rVB3	693	503	0.02%	0.003%
78	9.998	2779	2786	2789	rBV3	857	1005	0.04%	0.005%
79	10.063	2804	2806	2807	rBV	381	173	0.01%	0.001%
80	10.104	2817	2819	2821	rBV	403	228	0.01%	0.001%
81	10.117	2821	2823	2826	rVB2	664	281	0.01%	0.002%
82	10.172	2838	2840	2842	rBV	463	233	0.01%	0.001%
83	10.220	2842	2855	2878	rBV	765916	1207073	51.24%	6.571%
84	10.323	2884	2887	2889	rBV3	1017	607	0.03%	0.003%
85	10.657	2988	2991	2994	rVB3	911	568	0.02%	0.003%
86	10.719	3008	3010	3015	rBV3	745	467	0.02%	0.003%
87	10.850	3048	3051	3053	rBV2	964	763	0.03%	0.004%
88	11.050	3111	3113	3114	rBV	399	152	0.01%	0.001%
89	11.088	3122	3125	3128	rBV2	827	556	0.02%	0.003%
90	11.165	3143	3149	3151	rBV3	936	1061	0.05%	0.006%
91	11.255	3165	3177	3201	rBV	1140627	1781784	75.64%	9.699%
92	11.632	3282	3294	3320	rBV	1160060	1837747	78.02%	10.004%
93	11.879	3369	3371	3374	rBV2	836	621	0.03%	0.003%
94	11.963	3395	3397	3401	rBV2	738	436	0.02%	0.002%
95	12.040	3417	3421	3422	rBV2	770	560	0.02%	0.003%
96	12.252	3482	3487	3489	rBV4	742	699	0.03%	0.004%
97	12.342	3513	3515	3519	rVB3	756	519	0.02%	0.003%
98	12.661	3610	3614	3617	rBV3	955	850	0.04%	0.005%
99	12.789	3652	3654	3657	rBV2	1174	618	0.03%	0.003%
100	12.905	3685	3690	3693	rBV3	944	846	0.04%	0.005%




Sum of corrected areas: 18370724

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020757.D
Acq On : 26 Mar 2021 15:22
Operator : SY/MD
Sample : M1784-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4W4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

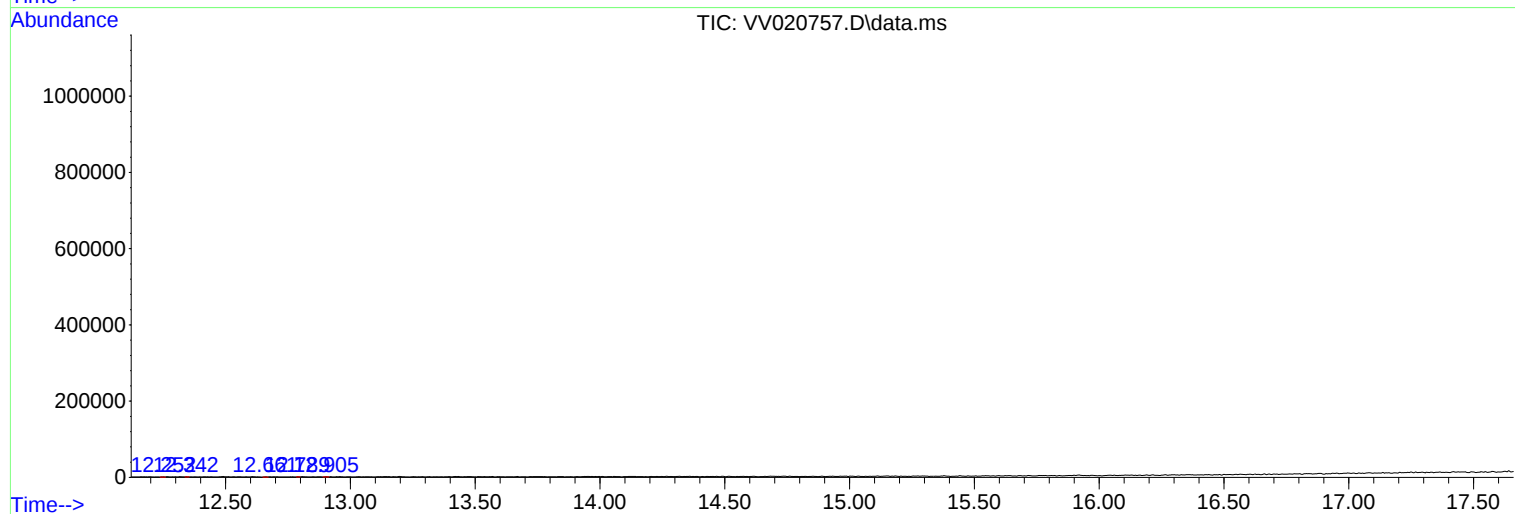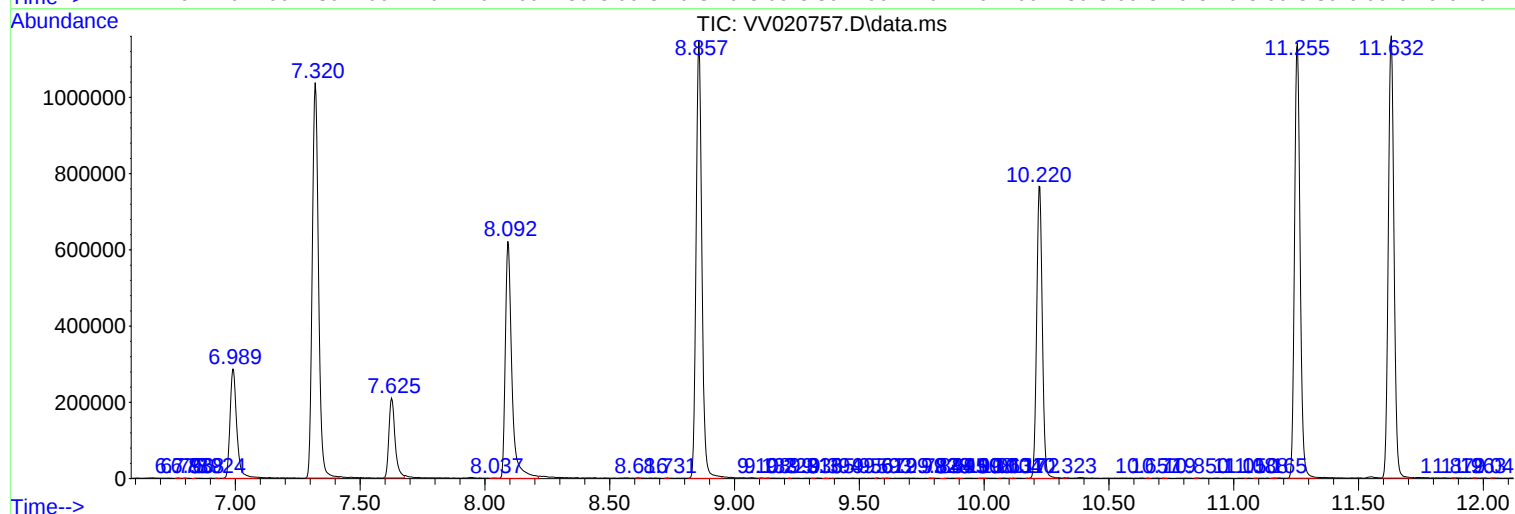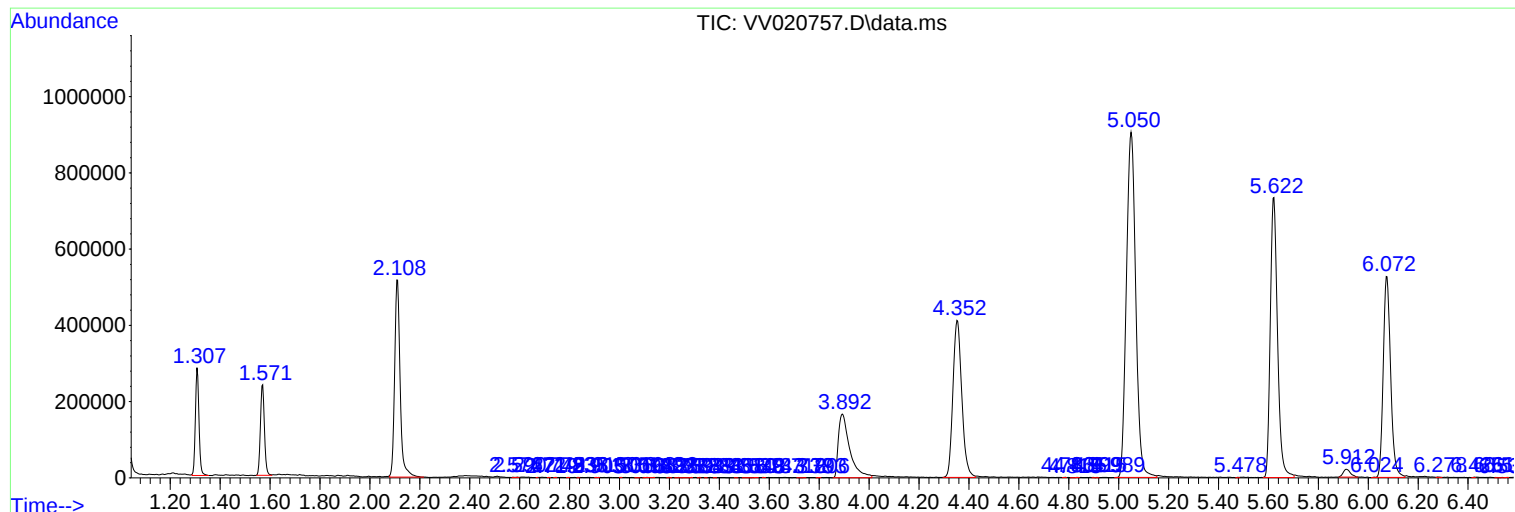

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020757.D
Acq On : 26 Mar 2021 15:22
Operator : SY/MD
Sample : M1784-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4W4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020757.D
Acq On : 26 Mar 2021 15:22
Operator : SY/MD
Sample : M1784-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4W4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
