

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020760.D
 Acq On : 26 Mar 2021 16:32
 Operator : SY/MD
 Sample : M1784-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4X0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020760.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	95	rVB	263306	263828	11.61%	1.447%
2	1.571	158	165	174	rBV	230261	253047	11.13%	1.388%
3	2.111	323	333	367	rVB	497453	768246	33.80%	4.214%
4	2.587	479	481	483	rBV	641	306	0.01%	0.002%
5	2.625	491	493	496	rVB2	732	356	0.02%	0.002%
6	2.715	519	521	526	rVB3	1177	823	0.04%	0.005%
7	2.770	533	538	544	rVV5	964	978	0.04%	0.005%
8	2.828	553	556	559	rBV	509	310	0.01%	0.002%
9	2.844	559	561	562	rVV	444	194	0.01%	0.001%
10	2.863	565	567	569	rBV2	394	210	0.01%	0.001%
11	2.918	582	584	588	rVB2	330	233	0.01%	0.001%
12	2.941	588	591	593	rBV2	336	207	0.01%	0.001%
13	2.953	593	595	600	rBV3	440	434	0.02%	0.002%
14	3.002	608	610	613	rBV3	387	187	0.01%	0.001%
15	3.034	618	620	622	rBV	453	220	0.01%	0.001%
16	3.156	656	658	661	rVB3	751	417	0.02%	0.002%
17	3.198	668	671	677	rVV3	994	646	0.03%	0.004%
18	3.317	707	708	711	rBV	306	187	0.01%	0.001%
19	3.378	722	727	730	rBV3	474	503	0.02%	0.003%
20	3.497	761	764	767	rBV	640	427	0.02%	0.002%
21	3.516	767	770	773	rVV	576	353	0.02%	0.002%
22	3.539	773	777	779	rVB	465	287	0.01%	0.002%
23	3.551	779	781	785	rBV	552	358	0.02%	0.002%
24	3.635	804	807	809	rBV2	516	279	0.01%	0.002%
25	3.690	820	824	828	rBV2	432	381	0.02%	0.002%
26	3.754	841	844	845	rBV2	549	362	0.02%	0.002%
27	3.892	874	887	923	rBV2	151218	465046	20.46%	2.551%
28	4.352	1011	1030	1062	rBV	398074	995311	43.79%	5.459%
29	4.590	1102	1104	1105	rBV	611	274	0.01%	0.002%
30	4.767	1157	1159	1161	rBV2	384	184	0.01%	0.001%
31	4.834	1178	1180	1184	rBV2	826	478	0.02%	0.003%
32	4.870	1189	1191	1196	rVB3	1198	794	0.03%	0.004%
33	4.889	1196	1197	1200	rVB	575	266	0.01%	0.001%
34	4.905	1200	1202	1204	rVB2	426	202	0.01%	0.001%
35	4.921	1204	1207	1208	rBV3	616	407	0.02%	0.002%
36	4.957	1213	1218	1221	rBV3	821	667	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020760.D
 Acq On : 26 Mar 2021 16:32
 Operator : SY/MD
 Sample : M1784-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4X0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	4.989	1225	1228	1229	rBV2	406	188	0.01%	0.001%
38	5.050	1229	1247	1277	rBV2	880403	2273150	100.00%	12.468%
39	5.500	1385	1387	1389	rVB3	1019	463	0.02%	0.003%
40	5.513	1389	1391	1395	rBV3	359	265	0.01%	0.001%
41	5.567	1404	1408	1411	rVB4	789	497	0.02%	0.003%
42	5.622	1411	1425	1455	rBV	778606	1584838	69.72%	8.693%
43	5.911	1505	1515	1534	rBV3	18368	39496	1.74%	0.217%
44	6.075	1552	1566	1597	rBV	503431	1028052	45.23%	5.639%
45	6.355	1648	1653	1654	rBV3	645	491	0.02%	0.003%
46	6.481	1691	1692	1694	rVB	689	197	0.01%	0.001%
47	6.548	1711	1713	1714	rBV	560	292	0.01%	0.002%
48	6.628	1736	1738	1741	rBV4	557	405	0.02%	0.002%
49	6.731	1768	1770	1774	rVB2	738	412	0.02%	0.002%
50	6.921	1826	1829	1832	rVB2	445	323	0.01%	0.002%
51	6.940	1832	1835	1837	rBV2	383	288	0.01%	0.002%
52	6.992	1837	1851	1874	rBV	277672	510970	22.48%	2.803%
53	7.320	1940	1953	1973	rBV	1005490	1739318	76.52%	9.540%
54	7.625	2038	2048	2073	rBV	201179	352344	15.50%	1.933%
55	7.899	2131	2133	2135	rBV2	764	427	0.02%	0.002%
56	8.040	2173	2177	2179	rBV2	646	554	0.02%	0.003%
57	8.091	2183	2193	2227	rBV	593503	1064917	46.85%	5.841%
58	8.384	2280	2284	2287	rBV5	1449	1136	0.05%	0.006%
59	8.638	2360	2363	2365	rBV2	559	409	0.02%	0.002%
60	8.741	2393	2395	2396	rBV3	700	267	0.01%	0.001%
61	8.805	2410	2415	2419	rBV4	791	945	0.04%	0.005%
62	8.857	2419	2431	2457	rBV	1219245	1971051	86.71%	10.811%
63	9.152	2521	2523	2525	rBV	752	289	0.01%	0.002%
64	9.181	2530	2532	2534	rBV2	566	306	0.01%	0.002%
65	9.554	2645	2648	2649	rBV2	811	382	0.02%	0.002%
66	9.619	2666	2668	2671	rBV2	345	206	0.01%	0.001%
67	9.635	2671	2673	2676	rBV3	464	301	0.01%	0.002%
68	9.693	2687	2691	2695	rBV4	755	681	0.03%	0.004%
69	9.821	2729	2731	2732	rBV	750	370	0.02%	0.002%
70	9.879	2746	2749	2752	rBV3	815	524	0.02%	0.003%
71	9.902	2753	2756	2758	rBV2	611	285	0.01%	0.002%
72	9.976	2777	2779	2781	rBV	554	338	0.01%	0.002%
73	10.030	2793	2796	2797	rBV	519	281	0.01%	0.002%
74	10.146	2830	2832	2833	rBV	755	356	0.02%	0.002%
75	10.223	2843	2856	2879	rBV	743470	1169093	51.43%	6.412%
76	10.487	2934	2938	2939	rBV2	673	484	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020760.D
 Acq On : 26 Mar 2021 16:32
 Operator : SY/MD
 Sample : M1784-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4X0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

77	10.513	2942	2946	2949	rBV3	864	693	0.03%	0.004%
78	10.657	2987	2991	2992	rBV2	515	384	0.02%	0.002%
79	10.689	2998	3001	3006	rBV2	860	902	0.04%	0.005%
80	10.741	3014	3017	3018	rBV2	578	387	0.02%	0.002%
81	10.770	3022	3026	3029	rBV2	786	557	0.02%	0.003%
82	10.818	3037	3041	3043	rBV3	613	418	0.02%	0.002%
83	10.831	3043	3045	3050	rVB2	1070	700	0.03%	0.004%
84	10.863	3051	3055	3057	rBV	1117	770	0.03%	0.004%
85	10.972	3087	3089	3092	rBV2	670	393	0.02%	0.002%
86	10.992	3092	3095	3097	rVV3	710	515	0.02%	0.003%
87	11.014	3100	3102	3110	rVB2	552	509	0.02%	0.003%
88	11.107	3128	3131	3135	rBV2	589	452	0.02%	0.002%
89	11.162	3140	3148	3158	rBV9	4384	8574	0.38%	0.047%
90	11.255	3165	3177	3198	rBV	1214391	1904229	83.77%	10.444%
91	11.631	3282	3294	3316	rBV	1148667	1784768	78.52%	9.789%
92	11.792	3342	3344	3348	rBV2	897	487	0.02%	0.003%
93	11.889	3372	3374	3376	rBV3	723	381	0.02%	0.002%
94	11.931	3385	3387	3389	rBV2	742	383	0.02%	0.002%
95	12.117	3443	3445	3447	rVB2	833	390	0.02%	0.002%
96	12.136	3447	3451	3454	rBV2	606	594	0.03%	0.003%
97	12.358	3512	3520	3529	rBV6	11743	19521	0.86%	0.107%
98	12.799	3653	3657	3659	rBV	844	732	0.03%	0.004%
99	13.091	3743	3748	3750	rBV3	1444	1446	0.06%	0.008%
100	13.464	3861	3864	3868	rBV3	893	790	0.03%	0.004%




Sum of corrected areas: 18231974

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020760.D
Acq On : 26 Mar 2021 16:32
Operator : SY/MD
Sample : M1784-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4X0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

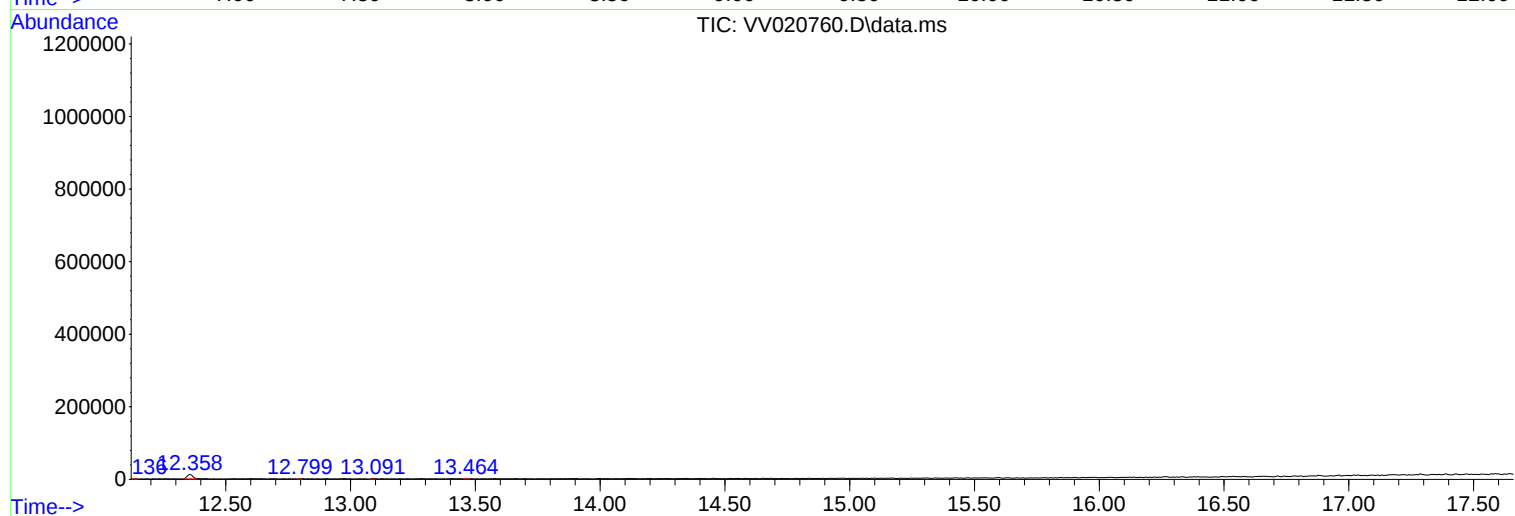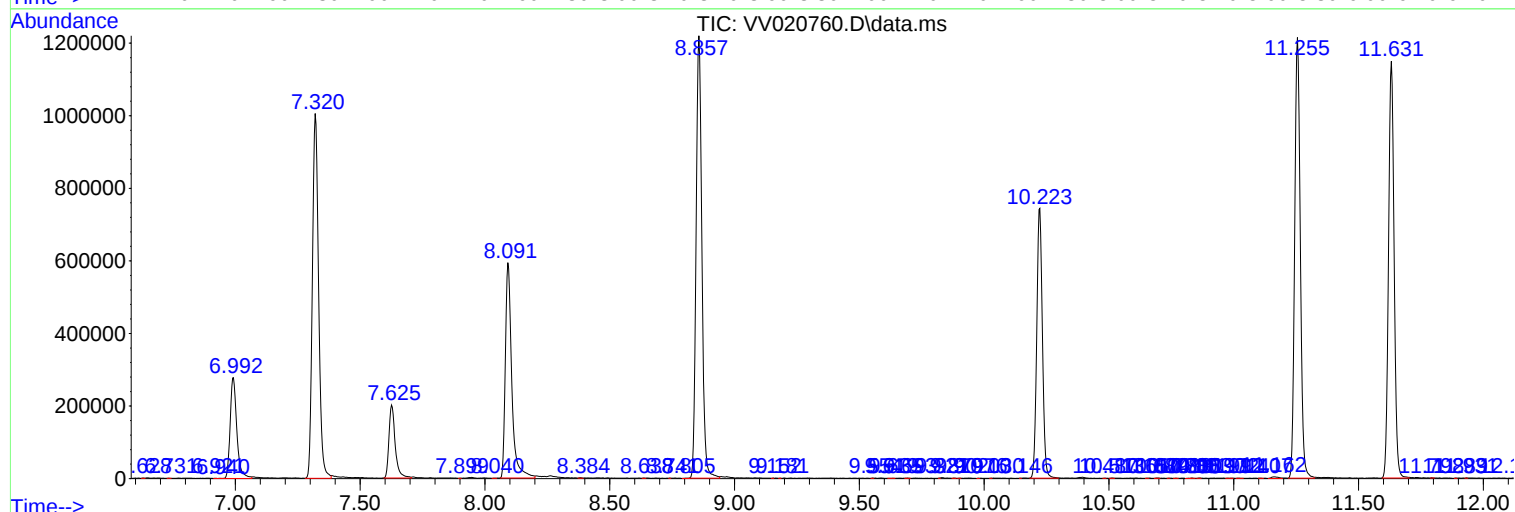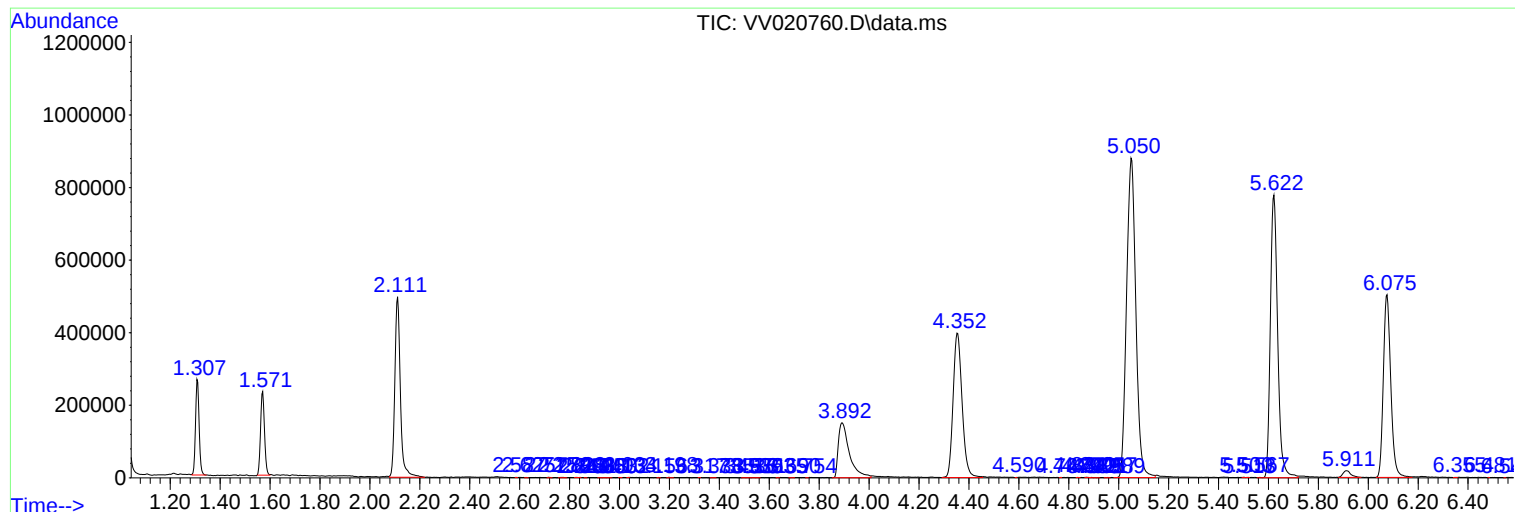

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020760.D
Acq On : 26 Mar 2021 16:32
Operator : SY/MD
Sample : M1784-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4X0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020760.D
Acq On : 26 Mar 2021 16:32
Operator : SY/MD
Sample : M1784-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4X0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------