

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020762.D
 Acq On : 26 Mar 2021 17:20
 Operator : SY/MD
 Sample : M1784-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4R9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020762.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	96	rVB	273997	274253	11.92%	1.489%
2	1.571	158	165	177	rVB	230308	257918	11.21%	1.401%
3	2.111	323	333	369	rVB	493952	765461	33.26%	4.157%
4	2.349	404	407	411	rBV3	1006	1008	0.04%	0.005%
5	2.625	490	493	496	rBV4	1010	785	0.03%	0.004%
6	2.654	500	502	504	rVB	427	166	0.01%	0.001%
7	2.696	513	515	516	rBV	396	123	0.01%	0.001%
8	2.860	565	566	569	rBV2	354	177	0.01%	0.001%
9	2.905	577	580	581	rBV2	439	194	0.01%	0.001%
10	2.931	586	588	590	rBV	188	105	0.00%	0.001%
11	3.021	614	616	620	rVB2	462	294	0.01%	0.002%
12	3.047	621	624	629	rBV4	611	396	0.02%	0.002%
13	3.182	663	666	667	rVB2	572	213	0.01%	0.001%
14	3.194	667	670	674	rBV2	705	581	0.03%	0.003%
15	3.217	676	677	679	rBV	522	212	0.01%	0.001%
16	3.259	688	690	691	rBV2	334	136	0.01%	0.001%
17	3.349	715	718	722	rBV2	531	526	0.02%	0.003%
18	3.371	723	725	727	rBV2	299	133	0.01%	0.001%
19	3.413	736	738	739	rBV2	305	130	0.01%	0.001%
20	3.500	763	765	767	rBV2	694	329	0.01%	0.002%
21	3.532	773	775	781	rBV2	440	320	0.01%	0.002%
22	3.558	781	783	784	rBV	491	166	0.01%	0.001%
23	3.641	807	809	813	rVB2	506	319	0.01%	0.002%
24	3.751	837	843	850	rBV5	968	1299	0.06%	0.007%
25	3.821	863	865	867	rBV	327	163	0.01%	0.001%
26	3.892	876	887	919	rBV2	152141	458207	19.91%	2.489%
27	4.352	1015	1030	1056	rBV	402198	991847	43.10%	5.387%
28	4.754	1152	1155	1161	rVB5	1037	869	0.04%	0.005%
29	4.783	1161	1164	1168	rBV4	958	702	0.03%	0.004%
30	4.802	1168	1170	1174	rVB2	674	350	0.02%	0.002%
31	4.860	1186	1188	1190	rVB2	655	250	0.01%	0.001%
32	4.873	1190	1192	1194	rBV2	649	301	0.01%	0.002%
33	4.889	1194	1197	1200	rBV2	551	349	0.02%	0.002%
34	4.928	1206	1209	1213	rBV3	685	562	0.02%	0.003%
35	4.985	1220	1227	1230	rBV3	773	1059	0.05%	0.006%
36	5.050	1230	1247	1281	rBV2	890780	2301392	100.00%	12.499%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032621\
 Data File : VW020762.D
 Acq On : 26 Mar 2021 17:20
 Operator : SY/MD
 Sample : M1784-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4R9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	5.339	1335	1337	1341	rBV4	1192	1062	0.05%	0.006%
38	5.416	1357	1361	1368	rBV6	1222	1222	0.05%	0.007%
39	5.477	1377	1380	1383	rBV2	916	542	0.02%	0.003%
40	5.493	1383	1385	1387	rVV4	677	269	0.01%	0.001%
41	5.561	1403	1406	1408	rBV2	1066	838	0.04%	0.005%
42	5.622	1411	1425	1455	rBV	784709	1589594	69.07%	8.633%
43	6.072	1552	1565	1591	rBV	504553	1033331	44.90%	5.612%
44	6.378	1656	1660	1662	rBV3	1327	896	0.04%	0.005%
45	6.426	1673	1675	1679	rBV4	872	507	0.02%	0.003%
46	6.497	1695	1697	1699	rBV2	512	285	0.01%	0.002%
47	6.509	1699	1701	1705	rVV4	765	615	0.03%	0.003%
48	6.590	1724	1726	1728	rBV	600	299	0.01%	0.002%
49	6.780	1781	1785	1786	rBV2	723	455	0.02%	0.002%
50	6.815	1793	1796	1800	rVB3	794	591	0.03%	0.003%
51	6.860	1806	1810	1812	rBV2	794	553	0.02%	0.003%
52	6.902	1818	1823	1825	rBV	579	492	0.02%	0.003%
53	6.931	1829	1832	1833	rBV2	607	305	0.01%	0.002%
54	6.989	1839	1850	1870	rBV	280609	515711	22.41%	2.801%
55	7.320	1942	1953	1976	rBV	1006428	1740359	75.62%	9.452%
56	7.625	2037	2048	2070	rBV2	198849	354189	15.39%	1.924%
57	7.979	2153	2158	2160	rBV5	2947	2975	0.13%	0.016%
58	8.056	2179	2182	2183	rBV3	922	448	0.02%	0.002%
59	8.091	2183	2193	2232	rVV	605879	1085453	47.17%	5.895%
60	8.632	2358	2361	2365	rBV4	847	709	0.03%	0.004%
61	8.670	2371	2373	2375	rBV2	660	296	0.01%	0.002%
62	8.718	2385	2388	2394	rBV5	643	771	0.03%	0.004%
63	8.857	2419	2431	2455	rBV	1228665	1986708	86.33%	10.790%
64	9.130	2513	2516	2517	rBV	536	269	0.01%	0.001%
65	9.152	2517	2523	2529	rVV8	2250	2684	0.12%	0.015%
66	9.201	2535	2538	2540	rBV2	727	435	0.02%	0.002%
67	9.242	2548	2551	2554	rBV3	1305	939	0.04%	0.005%
68	9.332	2577	2579	2582	rVB2	643	326	0.01%	0.002%
69	9.368	2588	2590	2593	rBV3	434	233	0.01%	0.001%
70	9.413	2601	2604	2606	rBV3	604	406	0.02%	0.002%
71	9.516	2632	2636	2637	rVB3	662	335	0.01%	0.002%
72	9.525	2637	2639	2640	rBV2	621	229	0.01%	0.001%
73	9.644	2674	2676	2681	rBV2	468	407	0.02%	0.002%
74	9.738	2703	2705	2706	rBV	498	233	0.01%	0.001%
75	9.963	2772	2775	2778	rVB3	1132	672	0.03%	0.004%
76	10.040	2795	2799	2803	rVB4	1170	1061	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020762.D
 Acq On : 26 Mar 2021 17:20
 Operator : SY/MD
 Sample : M1784-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4R9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

77	10.069	2805	2808	2813	rBV4	603	563	0.02%	0.003%
78	10.162	2835	2837	2839	rBV	377	179	0.01%	0.001%
79	10.220	2843	2855	2881	rVV	762436	1203590	52.30%	6.537%
80	10.394	2902	2909	2917	rVB7	3212	5108	0.22%	0.028%
81	10.541	2953	2955	2957	rBV2	476	289	0.01%	0.002%
82	10.558	2957	2960	2963	rVV2	1182	617	0.03%	0.003%
83	10.599	2970	2973	2975	rBV3	959	664	0.03%	0.004%
84	10.654	2989	2990	2991	rBV3	389	114	0.00%	0.001%
85	10.776	3026	3028	3030	rBV	611	378	0.02%	0.002%
86	10.853	3050	3052	3053	rBV	574	241	0.01%	0.001%
87	10.979	3088	3091	3096	rBV3	814	702	0.03%	0.004%
88	11.001	3096	3098	3102	rVV3	757	429	0.02%	0.002%
89	11.104	3124	3130	3137	rBV3	1977	2593	0.11%	0.014%
90	11.133	3137	3139	3140	rVV	919	260	0.01%	0.001%
91	11.162	3140	3148	3160	rVB	6875	12184	0.53%	0.066%
92	11.255	3166	3177	3203	rBV	1278356	1947993	84.64%	10.580%
93	11.480	3245	3247	3248	rBV	558	188	0.01%	0.001%
94	11.631	3282	3294	3313	rBV	1175768	1819034	79.04%	9.879%
95	11.966	3395	3398	3400	rBV2	725	439	0.02%	0.002%
96	12.101	3438	3440	3442	rBV2	825	406	0.02%	0.002%
97	12.355	3511	3519	3532	rBV5	16738	25759	1.12%	0.140%
98	12.783	3650	3652	3658	rBV3	926	619	0.03%	0.003%
99	12.808	3658	3660	3663	rBV	968	615	0.03%	0.003%
100	13.705	3937	3939	3943	rBV3	983	704	0.03%	0.004%




Sum of corrected areas: 18412667

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020762.D
Acq On : 26 Mar 2021 17:20
Operator : SY/MD
Sample : M1784-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4R9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

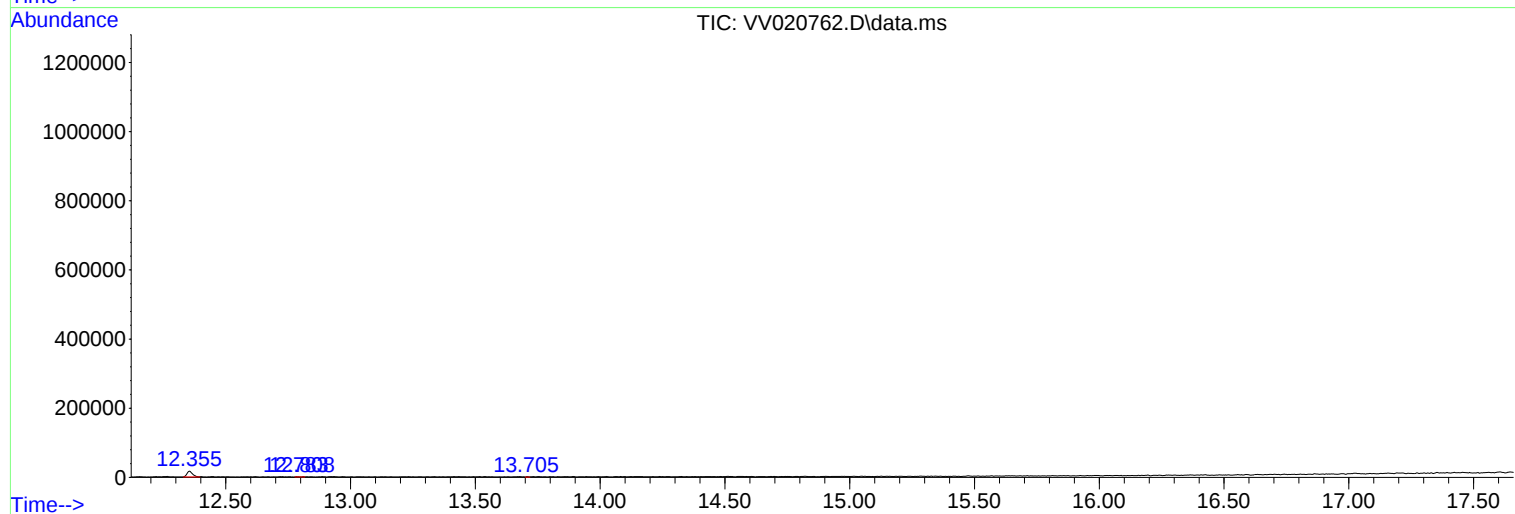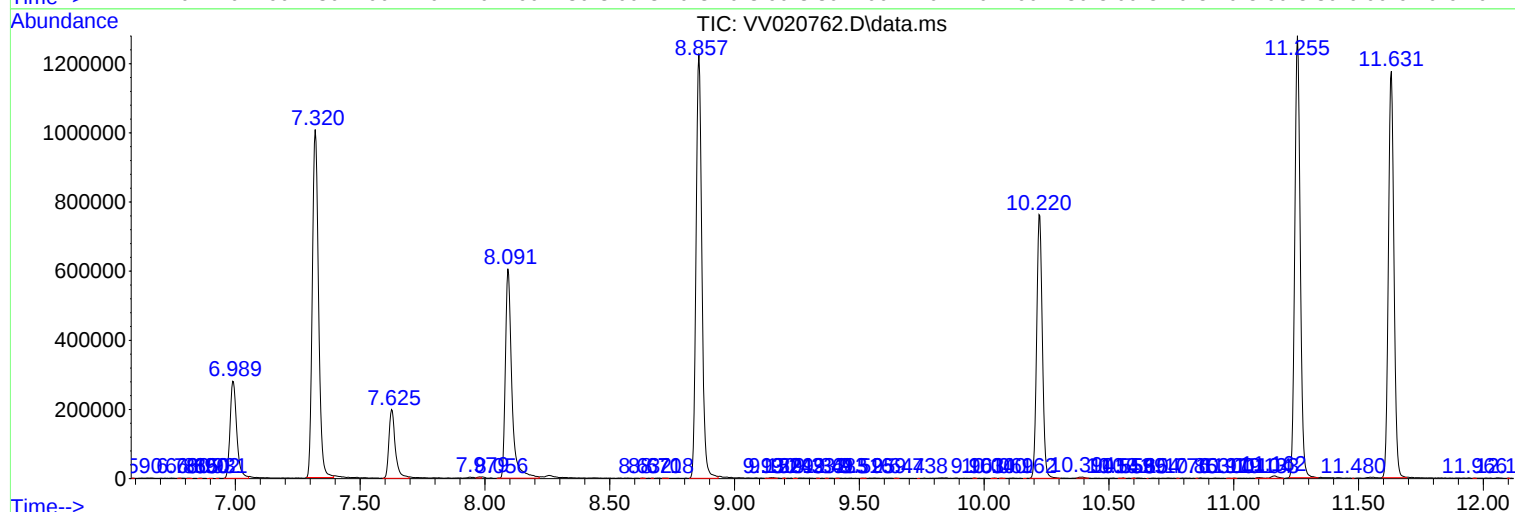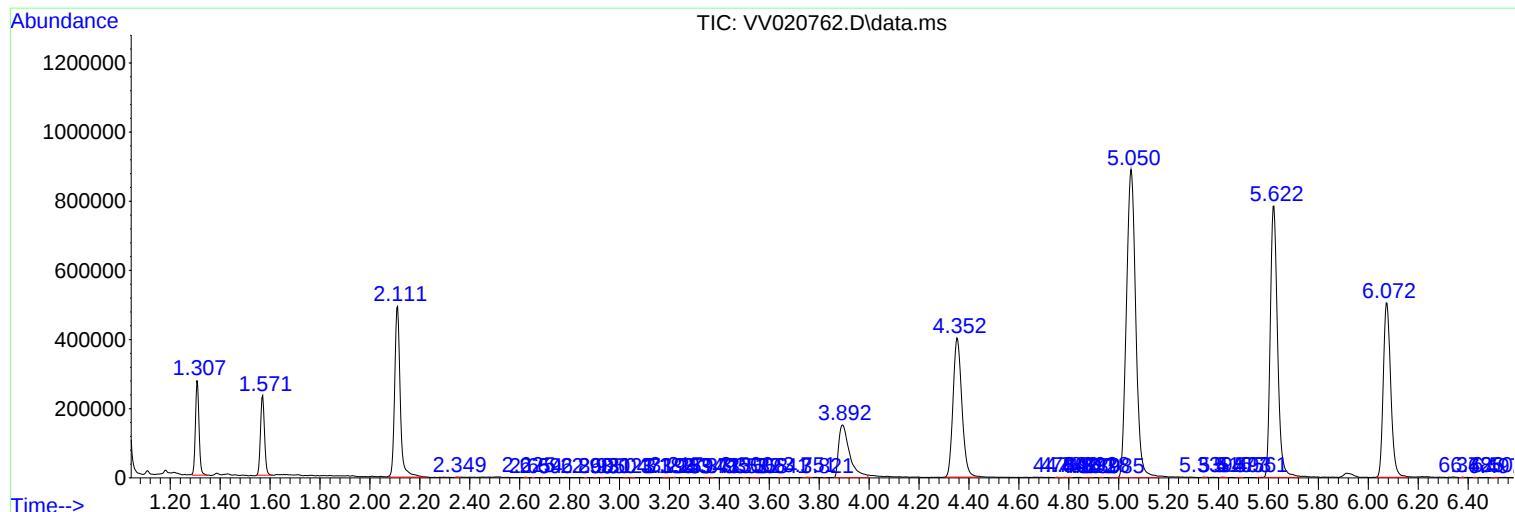

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020762.D
Acq On : 26 Mar 2021 17:20
Operator : SY/MD
Sample : M1784-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4R9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020762.D
Acq On : 26 Mar 2021 17:20
Operator : SY/MD
Sample : M1784-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4R9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
