

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020764.D
 Acq On : 26 Mar 2021 18:07
 Operator : SY/MD
 Sample : M1784-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4S1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020764.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.111	17	22	31	rVB	59604	55032	2.43%	0.301%
2	1.307	77	83	96	rVB	285315	293359	12.96%	1.607%
3	1.571	158	165	176	rVB	225905	249096	11.00%	1.364%
4	2.111	322	333	370	rVB	491987	767952	33.92%	4.206%
5	2.507	452	456	460	rBV4	1770	2099	0.09%	0.011%
6	2.674	507	508	510	rBV	254	142	0.01%	0.001%
7	2.841	558	560	562	rBV2	387	148	0.01%	0.001%
8	2.915	582	583	587	rVB3	491	141	0.01%	0.001%
9	3.002	608	610	611	rBV	474	241	0.01%	0.001%
10	3.044	618	623	632	rVB6	1626	1949	0.09%	0.011%
11	3.105	638	642	643	rBV2	561	432	0.02%	0.002%
12	3.134	649	651	655	rVB2	502	236	0.01%	0.001%
13	3.172	657	663	665	rBV3	504	429	0.02%	0.002%
14	3.208	671	674	675	rBV2	360	245	0.01%	0.001%
15	3.359	719	721	730	rVB5	586	524	0.02%	0.003%
16	3.401	730	734	736	rBV2	447	278	0.01%	0.002%
17	3.417	736	739	741	rBV3	542	319	0.01%	0.002%
18	3.523	770	772	775	rBV	546	331	0.01%	0.002%
19	3.590	789	793	795	rBV	724	449	0.02%	0.002%
20	3.619	799	802	805	rBV	668	391	0.02%	0.002%
21	3.655	811	813	815	rBV	369	169	0.01%	0.001%
22	3.667	815	817	818	rBV2	476	193	0.01%	0.001%
23	3.696	822	826	830	rVB3	576	386	0.02%	0.002%
24	3.728	831	836	837	rBV3	849	685	0.03%	0.004%
25	3.892	876	887	929	rBV	148696	458664	20.26%	2.512%
26	4.285	1005	1009	1013	rBV4	748	620	0.03%	0.003%
27	4.352	1014	1030	1057	rBV2	402719	1002566	44.28%	5.491%
28	4.642	1118	1120	1123	rBV2	1079	688	0.03%	0.004%
29	4.722	1143	1145	1147	rBV2	798	391	0.02%	0.002%
30	4.818	1172	1175	1176	rBV2	889	522	0.02%	0.003%
31	4.886	1194	1196	1198	rBV2	651	354	0.02%	0.002%
32	4.912	1202	1204	1208	rVB3	810	406	0.02%	0.002%
33	4.934	1209	1211	1215	rBV	563	298	0.01%	0.002%
34	4.979	1223	1225	1229	rVB3	844	507	0.02%	0.003%
35	5.050	1229	1247	1272	rBV2	879760	2263939	100.00%	12.399%
36	5.362	1339	1344	1348	rBV3	1101	981	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032621\
 Data File : VW020764.D
 Acq On : 26 Mar 2021 18:07
 Operator : SY/MD
 Sample : M1784-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4S1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	5.507	1386	1389	1391	rBV2	973	623	0.03%	0.003%
38	5.622	1412	1425	1460	rBV	777509	1565108	69.13%	8.571%
39	5.918	1506	1517	1538	rVB8	21685	55188	2.44%	0.302%
40	6.024	1548	1550	1551	rBV	895	332	0.01%	0.002%
41	6.076	1553	1566	1591	rVV	503213	1025545	45.30%	5.617%
42	6.297	1633	1635	1638	rBV3	851	528	0.02%	0.003%
43	6.445	1678	1681	1683	rBV3	1064	562	0.02%	0.003%
44	6.478	1689	1691	1692	rBV	559	211	0.01%	0.001%
45	6.510	1696	1701	1707	rBV4	528	713	0.03%	0.004%
46	6.542	1710	1711	1713	rBV	423	143	0.01%	0.001%
47	6.551	1713	1714	1717	rBV	333	183	0.01%	0.001%
48	6.587	1723	1725	1729	rVB4	788	396	0.02%	0.002%
49	6.658	1744	1747	1748	rBV2	925	518	0.02%	0.003%
50	6.722	1765	1767	1769	rBV	411	252	0.01%	0.001%
51	6.751	1774	1776	1779	rBV2	483	292	0.01%	0.002%
52	6.789	1784	1788	1793	rBV2	377	304	0.01%	0.002%
53	6.902	1820	1823	1826	rBV2	513	346	0.02%	0.002%
54	6.989	1832	1850	1879	rBV	281698	516786	22.83%	2.830%
55	7.320	1941	1953	1974	rBV	1006516	1729073	76.37%	9.469%
56	7.625	2038	2048	2074	rBV	196987	349068	15.42%	1.912%
57	7.805	2102	2104	2106	rVB3	1128	377	0.02%	0.002%
58	8.092	2183	2193	2229	rBV	574597	1049791	46.37%	5.749%
59	8.616	2354	2356	2358	rBV2	788	545	0.02%	0.003%
60	8.658	2366	2369	2373	rBV3	675	524	0.02%	0.003%
61	8.757	2399	2400	2402	rVB	701	208	0.01%	0.001%
62	8.809	2411	2416	2418	rBV3	980	869	0.04%	0.005%
63	8.857	2419	2431	2452	rBV	1196578	1938383	85.62%	10.616%
64	9.140	2516	2519	2521	rBV3	1219	942	0.04%	0.005%
65	9.256	2552	2555	2556	rBV	516	300	0.01%	0.002%
66	9.333	2577	2579	2584	rBV3	752	637	0.03%	0.003%
67	9.371	2588	2591	2593	rBV3	857	528	0.02%	0.003%
68	9.535	2635	2642	2643	rBV6	1394	1447	0.06%	0.008%
69	9.625	2667	2670	2673	rBV3	882	519	0.02%	0.003%
70	9.645	2673	2676	2681	rVB5	1162	1068	0.05%	0.006%
71	9.757	2708	2711	2715	rBV2	897	782	0.03%	0.004%
72	9.928	2761	2764	2767	rBV3	586	409	0.02%	0.002%
73	10.005	2784	2788	2790	rVB2	691	462	0.02%	0.003%
74	10.021	2790	2793	2794	rBV3	514	215	0.01%	0.001%
75	10.043	2794	2800	2804	rBV5	1017	868	0.04%	0.005%
76	10.088	2813	2814	2816	rBV2	414	147	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020764.D
 Acq On : 26 Mar 2021 18:07
 Operator : SY/MD
 Sample : M1784-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4S1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

77	10.101	2816	2818	2821	rVV2	396	221	0.01%	0.001%
78	10.220	2843	2855	2875	rBV	761003	1185794	52.38%	6.494%
79	10.374	2901	2903	2905	rBV3	1578	1008	0.04%	0.006%
80	10.439	2922	2923	2925	rBV	800	375	0.02%	0.002%
81	10.545	2954	2956	2961	rVB2	1059	680	0.03%	0.004%
82	10.567	2961	2963	2966	rVB4	929	478	0.02%	0.003%
83	10.603	2968	2974	2978	rBV4	1128	1284	0.06%	0.007%
84	10.657	2988	2991	2994	rBV2	607	493	0.02%	0.003%
85	10.690	3000	3001	3003	rBV	464	260	0.01%	0.001%
86	10.786	3029	3031	3033	rBV2	458	179	0.01%	0.001%
87	11.066	3117	3118	3120	rBV	565	273	0.01%	0.001%
88	11.162	3140	3148	3158	rBV6	4771	8161	0.36%	0.045%
89	11.255	3165	3177	3194	rBV	1253769	1899054	83.88%	10.400%
90	11.632	3281	3294	3311	rBV	1169333	1804953	79.73%	9.885%
91	11.873	3368	3369	3373	rBV2	699	419	0.02%	0.002%
92	11.985	3402	3404	3408	rBV4	802	586	0.03%	0.003%
93	12.024	3413	3416	3418	rBV3	885	493	0.02%	0.003%
94	12.741	3637	3639	3641	rBV2	601	276	0.01%	0.002%
95	12.889	3681	3685	3686	rBV	1446	752	0.03%	0.004%
96	12.934	3697	3699	3701	rBV2	760	312	0.01%	0.002%
97	12.992	3714	3717	3723	rBV5	746	892	0.04%	0.005%
98	13.017	3723	3725	3730	rVB3	1042	568	0.03%	0.003%
99	13.587	3900	3902	3905	rBV3	722	438	0.02%	0.002%
100	14.239	4101	4105	4108	rBV5	1379	1166	0.05%	0.006%




Sum of corrected areas: 18259469

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020764.D
Acq On : 26 Mar 2021 18:07
Operator : SY/MD
Sample : M1784-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
BG4S1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

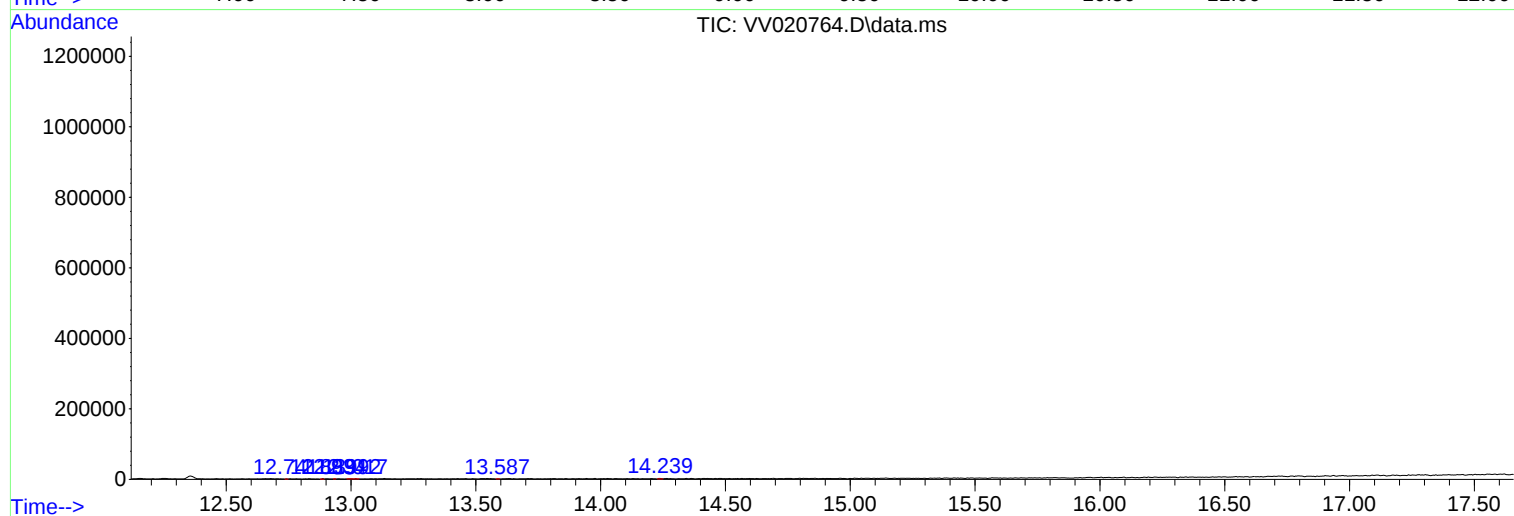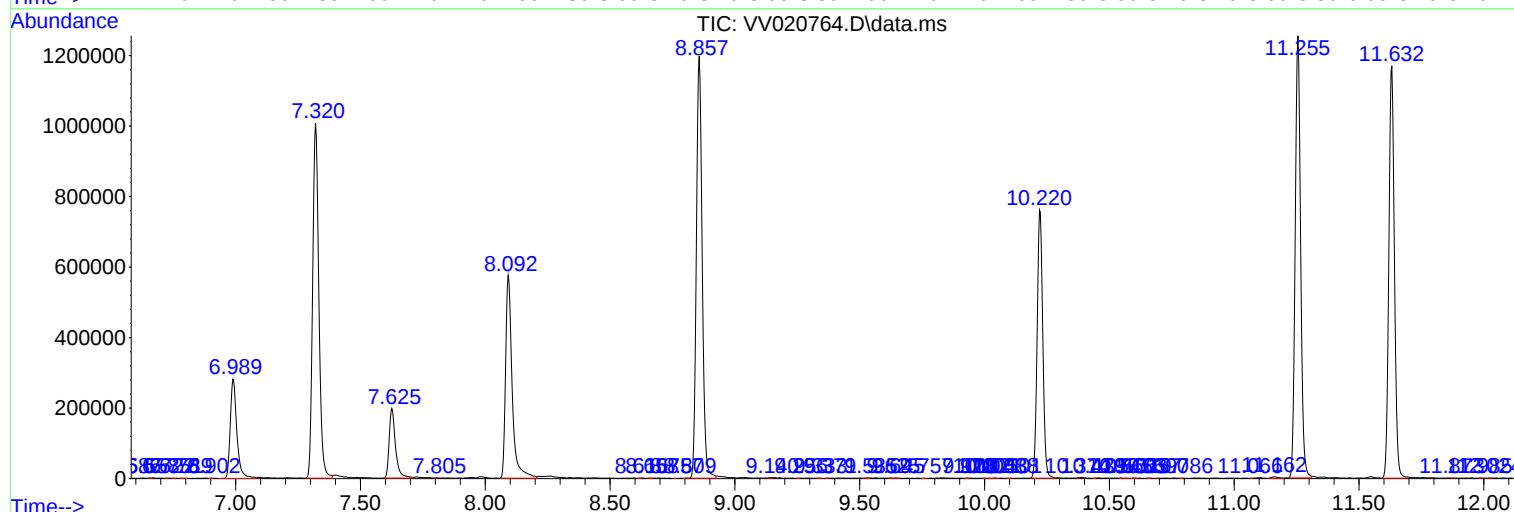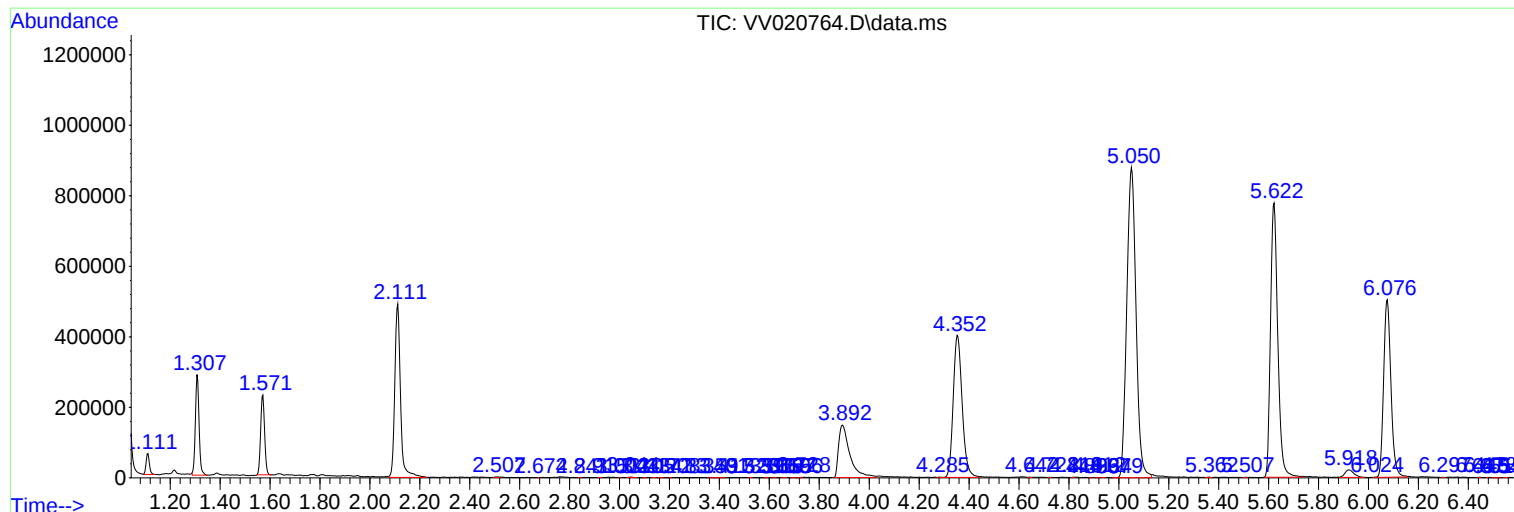

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020764.D
Acq On : 26 Mar 2021 18:07
Operator : SY/MD
Sample : M1784-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4S1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020764.D
Acq On : 26 Mar 2021 18:07
Operator : SY/MD
Sample : M1784-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4S1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
