

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020766.D
 Acq On : 26 Mar 2021 18:54
 Operator : SY/MD
 Sample : M1784-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4S3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020766.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	17	21	32	rVB2	50151	45282	1.99%	0.248%
2	1.307	76	83	97	rVB	275915	293113	12.90%	1.608%
3	1.571	158	165	178	rVB	226640	253405	11.15%	1.390%
4	2.111	323	333	351	rBV	486853	734935	32.34%	4.031%
5	2.298	388	391	394	rBV4	1169	1054	0.05%	0.006%
6	2.622	489	492	497	rVB3	569	418	0.02%	0.002%
7	2.645	497	499	505	rVB3	333	208	0.01%	0.001%
8	2.674	506	508	510	rBV2	691	370	0.02%	0.002%
9	2.732	523	526	527	rBV2	1017	600	0.03%	0.003%
10	2.806	547	549	553	rVB3	982	466	0.02%	0.003%
11	2.825	553	555	557	rVB2	632	257	0.01%	0.001%
12	2.841	557	560	563	rBV	733	480	0.02%	0.003%
13	2.873	566	570	575	rVB3	734	626	0.03%	0.003%
14	2.992	605	607	611	rVB4	1048	548	0.02%	0.003%
15	3.024	614	617	621	rBV4	899	688	0.03%	0.004%
16	3.095	636	639	644	rVB3	616	431	0.02%	0.002%
17	3.130	644	650	652	rVB3	681	568	0.02%	0.003%
18	3.143	652	654	656	rBV	499	250	0.01%	0.001%
19	3.208	673	674	678	rVB3	725	244	0.01%	0.001%
20	3.278	693	696	697	rBV2	468	225	0.01%	0.001%
21	3.507	764	767	770	rBV2	636	482	0.02%	0.003%
22	3.526	770	773	776	rVB2	604	365	0.02%	0.002%
23	3.542	776	778	780	rVB2	641	305	0.01%	0.002%
24	3.558	780	783	785	rBV2	577	349	0.02%	0.002%
25	3.603	795	797	800	rBV2	771	451	0.02%	0.002%
26	3.626	802	804	806	rBV2	453	189	0.01%	0.001%
27	3.661	812	815	819	rBV3	427	324	0.01%	0.002%
28	3.683	820	822	826	rBV5	464	278	0.01%	0.002%
29	3.703	826	828	830	rBV2	858	496	0.02%	0.003%
30	3.809	859	861	864	rBV3	723	551	0.02%	0.003%
31	3.892	876	887	915	rBV2	146427	443063	19.50%	2.430%
32	4.352	1015	1030	1057	rBV	397721	973864	42.86%	5.342%
33	4.777	1160	1162	1167	rVB4	1368	1016	0.04%	0.006%
34	4.818	1174	1175	1178	rVB2	860	381	0.02%	0.002%
35	4.838	1178	1181	1184	rBV2	539	362	0.02%	0.002%
36	4.892	1195	1198	1201	rBV3	720	489	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032621\
 Data File : VW020766.D
 Acq On : 26 Mar 2021 18:54
 Operator : SY/MD
 Sample : M1784-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4S3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

37	4.931	1208	1210	1213	rBV2	526	299	0.01%	0.002%
38	4.970	1220	1222	1225	rVB	666	395	0.02%	0.002%
39	5.050	1229	1247	1276	rBV2	869364	2272198	100.00%	12.463%
40	5.458	1372	1374	1376	rBV2	557	338	0.01%	0.002%
41	5.619	1412	1424	1460	rBV	780459	1570030	69.10%	8.612%
42	5.873	1499	1503	1506	rBV4	924	972	0.04%	0.005%
43	5.918	1506	1517	1537	rVB7	12677	31036	1.37%	0.170%
44	6.021	1546	1549	1552	rBV3	858	762	0.03%	0.004%
45	6.072	1552	1565	1589	rBV	501725	1019747	44.88%	5.594%
46	6.317	1635	1641	1646	rBV8	2458	3518	0.15%	0.019%
47	6.529	1702	1707	1708	rBV3	690	574	0.03%	0.003%
48	6.539	1708	1710	1712	rVB2	791	349	0.02%	0.002%
49	6.699	1758	1760	1762	rBV3	577	183	0.01%	0.001%
50	6.764	1778	1780	1782	rBV2	926	507	0.02%	0.003%
51	6.989	1839	1850	1873	rBV	275523	503634	22.17%	2.763%
52	7.265	1933	1936	1940	rBV	1115	636	0.03%	0.003%
53	7.320	1940	1953	1973	rBV	999526	1727099	76.01%	9.473%
54	7.625	2037	2048	2076	rBV	200918	357197	15.72%	1.959%
55	7.879	2125	2127	2130	rBV3	609	416	0.02%	0.002%
56	8.053	2179	2181	2182	rBV	775	346	0.02%	0.002%
57	8.092	2183	2193	2231	rBV	585337	1063272	46.79%	5.832%
58	8.651	2363	2367	2369	rBV4	673	420	0.02%	0.002%
59	8.690	2375	2379	2380	rBV	995	512	0.02%	0.003%
60	8.725	2387	2390	2393	rBV3	871	771	0.03%	0.004%
61	8.741	2393	2395	2400	rVB4	1206	706	0.03%	0.004%
62	8.770	2400	2404	2406	rBV2	828	580	0.03%	0.003%
63	8.857	2419	2431	2454	rBV	1218595	1963000	86.39%	10.767%
64	9.111	2506	2510	2515	rVB5	1466	1283	0.06%	0.007%
65	9.143	2516	2520	2521	rBV4	944	723	0.03%	0.004%
66	9.191	2532	2535	2537	rBV3	964	573	0.03%	0.003%
67	9.326	2574	2577	2579	rBV3	1095	787	0.03%	0.004%
68	9.423	2604	2607	2611	rVB3	814	588	0.03%	0.003%
69	9.442	2611	2613	2615	rBV	531	354	0.02%	0.002%
70	9.474	2621	2623	2626	rBV	567	428	0.02%	0.002%
71	9.529	2638	2640	2643	rBV2	524	217	0.01%	0.001%
72	9.657	2678	2680	2681	rBV	608	255	0.01%	0.001%
73	9.712	2695	2697	2698	rBV	769	355	0.02%	0.002%
74	9.802	2723	2725	2726	rBV	742	304	0.01%	0.002%
75	9.879	2747	2749	2751	rBV	570	340	0.01%	0.002%
76	9.889	2751	2752	2758	rVB4	981	667	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020766.D
 Acq On : 26 Mar 2021 18:54
 Operator : SY/MD
 Sample : M1784-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4S3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

77	9.918	2758	2761	2762	rBV	689	341	0.02%	0.002%
78	10.014	2786	2791	2792	rBV3	803	572	0.03%	0.003%
79	10.108	2817	2820	2822	rBV2	675	384	0.02%	0.002%
80	10.220	2843	2855	2879	rBV	749863	1193299	52.52%	6.545%
81	10.461	2928	2930	2932	rBV2	753	333	0.01%	0.002%
82	10.503	2941	2943	2944	rBV	700	316	0.01%	0.002%
83	10.654	2988	2990	2994	rBV2	584	380	0.02%	0.002%
84	10.719	3008	3010	3012	rBV2	855	366	0.02%	0.002%
85	10.731	3012	3014	3016	rVV2	992	541	0.02%	0.003%
86	10.754	3019	3021	3024	rBV	830	435	0.02%	0.002%
87	10.911	3067	3070	3071	rBV2	782	365	0.02%	0.002%
88	10.921	3071	3073	3075	rBV3	1104	561	0.02%	0.003%
89	11.159	3140	3147	3160	rVB3	9691	14865	0.65%	0.082%
90	11.255	3165	3177	3202	rBV	1246450	1915190	84.29%	10.505%
91	11.500	3250	3253	3256	rBV5	1074	968	0.04%	0.005%
92	11.632	3282	3294	3312	rBV	1164770	1785895	78.60%	9.796%
93	12.091	3432	3437	3441	rBV5	957	989	0.04%	0.005%
94	12.130	3445	3449	3450	rBV3	746	468	0.02%	0.003%
95	12.352	3511	3518	3535	rVB9	16707	28242	1.24%	0.155%
96	12.635	3603	3606	3610	rBV4	1186	904	0.04%	0.005%
97	12.808	3657	3660	3661	rBV2	881	459	0.02%	0.003%
98	13.210	3783	3785	3787	rBV3	980	505	0.02%	0.003%
99	13.387	3839	3840	3842	rBV	893	425	0.02%	0.002%
100	14.140	4072	4074	4077	rBV3	1111	544	0.02%	0.003%


Sum of corrected areas: 18230851

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020766.D
Acq On : 26 Mar 2021 18:54
Operator : SY/MD
Sample : M1784-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4S3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

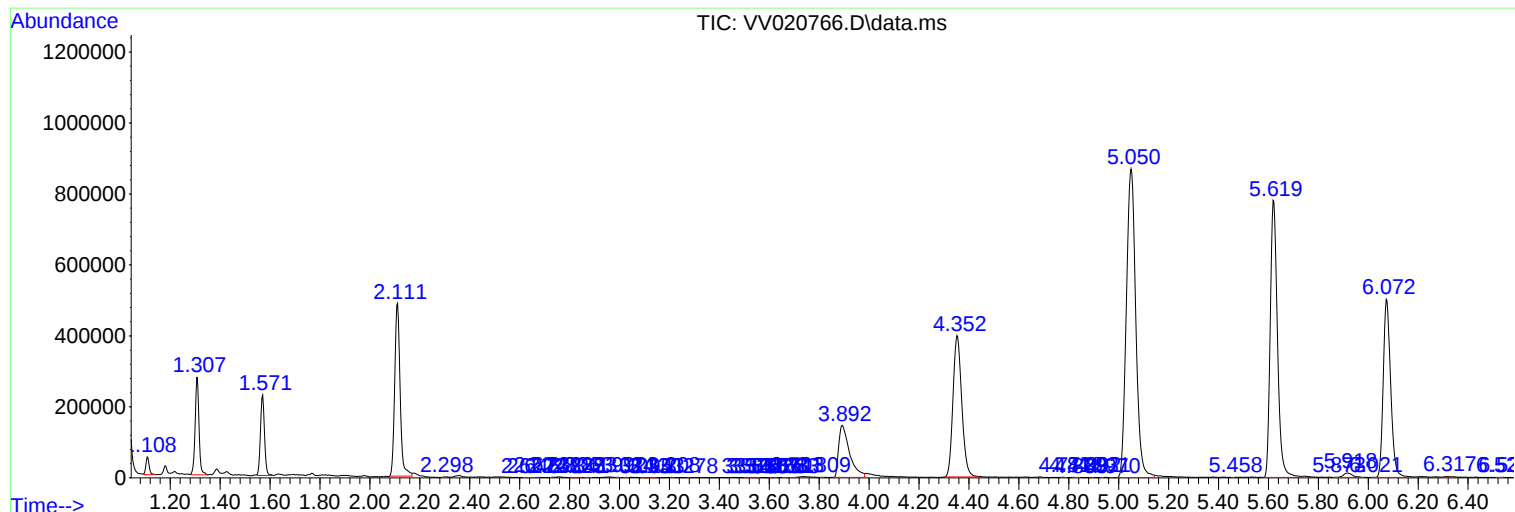

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020766.D
Acq On : 26 Mar 2021 18:54
Operator : SY/MD
Sample : M1784-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4S3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020766.D
Acq On : 26 Mar 2021 18:54
Operator : SY/MD
Sample : M1784-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4S3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
