

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020770.D
 Acq On : 26 Mar 2021 20:54
 Operator : SY/MD
 Sample : VV0326WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK81

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020770.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	99	rVB	340550	341668	13.31%	1.744%
2	1.571	157	165	175	rBV	275126	305498	11.90%	1.559%
3	2.111	322	333	363	rVB	611896	927433	36.14%	4.733%
4	2.449	437	438	441	rBV2	425	253	0.01%	0.001%
5	2.494	450	452	453	rBV	722	297	0.01%	0.002%
6	2.581	477	479	482	rBV3	368	267	0.01%	0.001%
7	2.613	487	489	490	rBV	501	245	0.01%	0.001%
8	2.651	499	501	502	rBV	543	220	0.01%	0.001%
9	2.699	513	516	518	rBV	361	210	0.01%	0.001%
10	2.757	528	534	536	rBV3	1113	1042	0.04%	0.005%
11	2.838	557	559	562	rVB3	1037	510	0.02%	0.003%
12	2.873	567	570	574	rVB2	745	516	0.02%	0.003%
13	2.908	574	581	586	rVB3	327	479	0.02%	0.002%
14	2.934	586	589	592	rBV2	487	320	0.01%	0.002%
15	3.024	612	617	619	rBV2	424	324	0.01%	0.002%
16	3.085	632	636	638	rBV3	418	328	0.01%	0.002%
17	3.124	644	648	650	rBV3	687	590	0.02%	0.003%
18	3.172	661	663	665	rBV	713	270	0.01%	0.001%
19	3.259	687	690	692	rVB2	322	211	0.01%	0.001%
20	3.275	692	695	697	rBV3	483	377	0.01%	0.002%
21	3.310	703	706	708	rBV2	379	283	0.01%	0.001%
22	3.336	713	714	718	rVV	498	332	0.01%	0.002%
23	3.355	718	720	726	rVV2	395	258	0.01%	0.001%
24	3.442	745	747	751	rBV	477	248	0.01%	0.001%
25	3.484	756	760	762	rVV2	323	252	0.01%	0.001%
26	3.503	762	766	769	rVB2	441	354	0.01%	0.002%
27	3.526	769	773	775	rBV	534	267	0.01%	0.001%
28	3.539	775	777	782	rVB2	702	441	0.02%	0.002%
29	3.568	782	786	789	rBV3	430	243	0.01%	0.001%
30	3.629	802	805	806	rBV2	428	234	0.01%	0.001%
31	3.719	829	833	835	rBV3	302	227	0.01%	0.001%
32	3.732	835	837	839	rBV3	525	254	0.01%	0.001%
33	3.838	867	870	873	rVB	370	234	0.01%	0.001%
34	3.896	877	888	923	rBV	153182	476705	18.58%	2.433%
35	4.352	1012	1030	1058	rBV	443120	1090421	42.49%	5.564%
36	4.754	1153	1155	1158	rBV3	396	317	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020770.D
 Acq On : 26 Mar 2021 20:54
 Operator : SY/MD
 Sample : VV0326WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK81

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	4.767	1158	1159	1165	rVB4	775	590	0.02%	0.003%
38	4.796	1165	1168	1171	rVB3	694	503	0.02%	0.003%
39	4.815	1171	1174	1175	rBV3	854	506	0.02%	0.003%
40	4.921	1204	1207	1210	rVV3	794	652	0.03%	0.003%
41	4.957	1217	1218	1220	rBV	458	208	0.01%	0.001%
42	5.050	1229	1247	1279	rBV2	1000623	2566213	100.00%	13.095%
43	5.420	1360	1362	1365	rBV2	745	387	0.02%	0.002%
44	5.436	1365	1367	1369	rBV3	776	404	0.02%	0.002%
45	5.548	1399	1402	1404	rBV	461	274	0.01%	0.001%
46	5.568	1406	1408	1410	rBV3	753	356	0.01%	0.002%
47	5.622	1412	1425	1454	rBV	772841	1547503	60.30%	7.897%
48	6.076	1552	1566	1590	rBV	549051	1123004	43.76%	5.731%
49	6.474	1686	1690	1691	rBV2	591	373	0.01%	0.002%
50	6.503	1695	1699	1704	rVB4	644	670	0.03%	0.003%
51	6.542	1708	1711	1713	rVB2	550	310	0.01%	0.002%
52	6.555	1713	1715	1717	rBV	604	351	0.01%	0.002%
53	6.584	1722	1724	1727	rBV2	370	217	0.01%	0.001%
54	6.658	1744	1747	1749	rBV2	565	369	0.01%	0.002%
55	6.690	1754	1757	1759	rBV2	471	260	0.01%	0.001%
56	6.722	1765	1767	1770	rVB	509	278	0.01%	0.001%
57	6.764	1778	1780	1783	rBV2	567	353	0.01%	0.002%
58	6.793	1786	1789	1791	rVB2	605	287	0.01%	0.001%
59	6.815	1791	1796	1799	rBV3	472	529	0.02%	0.003%
60	6.989	1839	1850	1876	rBV	309317	570926	22.25%	2.913%
61	7.178	1907	1909	1912	rBV3	891	502	0.02%	0.003%
62	7.320	1941	1953	1975	rBV	1181454	2035245	79.31%	10.386%
63	7.625	2038	2048	2080	rBV	219126	394619	15.38%	2.014%
64	7.847	2116	2117	2121	rVB3	667	388	0.02%	0.002%
65	8.092	2183	2193	2226	rBV	609250	1106392	43.11%	5.646%
66	8.603	2347	2352	2353	rBV3	547	511	0.02%	0.003%
67	8.857	2419	2431	2456	rBV	1207544	1944403	75.77%	9.922%
68	9.091	2501	2504	2506	rBV3	873	560	0.02%	0.003%
69	9.133	2515	2517	2521	rBV3	694	450	0.02%	0.002%
70	9.204	2537	2539	2546	rVB5	915	814	0.03%	0.004%
71	9.252	2552	2554	2557	rBV2	693	305	0.01%	0.002%
72	9.272	2557	2560	2563	rBV3	718	434	0.02%	0.002%
73	9.333	2577	2579	2584	rVB3	612	393	0.02%	0.002%
74	9.391	2592	2597	2601	rBV4	578	713	0.03%	0.004%
75	9.487	2623	2627	2628	rBV2	429	359	0.01%	0.002%
76	9.522	2633	2638	2639	rBV3	704	603	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020770.D
 Acq On : 26 Mar 2021 20:54
 Operator : SY/MD
 Sample : VV0326WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK81

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

77	9.731	2701	2703	2705	rVB	858	321	0.01%	0.002%
78	9.747	2705	2708	2710	rBV2	594	384	0.01%	0.002%
79	9.828	2730	2733	2742	rBV5	1025	1223	0.05%	0.006%
80	9.870	2742	2746	2749	rBV3	534	497	0.02%	0.003%
81	9.944	2765	2769	2770	rBV2	795	536	0.02%	0.003%
82	9.989	2779	2783	2784	rBV	653	430	0.02%	0.002%
83	10.108	2818	2820	2823	rVB2	578	314	0.01%	0.002%
84	10.220	2841	2855	2877	rBV	797157	1249104	48.67%	6.374%
85	10.461	2928	2930	2932	rVB2	788	222	0.01%	0.001%
86	10.484	2935	2937	2942	rVB4	669	530	0.02%	0.003%
87	10.857	3049	3053	3056	rBV5	1525	1332	0.05%	0.007%
88	10.982	3086	3092	3093	rBV2	617	555	0.02%	0.003%
89	11.169	3146	3150	3152	rBV3	988	739	0.03%	0.004%
90	11.255	3165	3177	3198	rBV	1237885	1899618	74.02%	9.694%
91	11.525	3259	3261	3265	rBV3	543	440	0.02%	0.002%
92	11.632	3280	3294	3316	rBV	1256504	1979843	77.15%	10.103%
93	12.323	3506	3509	3511	rBV2	717	356	0.01%	0.002%
94	12.435	3541	3544	3548	rBV3	1335	1253	0.05%	0.006%
95	12.651	3607	3611	3613	rBV3	1772	1478	0.06%	0.008%
96	12.908	3688	3691	3693	rBV	764	382	0.01%	0.002%
97	13.098	3746	3750	3752	rBV2	824	702	0.03%	0.004%
98	13.159	3766	3769	3772	rBV3	946	711	0.03%	0.004%
99	13.873	3989	3991	3993	rBV	874	371	0.01%	0.002%
100	14.593	4213	4215	4219	rVB5	1100	657	0.03%	0.003%




Sum of corrected areas: 19596340

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020770.D
Acq On : 26 Mar 2021 20:54
Operator : SY/MD
Sample : VV0326WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK81

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

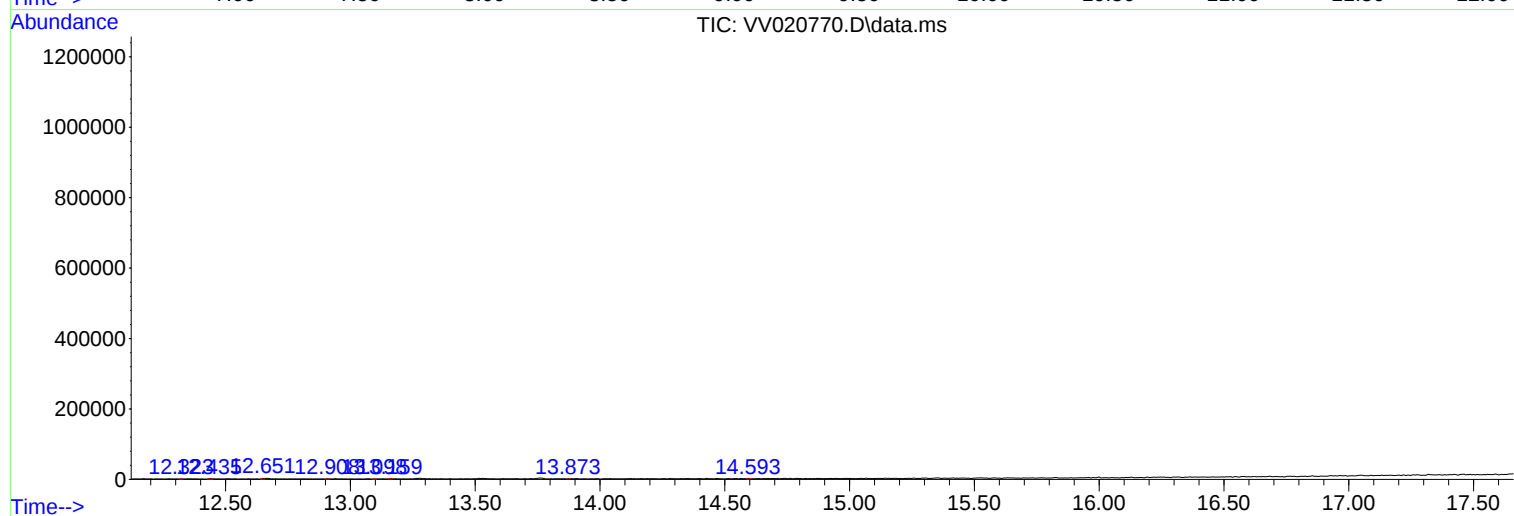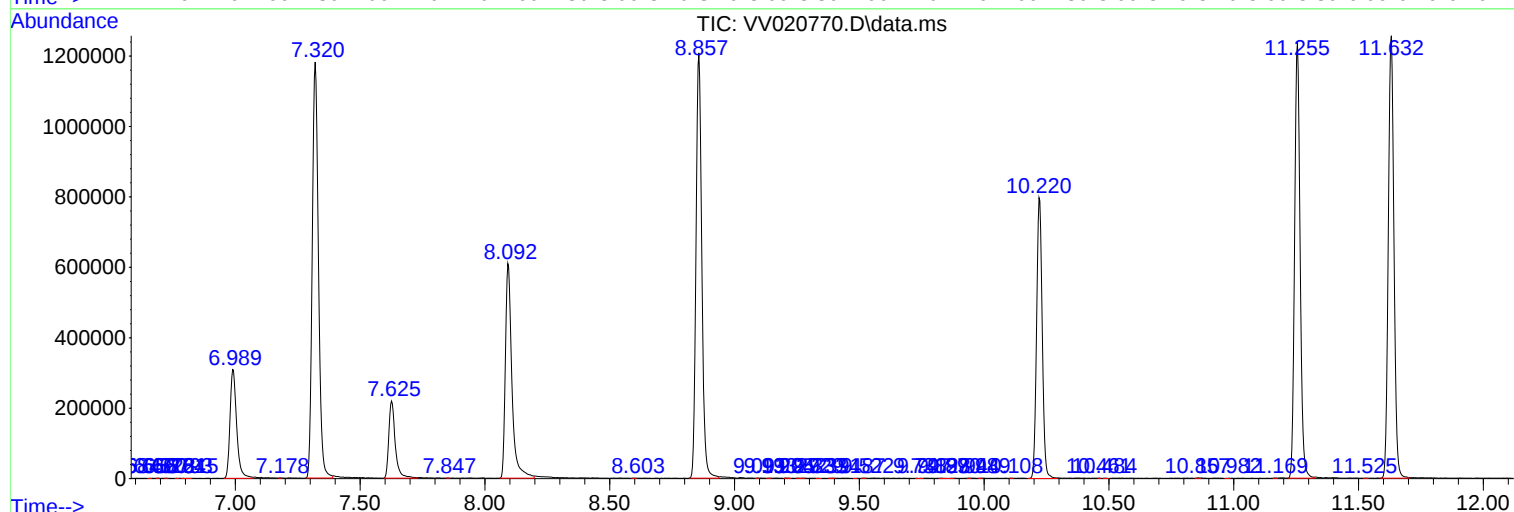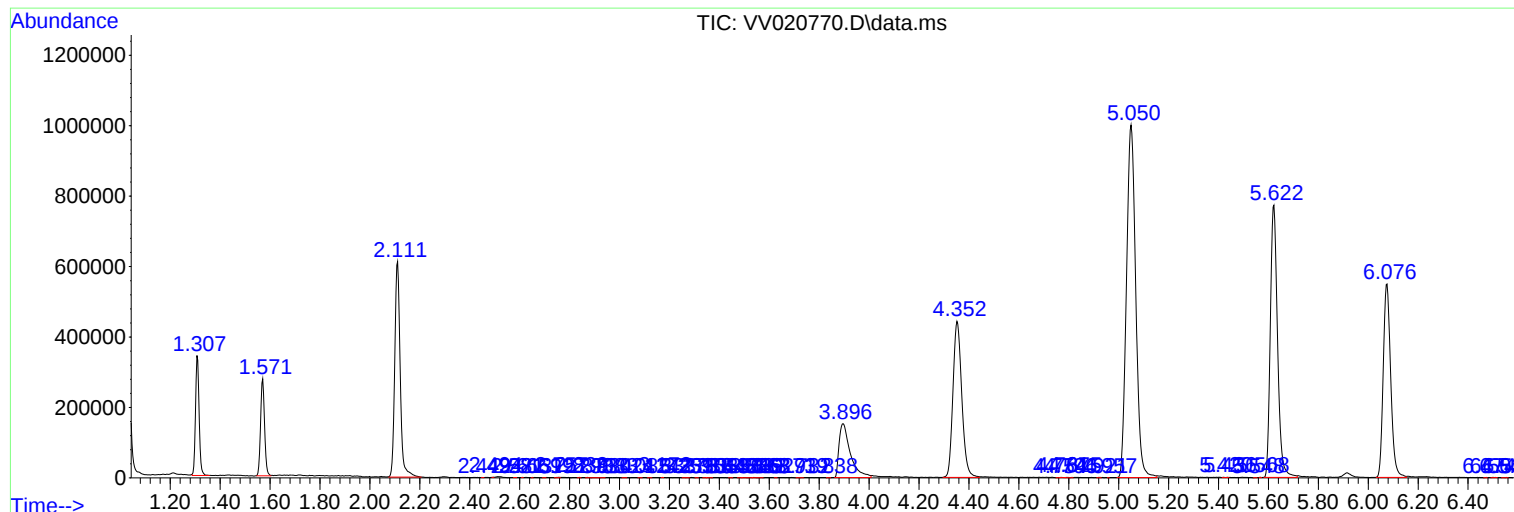

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020770.D
Acq On : 26 Mar 2021 20:54
Operator : SY/MD
Sample : VV0326WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK81

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020770.D
Acq On : 26 Mar 2021 20:54
Operator : SY/MD
Sample : VV0326WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK81

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
