

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020771.D
 Acq On : 26 Mar 2021 21:18
 Operator : SY/MD
 Sample : M1824-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4S6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

Signal : TIC: VV020771.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	98	rVB	260786	265487	11.82%	1.458%
2	1.571	157	165	175	rBV	225144	255445	11.37%	1.403%
3	2.111	322	333	367	rVB	490251	757531	33.72%	4.160%
4	2.269	380	382	383	rBV	474	144	0.01%	0.001%
5	2.352	407	408	411	rBV3	796	396	0.02%	0.002%
6	2.571	474	476	478	rBV	798	517	0.02%	0.003%
7	2.603	483	486	488	rBV3	920	549	0.02%	0.003%
8	2.651	498	501	506	rBV4	439	392	0.02%	0.002%
9	2.683	509	511	513	rBV	465	248	0.01%	0.001%
10	2.699	513	516	518	rBV2	637	354	0.02%	0.002%
11	2.822	551	554	559	rBV6	745	824	0.04%	0.005%
12	2.857	562	565	566	rBV	411	240	0.01%	0.001%
13	2.912	578	582	586	rBV2	913	764	0.03%	0.004%
14	2.960	592	597	601	rBV3	685	668	0.03%	0.004%
15	3.031	613	619	622	rVB5	584	555	0.02%	0.003%
16	3.056	622	627	632	rBV2	586	592	0.03%	0.003%
17	3.092	635	638	639	rBV2	227	123	0.01%	0.001%
18	3.105	640	642	644	rVB	354	140	0.01%	0.001%
19	3.117	644	646	648	rBV2	533	271	0.01%	0.001%
20	3.153	656	657	658	rBV	231	47	0.00%	0.000%
21	3.169	658	662	663	rBV2	602	419	0.02%	0.002%
22	3.211	672	675	683	rVB3	741	856	0.04%	0.005%
23	3.246	683	686	687	rBV	162	90	0.00%	0.000%
24	3.269	690	693	695	rBV2	527	369	0.02%	0.002%
25	3.281	695	697	699	rVV	354	172	0.01%	0.001%
26	3.378	723	727	731	rBV4	472	451	0.02%	0.002%
27	3.455	748	751	752	rBV	473	277	0.01%	0.002%
28	3.478	756	758	759	rVB	218	52	0.00%	0.000%
29	3.487	759	761	762	rBV	335	119	0.01%	0.001%
30	3.519	768	771	774	rBV3	571	339	0.02%	0.002%
31	3.552	779	781	785	rVB2	537	322	0.01%	0.002%
32	3.577	785	789	790	rBV	571	267	0.01%	0.001%
33	3.587	790	792	795	rVB2	415	192	0.01%	0.001%
34	3.616	797	801	804	rVB3	652	402	0.02%	0.002%
35	3.635	804	807	810	rBV2	299	206	0.01%	0.001%
36	3.693	824	825	826	rBV2	276	59	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020771.D
 Acq On : 26 Mar 2021 21:18
 Operator : SY/MD
 Sample : M1824-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4S6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	3.712	826	831	832	rBV2	383	309	0.01%	0.002%
38	3.760	844	846	850	rVB3	575	355	0.02%	0.002%
39	3.783	851	853	856	rBV3	678	357	0.02%	0.002%
40	3.818	862	864	867	rBV3	433	206	0.01%	0.001%
41	3.892	876	887	931	rBV	151132	468592	20.86%	2.573%
42	4.352	1013	1030	1058	rBV	391510	980030	43.62%	5.382%
43	4.982	1223	1226	1227	rBV	411	263	0.01%	0.001%
44	5.050	1229	1247	1271	rBV2	870566	2246685	100.00%	12.337%
45	5.404	1355	1357	1360	rBV2	851	441	0.02%	0.002%
46	5.622	1411	1425	1459	rBV	784522	1586863	70.63%	8.714%
47	6.008	1542	1545	1547	rBV4	526	386	0.02%	0.002%
48	6.072	1552	1565	1596	rBV	497981	1022590	45.52%	5.615%
49	6.371	1656	1658	1663	rVB2	672	365	0.02%	0.002%
50	6.510	1697	1701	1703	rBV5	716	493	0.02%	0.003%
51	6.600	1727	1729	1731	rVB2	552	298	0.01%	0.002%
52	6.629	1736	1738	1739	rBV	466	189	0.01%	0.001%
53	6.645	1739	1743	1746	rBV3	456	416	0.02%	0.002%
54	6.767	1777	1781	1786	rBV7	856	773	0.03%	0.004%
55	6.802	1790	1792	1794	rVB	593	251	0.01%	0.001%
56	6.818	1794	1797	1798	rBV2	304	167	0.01%	0.001%
57	6.828	1798	1800	1804	rBV2	650	402	0.02%	0.002%
58	6.860	1808	1810	1814	rBV2	445	292	0.01%	0.002%
59	6.905	1821	1824	1826	rBV3	461	284	0.01%	0.002%
60	6.989	1838	1850	1876	rBV	277210	507093	22.57%	2.785%
61	7.320	1941	1953	1975	rBV	982431	1707688	76.01%	9.377%
62	7.625	2038	2048	2067	rBV	197960	346124	15.41%	1.901%
63	7.850	2112	2118	2122	rBV6	1484	2060	0.09%	0.011%
64	7.928	2139	2142	2143	rBV	1554	889	0.04%	0.005%
65	7.982	2149	2159	2177	rVB4	56569	101088	4.50%	0.555%
66	8.091	2183	2193	2229	rBV	571155	1051249	46.79%	5.773%
67	8.657	2366	2369	2373	rBV4	1272	955	0.04%	0.005%
68	8.728	2389	2391	2393	rBV2	739	347	0.02%	0.002%
69	8.857	2417	2431	2457	rBV	1222639	1979137	88.09%	10.868%
70	9.390	2595	2597	2599	rBV	554	226	0.01%	0.001%
71	9.423	2605	2607	2611	rVB3	809	363	0.02%	0.002%
72	9.503	2629	2632	2634	rBV2	718	454	0.02%	0.002%
73	9.545	2637	2645	2646	rBV4	1448	1468	0.07%	0.008%
74	9.690	2685	2690	2692	rBV3	761	538	0.02%	0.003%
75	9.722	2698	2700	2703	rBV2	748	403	0.02%	0.002%
76	9.780	2715	2718	2719	rBV	342	173	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020771.D
 Acq On : 26 Mar 2021 21:18
 Operator : SY/MD
 Sample : M1824-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4S6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

77	9.831	2731	2734	2737	rBV4	807	766	0.03%	0.004%
78	9.940	2764	2768	2776	rVB4	2107	2281	0.10%	0.013%
79	10.146	2828	2832	2835	rBV3	573	554	0.02%	0.003%
80	10.220	2843	2855	2875	rBV	748764	1172068	52.17%	6.436%
81	10.616	2976	2978	2979	rBV	506	211	0.01%	0.001%
82	10.664	2992	2993	2995	rVB	332	74	0.00%	0.000%
83	10.927	3068	3075	3082	rBV6	2564	3418	0.15%	0.019%
84	11.082	3120	3123	3127	rBV5	996	920	0.04%	0.005%
85	11.255	3165	3177	3203	rBV	1247086	1923005	85.59%	10.560%
86	11.529	3259	3262	3263	rBV2	818	414	0.02%	0.002%
87	11.542	3264	3266	3268	rBV3	1526	818	0.04%	0.004%
88	11.632	3281	3294	3317	rBV	1142447	1788115	79.59%	9.819%
89	11.866	3363	3367	3369	rBV2	979	767	0.03%	0.004%
90	12.101	3438	3440	3442	rBV2	790	304	0.01%	0.002%
91	12.146	3451	3454	3461	rVB3	2316	2018	0.09%	0.011%
92	12.355	3513	3519	3529	rBV10	7124	10038	0.45%	0.055%
93	12.429	3540	3542	3544	rBV3	1273	797	0.04%	0.004%
94	12.921	3693	3695	3699	rBV3	784	551	0.02%	0.003%
95	13.120	3755	3757	3760	rBV2	701	364	0.02%	0.002%
96	13.458	3859	3862	3866	rBV5	1496	1006	0.04%	0.006%
97	13.593	3901	3904	3909	rBV2	1213	901	0.04%	0.005%




Sum of corrected areas: 18210531

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020771.D
Acq On : 26 Mar 2021 21:18
Operator : SY/MD
Sample : M1824-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4S6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

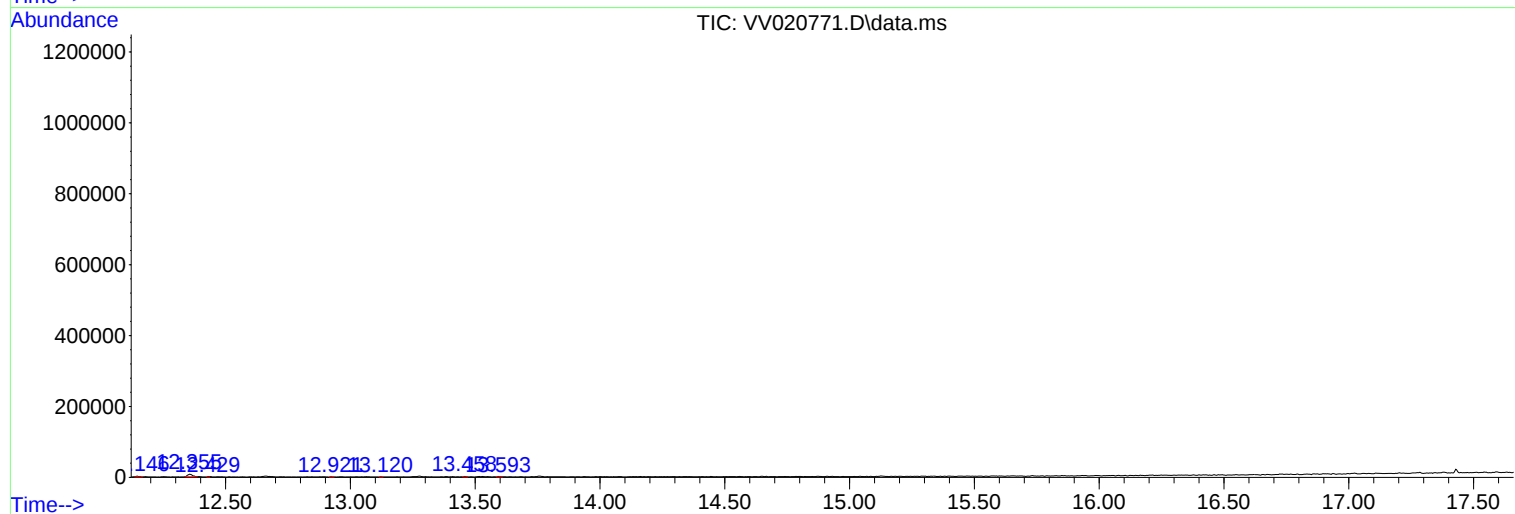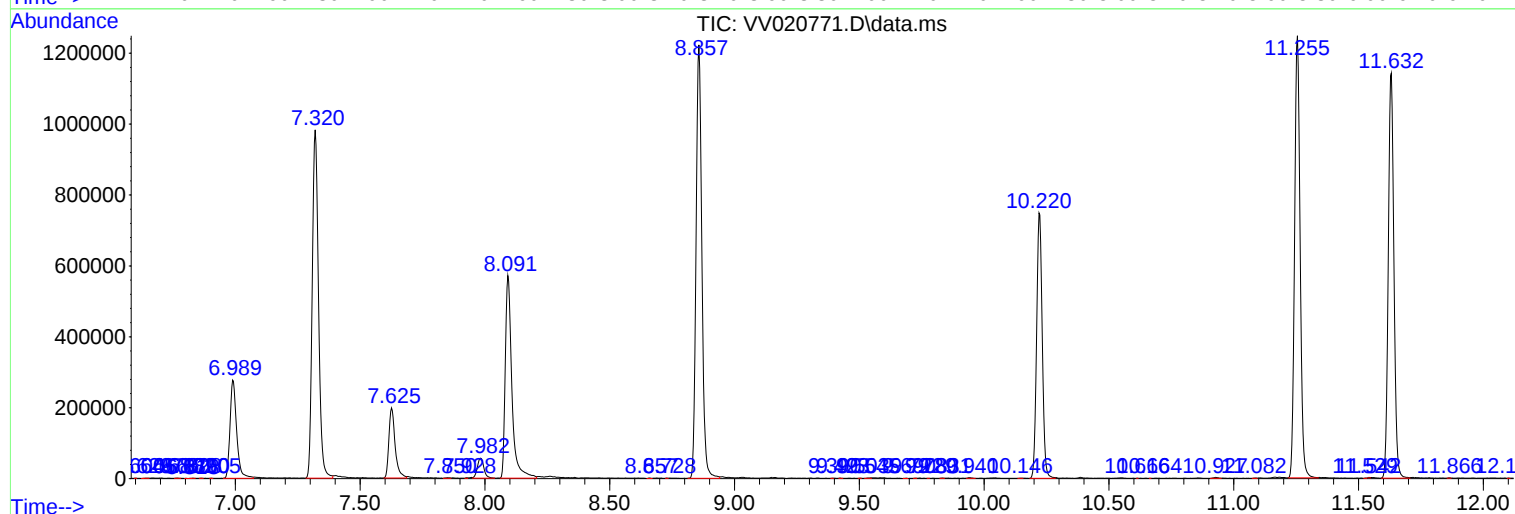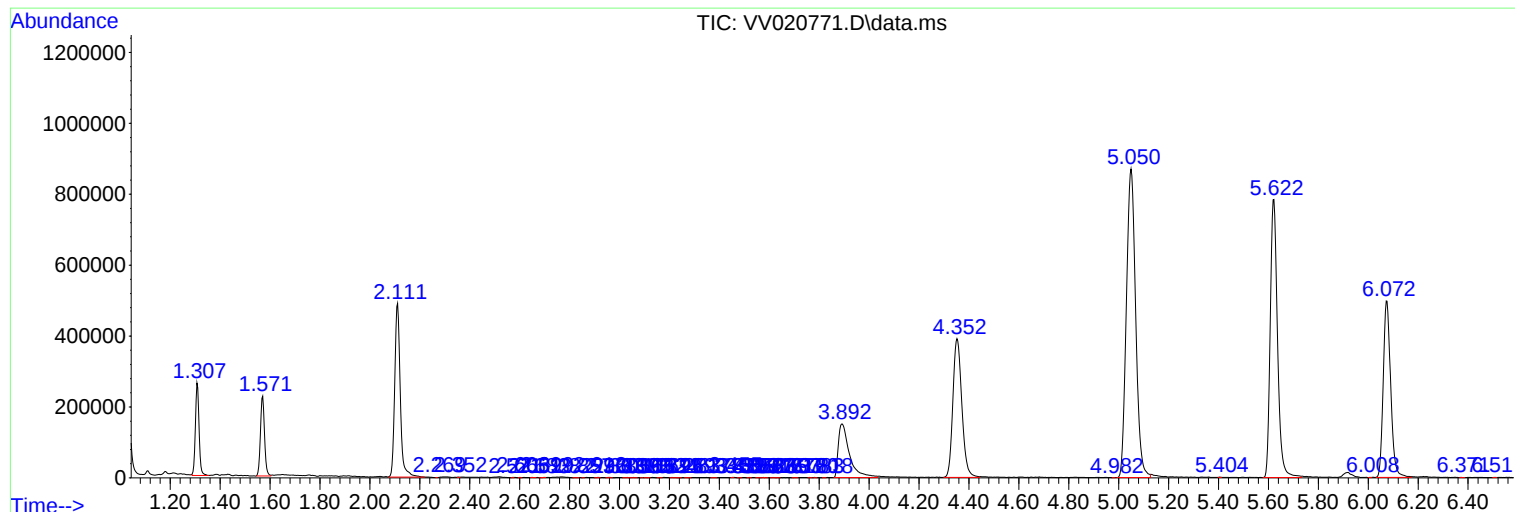

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020771.D
Acq On : 26 Mar 2021 21:18
Operator : SY/MD
Sample : M1824-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4S6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020771.D
Acq On : 26 Mar 2021 21:18
Operator : SY/MD
Sample : M1824-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4S6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
