

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020780.D
 Acq On : 27 Mar 2021 00:49
 Operator : SY/MD
 Sample : M1824-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4T5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020780.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	17	21	28	rVB	29467	25979	1.18%	0.148%
2	1.307	77	83	99	rVB	252379	259194	11.78%	1.477%
3	1.568	157	164	177	rBV	216901	243778	11.08%	1.389%
4	2.111	323	333	350	rBV	457012	695460	31.60%	3.963%
5	2.291	386	389	391	rBV3	1077	800	0.04%	0.005%
6	2.609	487	488	490	rBV2	637	336	0.02%	0.002%
7	2.664	499	505	508	rVB4	874	694	0.03%	0.004%
8	2.690	510	513	518	rVB2	922	757	0.03%	0.004%
9	2.715	518	521	522	rBV2	360	248	0.01%	0.001%
10	2.770	536	538	540	rVB	584	251	0.01%	0.001%
11	2.786	540	543	547	rBV3	440	443	0.02%	0.003%
12	2.806	547	549	553	rVB4	641	471	0.02%	0.003%
13	2.838	553	559	562	rBV3	800	554	0.03%	0.003%
14	2.867	562	568	571	rBV2	684	751	0.03%	0.004%
15	2.998	605	609	611	rBV2	437	321	0.01%	0.002%
16	3.053	623	626	628	rVV	766	436	0.02%	0.002%
17	3.121	642	647	649	rBV2	486	323	0.01%	0.002%
18	3.375	722	726	730	rVB2	387	334	0.02%	0.002%
19	3.478	755	758	759	rBV	455	228	0.01%	0.001%
20	3.503	764	766	769	rVB4	744	386	0.02%	0.002%
21	3.613	797	800	803	rVV3	456	261	0.01%	0.001%
22	3.805	857	860	864	rBV2	573	505	0.02%	0.003%
23	3.889	875	886	920	rBV2	151603	432425	19.65%	2.464%
24	4.352	1014	1030	1064	rBV	390167	961716	43.70%	5.480%
25	4.825	1173	1177	1178	rBV3	861	460	0.02%	0.003%
26	4.863	1187	1189	1192	rVB2	748	334	0.02%	0.002%
27	4.928	1207	1209	1211	rBV	365	231	0.01%	0.001%
28	4.992	1225	1229	1230	rBV3	582	359	0.02%	0.002%
29	5.050	1230	1247	1277	rBV2	854716	2200724	100.00%	12.541%
30	5.278	1316	1318	1322	rVB3	1115	711	0.03%	0.004%
31	5.494	1382	1385	1388	rBV3	1013	945	0.04%	0.005%
32	5.577	1409	1411	1412	rBV3	480	234	0.01%	0.001%
33	5.622	1412	1425	1449	rBV	759179	1522234	69.17%	8.674%
34	5.876	1502	1504	1505	rBV2	879	332	0.02%	0.002%
35	5.912	1506	1515	1529	rVV5	12077	24380	1.11%	0.139%
36	6.072	1552	1565	1591	rBV	487252	992465	45.10%	5.655%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020780.D
 Acq On : 27 Mar 2021 00:49
 Operator : SY/MD
 Sample : M1824-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4T5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	6.365	1654	1656	1658	rBV2	874	378	0.02%	0.002%
38	6.622	1734	1736	1741	rBV3	554	544	0.02%	0.003%
39	6.728	1767	1769	1771	rBV	663	304	0.01%	0.002%
40	6.866	1809	1812	1815	rVB2	592	431	0.02%	0.002%
41	6.886	1815	1818	1823	rVB3	987	769	0.03%	0.004%
42	6.915	1823	1827	1830	rBV3	794	635	0.03%	0.004%
43	6.989	1838	1850	1876	rBV	260342	488948	22.22%	2.786%
44	7.185	1909	1911	1912	rBV2	901	364	0.02%	0.002%
45	7.246	1928	1930	1932	rBV2	752	386	0.02%	0.002%
46	7.320	1941	1953	1975	rBV	971213	1675569	76.14%	9.548%
47	7.625	2038	2048	2073	rBV	191562	335420	15.24%	1.911%
48	7.924	2138	2141	2143	rBV2	1013	721	0.03%	0.004%
49	8.021	2169	2171	2172	rBV	576	259	0.01%	0.001%
50	8.091	2183	2193	2227	rBV	549813	997804	45.34%	5.686%
51	8.654	2366	2368	2370	rBV2	441	257	0.01%	0.001%
52	8.690	2377	2379	2383	rBV2	643	460	0.02%	0.003%
53	8.725	2386	2390	2392	rBV2	623	479	0.02%	0.003%
54	8.792	2407	2411	2412	rBV2	566	380	0.02%	0.002%
55	8.802	2412	2414	2418	rVB4	740	554	0.03%	0.003%
56	8.857	2418	2431	2449	rBV	1187348	1902440	86.45%	10.841%
57	9.236	2546	2549	2551	rBV3	758	505	0.02%	0.003%
58	9.281	2561	2563	2567	rVB3	644	490	0.02%	0.003%
59	9.320	2573	2575	2579	rVB3	748	296	0.01%	0.002%
60	9.336	2579	2580	2585	rVB	796	461	0.02%	0.003%
61	9.362	2585	2588	2594	rBV5	699	994	0.05%	0.006%
62	9.468	2618	2621	2627	rVB2	529	529	0.02%	0.003%
63	9.503	2628	2632	2633	rBV2	479	366	0.02%	0.002%
64	9.651	2676	2678	2682	rVB2	422	274	0.01%	0.002%
65	9.722	2696	2700	2705	rBV3	608	659	0.03%	0.004%
66	9.789	2717	2721	2724	rBV2	500	335	0.02%	0.002%
67	9.815	2726	2729	2730	rBV2	756	303	0.01%	0.002%
68	9.876	2746	2748	2752	rVB3	711	447	0.02%	0.003%
69	9.895	2752	2754	2757	rBV	549	270	0.01%	0.002%
70	10.069	2805	2808	2810	rBV3	713	414	0.02%	0.002%
71	10.091	2813	2815	2817	rBV	573	295	0.01%	0.002%
72	10.223	2843	2856	2880	rBV	721354	1137721	51.70%	6.483%
73	10.387	2904	2907	2913	rVV6	1795	1743	0.08%	0.010%
74	10.509	2943	2945	2947	rBV	523	316	0.01%	0.002%
75	10.532	2950	2952	2954	rVB2	699	238	0.01%	0.001%
76	10.757	3020	3022	3024	rBV2	404	261	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020780.D
 Acq On : 27 Mar 2021 00:49
 Operator : SY/MD
 Sample : M1824-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4T5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

77	10.808	3036	3038	3045	rVB3	654	486	0.02%	0.003%
78	10.834	3045	3046	3048	rBV	475	244	0.01%	0.001%
79	10.857	3048	3053	3059	rVB6	1252	1473	0.07%	0.008%
80	10.972	3087	3089	3090	rBV	651	266	0.01%	0.002%
81	11.017	3101	3103	3105	rBV	618	309	0.01%	0.002%
82	11.056	3112	3115	3118	rBV2	656	328	0.01%	0.002%
83	11.104	3124	3130	3136	rVB4	4144	5267	0.24%	0.030%
84	11.162	3140	3148	3160	rBV9	3408	5883	0.27%	0.034%
85	11.255	3165	3177	3199	rBV	1204029	1844161	83.80%	10.509%
86	11.468	3242	3243	3245	rBV	1119	432	0.02%	0.002%
87	11.522	3259	3260	3263	rBV2	479	255	0.01%	0.001%
88	11.567	3270	3274	3278	rVB4	1375	1091	0.05%	0.006%
89	11.587	3278	3280	3281	rBV	812	380	0.02%	0.002%
90	11.632	3281	3294	3314	rBV	1133246	1749911	79.52%	9.972%
91	12.152	3453	3456	3457	rBV	760	387	0.02%	0.002%
92	12.204	3470	3472	3477	rBV4	657	422	0.02%	0.002%
93	12.230	3477	3480	3482	rBV2	758	437	0.02%	0.002%
94	12.355	3513	3519	3531	rBV10	6785	10218	0.46%	0.058%
95	12.464	3550	3553	3557	rBV2	725	427	0.02%	0.002%
96	12.593	3590	3593	3596	rBV3	645	380	0.02%	0.002%
97	12.902	3688	3689	3695	rVB2	733	444	0.02%	0.003%
98	12.956	3703	3706	3708	rBV2	768	557	0.03%	0.003%
99	13.053	3734	3736	3738	rBV3	1011	436	0.02%	0.002%
100	14.040	4041	4043	4045	rBV2	895	462	0.02%	0.003%




Sum of corrected areas: 17548735

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020780.D
Acq On : 27 Mar 2021 00:49
Operator : SY/MD
Sample : M1824-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4T5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

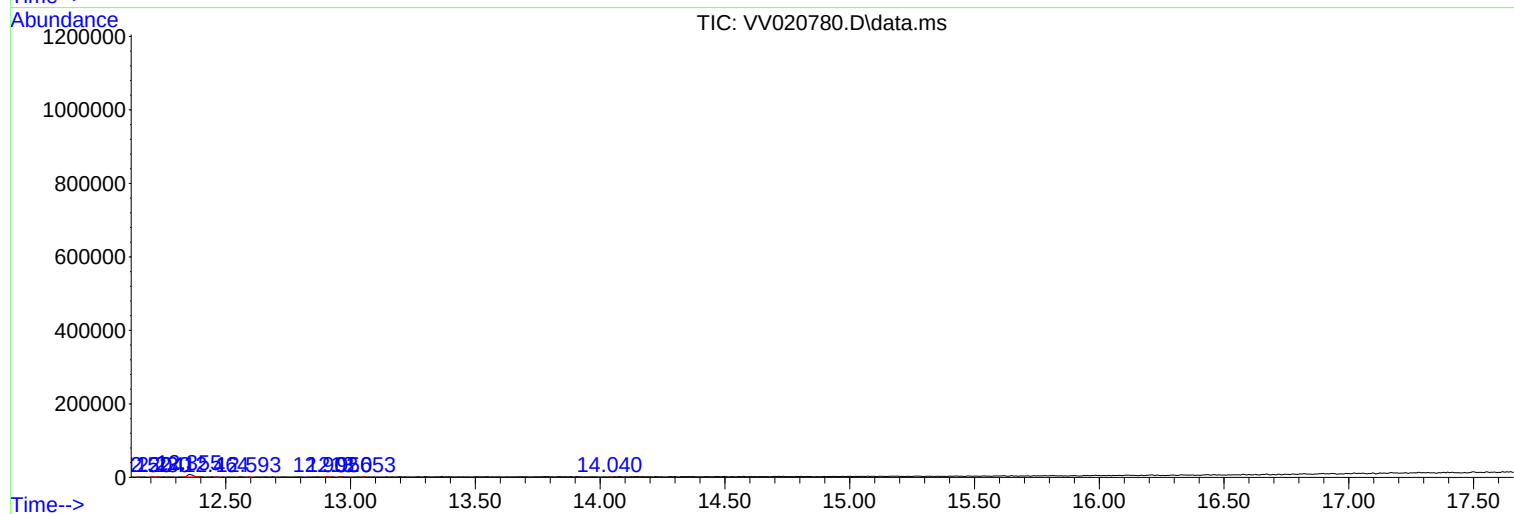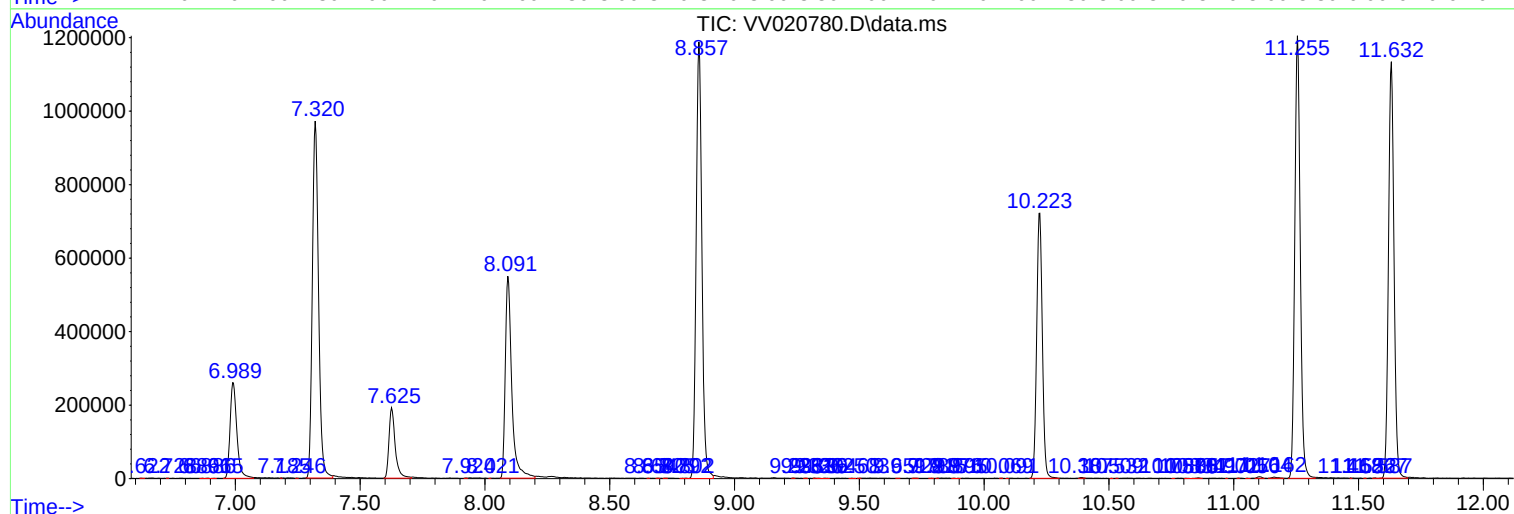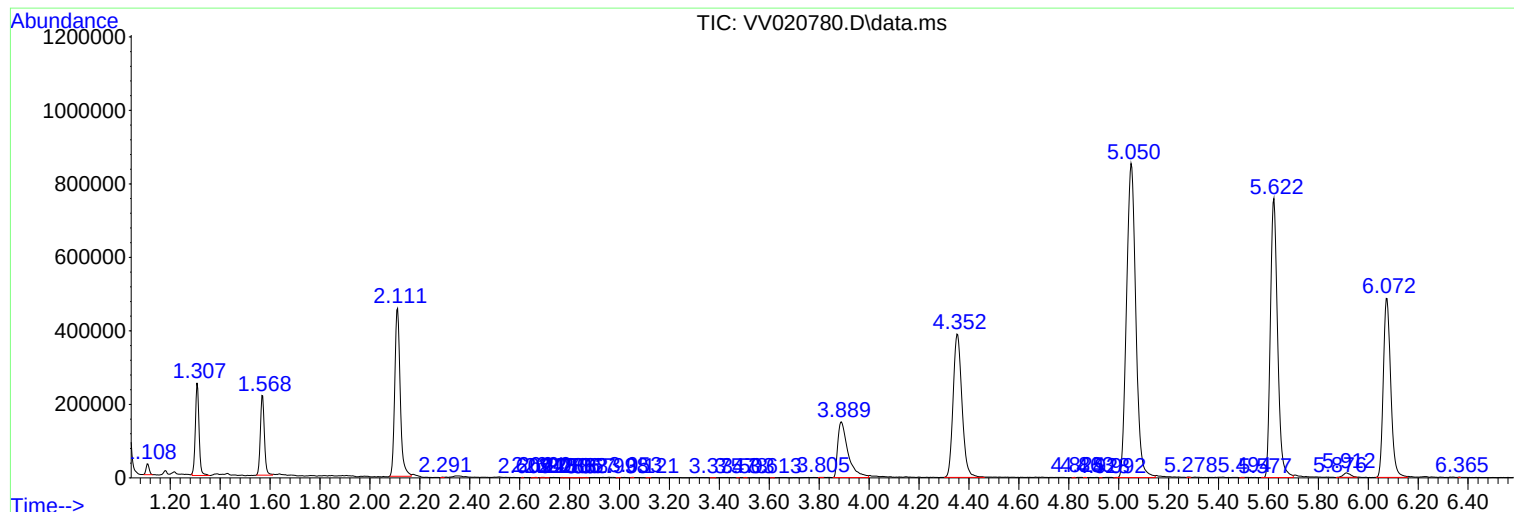

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020780.D
Acq On : 27 Mar 2021 00:49
Operator : SY/MD
Sample : M1824-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4T5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020780.D
Acq On : 27 Mar 2021 00:49
Operator : SY/MD
Sample : M1824-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4T5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
