

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020781.D
 Acq On : 27 Mar 2021 01:13
 Operator : SY/MD
 Sample : M1824-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4T6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020781.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.111	17	22	32	rVB	72968	68763	3.18%	0.391%
2	1.307	77	83	100	rVB	254734	266718	12.32%	1.517%
3	1.571	158	165	176	rVB	205898	229816	10.62%	1.308%
4	2.111	322	333	356	rBV	451332	690107	31.88%	3.926%
5	2.265	379	381	384	rVB3	942	486	0.02%	0.003%
6	2.294	385	390	391	rBV3	1154	887	0.04%	0.005%
7	2.593	481	483	488	rVB4	860	482	0.02%	0.003%
8	2.677	508	509	512	rBV2	478	239	0.01%	0.001%
9	2.741	523	529	530	rBV2	1968	1767	0.08%	0.010%
10	2.838	557	559	562	rVB2	619	325	0.02%	0.002%
11	2.854	562	564	567	rVB2	652	318	0.01%	0.002%
12	2.892	573	576	579	rBV2	967	664	0.03%	0.004%
13	2.953	592	595	596	rBV2	1038	598	0.03%	0.003%
14	3.008	610	612	615	rVB2	691	310	0.01%	0.002%
15	3.027	615	618	620	rBV	605	433	0.02%	0.002%
16	3.146	652	655	661	rVB2	513	452	0.02%	0.003%
17	3.204	671	673	678	rVB3	558	395	0.02%	0.002%
18	3.294	699	701	702	rBV3	613	200	0.01%	0.001%
19	3.330	710	712	715	rVB2	486	233	0.01%	0.001%
20	3.352	716	719	723	rVB2	280	198	0.01%	0.001%
21	3.371	723	725	728	rBV2	558	366	0.02%	0.002%
22	3.420	738	740	744	rVB	639	428	0.02%	0.002%
23	3.452	747	750	753	rVB3	616	364	0.02%	0.002%
24	3.513	767	769	772	rVB	425	210	0.01%	0.001%
25	3.539	772	777	781	rBV3	729	637	0.03%	0.004%
26	3.613	797	800	802	rVB	402	225	0.01%	0.001%
27	3.625	802	804	806	rBV	542	303	0.01%	0.002%
28	3.680	818	821	824	rBV2	450	262	0.01%	0.001%
29	3.696	824	826	829	rBV	483	219	0.01%	0.001%
30	3.889	876	886	918	rBV2	145232	415261	19.19%	2.363%
31	4.352	1015	1030	1065	rBV	381134	945540	43.69%	5.380%
32	4.895	1197	1199	1202	rBV3	538	299	0.01%	0.002%
33	4.934	1210	1211	1219	rVB4	676	461	0.02%	0.003%
34	5.050	1227	1247	1276	rBV2	834915	2164448	100.00%	12.314%
35	5.420	1359	1362	1366	rVB4	1132	781	0.04%	0.004%
36	5.503	1386	1388	1394	rBV4	912	677	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020781.D
 Acq On : 27 Mar 2021 01:13
 Operator : SY/MD
 Sample : M1824-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4T6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	5.622	1412	1425	1453	rBV	772134	1561173	72.13%	8.882%
38	6.002	1541	1543	1544	rBV	534	219	0.01%	0.001%
39	6.075	1552	1566	1592	rBV	479001	979151	45.24%	5.571%
40	6.493	1693	1696	1698	rBV3	687	317	0.01%	0.002%
41	6.529	1704	1707	1713	rBV5	1110	1023	0.05%	0.006%
42	6.616	1732	1734	1736	rBV	687	308	0.01%	0.002%
43	6.641	1740	1742	1746	rBV3	947	874	0.04%	0.005%
44	6.799	1787	1791	1795	rBV2	836	466	0.02%	0.003%
45	6.818	1795	1797	1799	rBV2	1018	463	0.02%	0.003%
46	6.857	1806	1809	1810	rBV	587	262	0.01%	0.001%
47	6.870	1810	1813	1815	rBV2	736	547	0.03%	0.003%
48	6.992	1839	1851	1879	rBV	262425	478250	22.10%	2.721%
49	7.320	1941	1953	1975	rBV	953095	1652597	76.35%	9.402%
50	7.625	2038	2048	2072	rBV	190719	331373	15.31%	1.885%
51	7.863	2116	2122	2125	rBV5	1213	1114	0.05%	0.006%
52	7.985	2158	2160	2162	rBV2	1092	610	0.03%	0.003%
53	8.037	2174	2176	2178	rBV2	1038	652	0.03%	0.004%
54	8.091	2183	2193	2235	rVV	538091	991175	45.79%	5.639%
55	8.522	2325	2327	2328	rBV	595	268	0.01%	0.002%
56	8.625	2358	2359	2362	rBV2	656	344	0.02%	0.002%
57	8.670	2370	2373	2378	rBV5	587	501	0.02%	0.003%
58	8.757	2397	2400	2403	rBV5	973	552	0.03%	0.003%
59	8.857	2416	2431	2452	rBV	1209813	1954463	90.30%	11.120%
60	9.050	2489	2491	2503	rVB6	1220	1644	0.08%	0.009%
61	9.114	2508	2511	2516	rVB3	827	683	0.03%	0.004%
62	9.140	2516	2519	2520	rBV	1299	775	0.04%	0.004%
63	9.268	2557	2559	2563	rVB3	888	528	0.02%	0.003%
64	9.310	2568	2572	2573	rBV	571	356	0.02%	0.002%
65	9.413	2602	2604	2606	rBV2	481	325	0.02%	0.002%
66	9.493	2623	2629	2633	rBV5	1281	1636	0.08%	0.009%
67	9.609	2663	2665	2666	rBV	454	205	0.01%	0.001%
68	9.632	2669	2672	2676	rBV3	878	730	0.03%	0.004%
69	9.689	2687	2690	2694	rBV2	514	331	0.02%	0.002%
70	9.776	2715	2717	2721	rVB2	740	318	0.01%	0.002%
71	9.799	2721	2724	2726	rBV3	581	305	0.01%	0.002%
72	9.828	2729	2733	2735	rBV3	1010	783	0.04%	0.004%
73	9.989	2780	2783	2788	rBV4	1039	767	0.04%	0.004%
74	10.223	2842	2856	2877	rBV	720615	1136663	52.52%	6.467%
75	10.525	2947	2950	2953	rBV3	899	751	0.03%	0.004%
76	10.619	2977	2979	2980	rBV	813	294	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020781.D
 Acq On : 27 Mar 2021 01:13
 Operator : SY/MD
 Sample : M1824-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4T6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

77	10.644	2985	2987	2988	rBV	667	205	0.01%	0.001%
78	10.792	3031	3033	3039	rVB3	764	654	0.03%	0.004%
79	10.818	3039	3041	3043	rBV4	670	373	0.02%	0.002%
80	10.853	3050	3052	3054	rBV2	1076	596	0.03%	0.003%
81	10.966	3085	3087	3089	rBV3	1006	531	0.02%	0.003%
82	11.030	3104	3107	3109	rBV2	647	438	0.02%	0.002%
83	11.107	3120	3131	3141	rVB4	5446	9569	0.44%	0.054%
84	11.162	3141	3148	3150	rBV5	3855	4075	0.19%	0.023%
85	11.255	3166	3177	3200	rBV	1234948	1904447	87.99%	10.835%
86	11.538	3263	3265	3267	rBV	741	328	0.02%	0.002%
87	11.574	3274	3276	3279	rVB4	654	257	0.01%	0.001%
88	11.632	3282	3294	3316	rVV	1113792	1740977	80.44%	9.905%
89	11.837	3356	3358	3359	rBV2	872	405	0.02%	0.002%
90	11.902	3376	3378	3380	rVB3	1055	447	0.02%	0.003%
91	11.914	3380	3382	3384	rBV	1229	686	0.03%	0.004%
92	12.085	3433	3435	3440	rBV3	932	764	0.04%	0.004%
93	12.239	3479	3483	3486	rBV3	881	709	0.03%	0.004%
94	12.358	3513	3520	3530	rVB5	7716	10679	0.49%	0.061%
95	12.474	3552	3556	3557	rBV2	748	558	0.03%	0.003%
96	12.705	3624	3628	3630	rBV3	897	647	0.03%	0.004%
97	12.992	3715	3717	3718	rBV	532	209	0.01%	0.001%
98	13.107	3751	3753	3756	rBV2	648	342	0.02%	0.002%
99	13.323	3818	3820	3829	rVB4	771	726	0.03%	0.004%
100	13.644	3919	3920	3923	rBV2	731	256	0.01%	0.001%




Sum of corrected areas: 17576546

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020781.D
Acq On : 27 Mar 2021 01:13
Operator : SY/MD
Sample : M1824-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4T6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

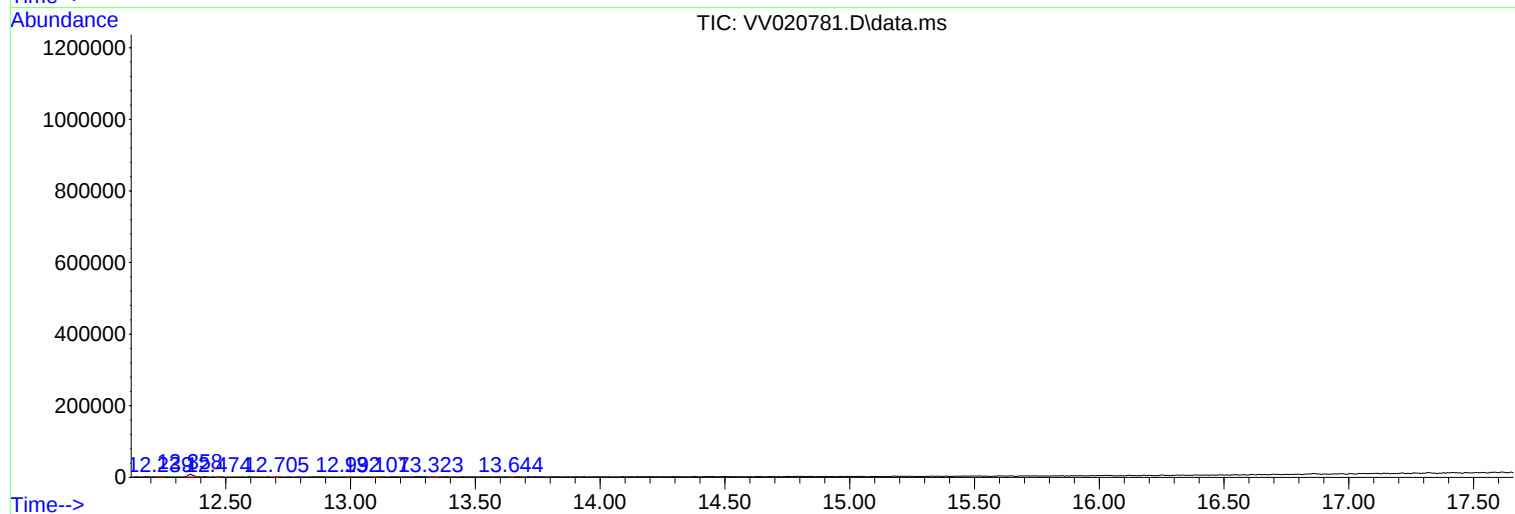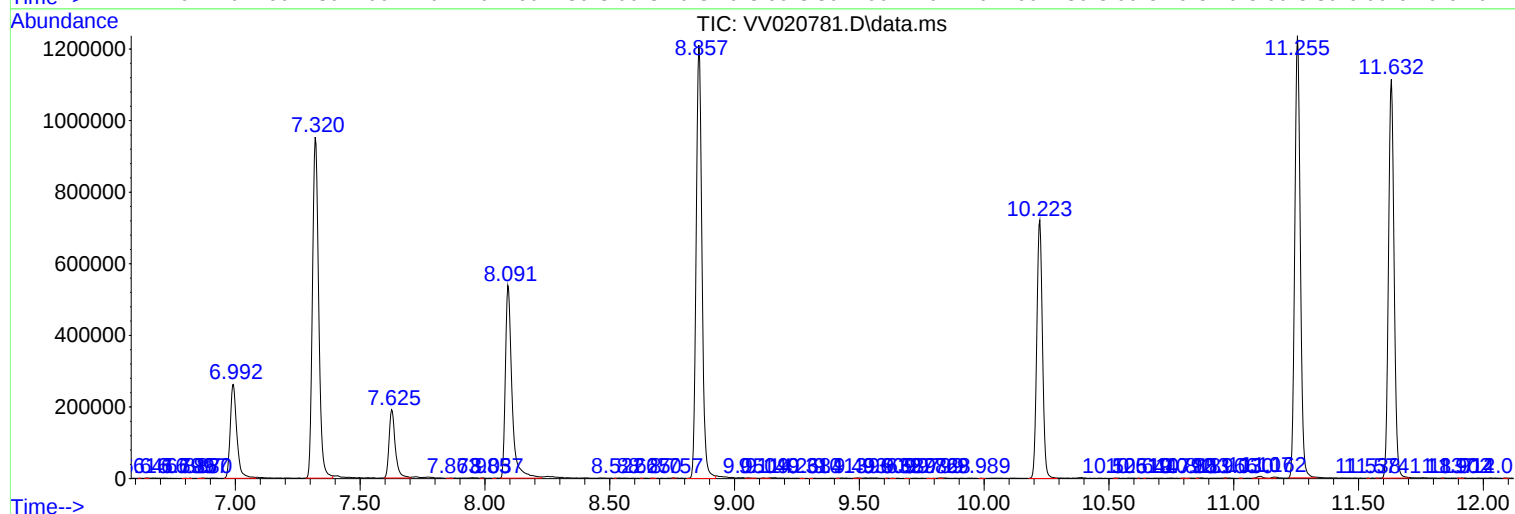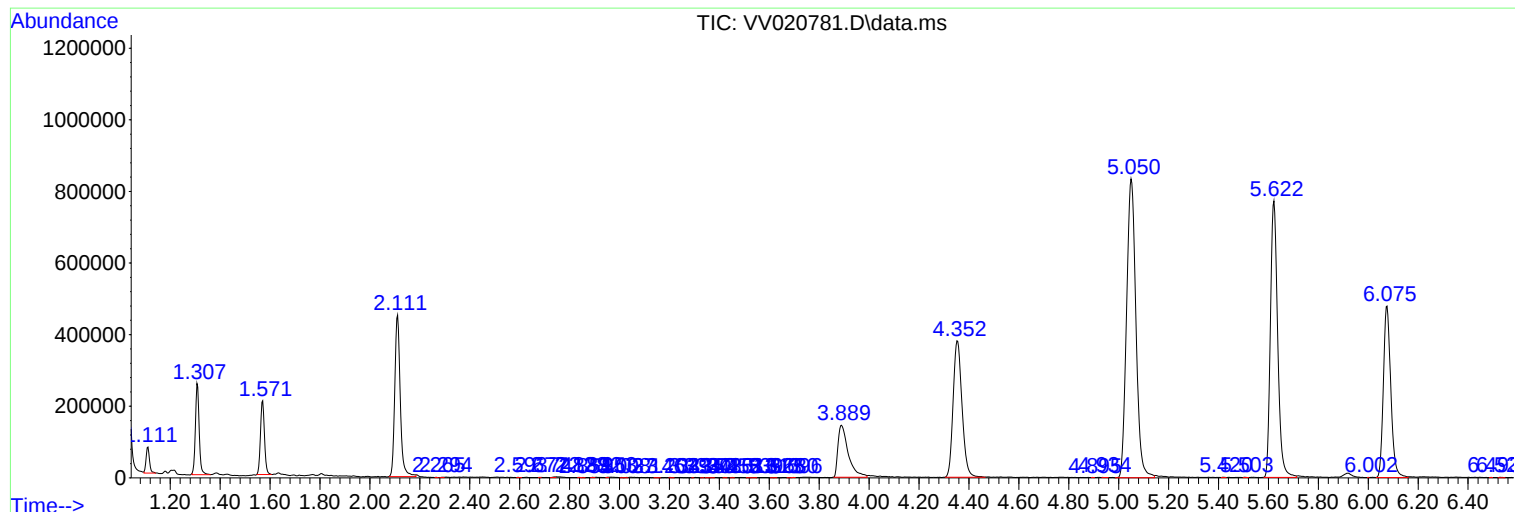

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020781.D
Acq On : 27 Mar 2021 01:13
Operator : SY/MD
Sample : M1824-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4T6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020781.D
Acq On : 27 Mar 2021 01:13
Operator : SY/MD
Sample : M1824-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4T6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
