

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020785.D
 Acq On : 27 Mar 2021 02:47
 Operator : SY/MD
 Sample : M1824-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4W3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020785.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	97	rVB	304757	305675	12.97%	1.658%
2	1.568	157	164	182	rVB	253108	282871	12.00%	1.534%
3	2.111	322	333	361	rVB	548197	827250	35.10%	4.487%
4	2.510	452	457	458	rBV4	1632	1713	0.07%	0.009%
5	2.558	469	472	475	rBV5	578	428	0.02%	0.002%
6	2.606	485	487	490	rBV3	618	305	0.01%	0.002%
7	2.744	529	530	536	rVB2	639	458	0.02%	0.002%
8	2.770	536	538	541	rBV3	811	388	0.02%	0.002%
9	2.793	542	545	550	rVV4	824	654	0.03%	0.004%
10	2.831	554	557	559	rBV2	542	294	0.01%	0.002%
11	2.847	559	562	565	rVB2	405	263	0.01%	0.001%
12	2.960	592	597	600	rVB4	367	338	0.01%	0.002%
13	2.982	600	604	606	rBV3	422	303	0.01%	0.002%
14	3.043	621	623	627	rVV3	535	436	0.02%	0.002%
15	3.314	703	707	709	rBV3	458	369	0.02%	0.002%
16	3.397	728	733	734	rBV	615	270	0.01%	0.001%
17	3.455	749	751	754	rVV3	621	286	0.01%	0.002%
18	3.519	769	771	776	rBV2	377	274	0.01%	0.001%
19	3.751	841	843	846	rBV2	763	417	0.02%	0.002%
20	3.886	873	885	921	rBV	150717	434711	18.45%	2.358%
21	4.262	998	1002	1006	rBV4	971	973	0.04%	0.005%
22	4.352	1015	1030	1054	rBV2	402578	998174	42.35%	5.415%
23	4.738	1148	1150	1151	rBV2	699	324	0.01%	0.002%
24	4.828	1175	1178	1179	rBV	616	341	0.01%	0.002%
25	4.879	1190	1194	1196	rBV2	871	595	0.03%	0.003%
26	4.921	1202	1207	1209	rBV3	534	380	0.02%	0.002%
27	5.050	1228	1247	1275	rBV2	917518	2356715	100.00%	12.784%
28	5.397	1352	1355	1359	rBV3	804	603	0.03%	0.003%
29	5.420	1359	1362	1367	rVV6	985	925	0.04%	0.005%
30	5.455	1370	1373	1375	rBV3	576	416	0.02%	0.002%
31	5.545	1398	1401	1404	rBV3	364	288	0.01%	0.002%
32	5.622	1409	1425	1450	rBV	778706	1559768	66.18%	8.461%
33	5.918	1508	1517	1531	rVB10	13349	29245	1.24%	0.159%
34	6.076	1551	1566	1595	rVV	516081	1046356	44.40%	5.676%
35	6.285	1629	1631	1637	rBV4	891	677	0.03%	0.004%
36	6.375	1654	1659	1661	rBV3	622	507	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020785.D
 Acq On : 27 Mar 2021 02:47
 Operator : SY/MD
 Sample : M1824-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4W3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	6.429	1674	1676	1678	rBV	583	323	0.01%	0.002%
38	6.465	1686	1687	1691	rVB2	600	319	0.01%	0.002%
39	6.503	1695	1699	1700	rBV2	519	259	0.01%	0.001%
40	6.551	1712	1714	1716	rBV2	507	275	0.01%	0.001%
41	6.744	1772	1774	1776	rBV3	871	389	0.02%	0.002%
42	6.757	1776	1778	1784	rVB2	889	606	0.03%	0.003%
43	6.789	1786	1788	1792	rBV3	376	302	0.01%	0.002%
44	6.860	1804	1810	1812	rVV4	477	468	0.02%	0.003%
45	6.928	1829	1831	1833	rBV2	477	317	0.01%	0.002%
46	6.992	1838	1851	1880	rBV	272204	511607	21.71%	2.775%
47	7.230	1921	1925	1928	rBV4	1195	1005	0.04%	0.005%
48	7.320	1941	1953	1973	rBV	1076381	1863476	79.07%	10.108%
49	7.625	2038	2048	2075	rBV	195365	353591	15.00%	1.918%
50	7.934	2139	2144	2146	rBV5	2043	1824	0.08%	0.010%
51	8.030	2171	2174	2176	rBV3	418	272	0.01%	0.001%
52	8.092	2183	2193	2226	rBV	554623	1010644	42.88%	5.482%
53	8.506	2320	2322	2326	rVB2	689	380	0.02%	0.002%
54	8.706	2380	2384	2386	rBV4	826	617	0.03%	0.003%
55	8.735	2391	2393	2397	rBV2	502	345	0.01%	0.002%
56	8.857	2419	2431	2459	rBV	1206279	1947625	82.64%	10.565%
57	9.233	2546	2548	2550	rBV3	569	285	0.01%	0.002%
58	9.265	2550	2558	2560	rBV4	716	800	0.03%	0.004%
59	9.278	2560	2562	2564	rBV2	686	343	0.01%	0.002%
60	9.329	2577	2578	2583	rVB2	540	277	0.01%	0.002%
61	9.362	2585	2588	2593	rBV3	736	608	0.03%	0.003%
62	9.497	2627	2630	2632	rBV	517	344	0.01%	0.002%
63	9.529	2637	2640	2642	rBV2	606	450	0.02%	0.002%
64	9.558	2647	2649	2651	rBV2	951	417	0.02%	0.002%
65	9.583	2655	2657	2659	rBV2	503	275	0.01%	0.001%
66	9.609	2661	2665	2666	rBV	617	410	0.02%	0.002%
67	9.815	2726	2729	2733	rBV2	611	457	0.02%	0.002%
68	9.918	2759	2761	2766	rVB2	598	462	0.02%	0.003%
69	9.963	2773	2775	2778	rBV	547	321	0.01%	0.002%
70	9.979	2778	2780	2782	rBV3	468	278	0.01%	0.002%
71	10.146	2830	2832	2836	rVB2	549	347	0.01%	0.002%
72	10.169	2836	2839	2840	rBV2	794	396	0.02%	0.002%
73	10.223	2843	2856	2875	rVV	731283	1146965	48.67%	6.222%
74	10.384	2901	2906	2912	rBV6	1434	1978	0.08%	0.011%
75	10.609	2971	2976	2979	rBV4	822	830	0.04%	0.005%
76	10.680	2993	2998	3000	rBV3	1012	830	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020785.D
 Acq On : 27 Mar 2021 02:47
 Operator : SY/MD
 Sample : M1824-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4W3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

77	10.767	3023	3025	3029	rVB2	560	362	0.02%	0.002%
78	10.812	3036	3039	3043	rBV4	754	538	0.02%	0.003%
79	10.863	3047	3055	3061	rBV6	1638	1991	0.08%	0.011%
80	10.898	3063	3066	3067	rBV6	445	260	0.01%	0.001%
81	11.107	3124	3131	3141	rVB5	4253	6360	0.27%	0.034%
82	11.156	3143	3146	3147	rBV	642	349	0.01%	0.002%
83	11.198	3155	3159	3163	rBV3	646	515	0.02%	0.003%
84	11.255	3163	3177	3197	rBV	1253291	1903999	80.79%	10.328%
85	11.522	3257	3260	3264	rBV3	909	815	0.03%	0.004%
86	11.632	3278	3294	3324	rBV	1149170	1806856	76.67%	9.801%
87	11.818	3350	3352	3358	rVB3	731	421	0.02%	0.002%
88	11.898	3374	3377	3381	rBV3	727	676	0.03%	0.004%
89	11.940	3389	3390	3392	rVB	1097	254	0.01%	0.001%
90	11.979	3396	3402	3405	rBV4	1044	1164	0.05%	0.006%
91	12.027	3415	3417	3419	rBV2	495	258	0.01%	0.001%
92	12.191	3464	3468	3470	rBV2	752	547	0.02%	0.003%
93	12.291	3497	3499	3501	rBV2	739	398	0.02%	0.002%
94	12.358	3518	3520	3522	rBV	775	453	0.02%	0.002%
95	12.381	3522	3527	3529	rBV2	943	894	0.04%	0.005%
96	12.718	3629	3632	3636	rBV2	721	559	0.02%	0.003%
97	12.821	3662	3664	3666	rVB	883	350	0.01%	0.002%
98	12.850	3671	3673	3675	rBV	774	383	0.02%	0.002%
99	12.914	3691	3693	3696	rBV2	561	299	0.01%	0.002%
100	13.165	3768	3771	3773	rBV2	973	561	0.02%	0.003%




Sum of corrected areas: 18434969

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020785.D
Acq On : 27 Mar 2021 02:47
Operator : SY/MD
Sample : M1824-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4W3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

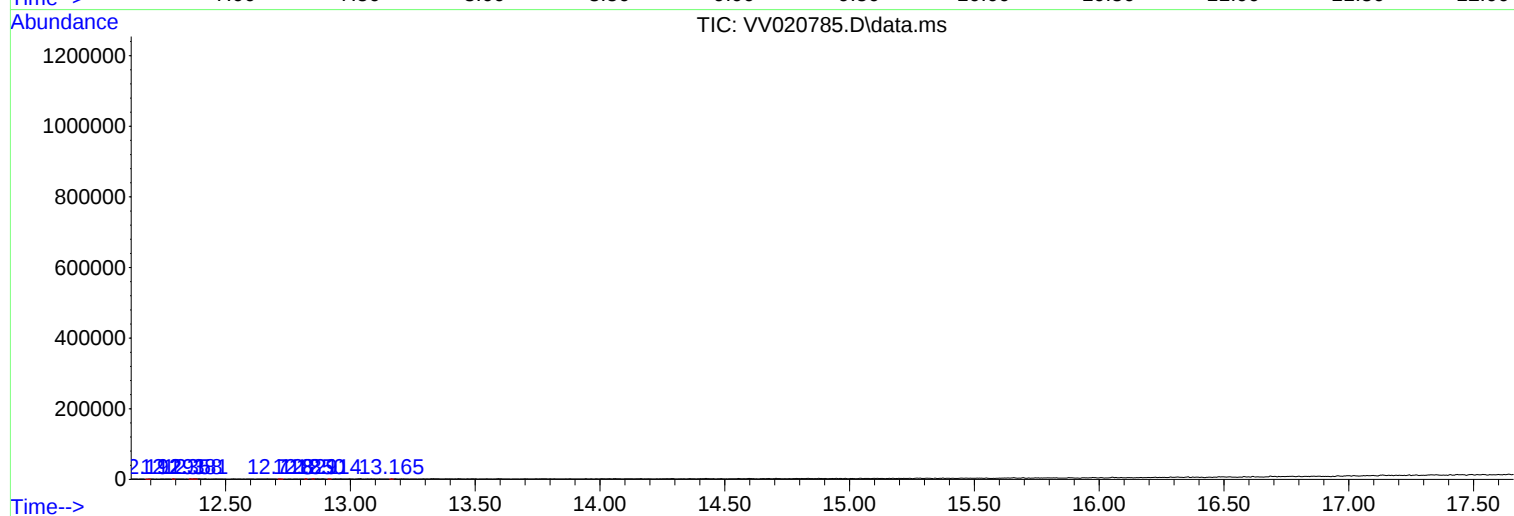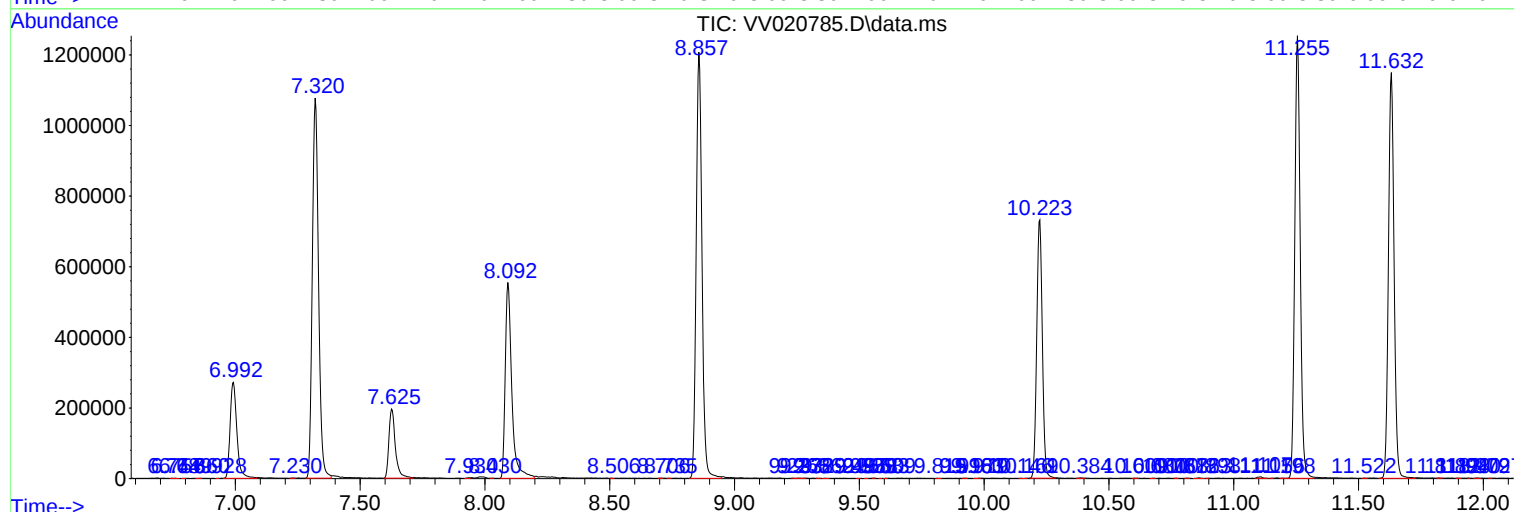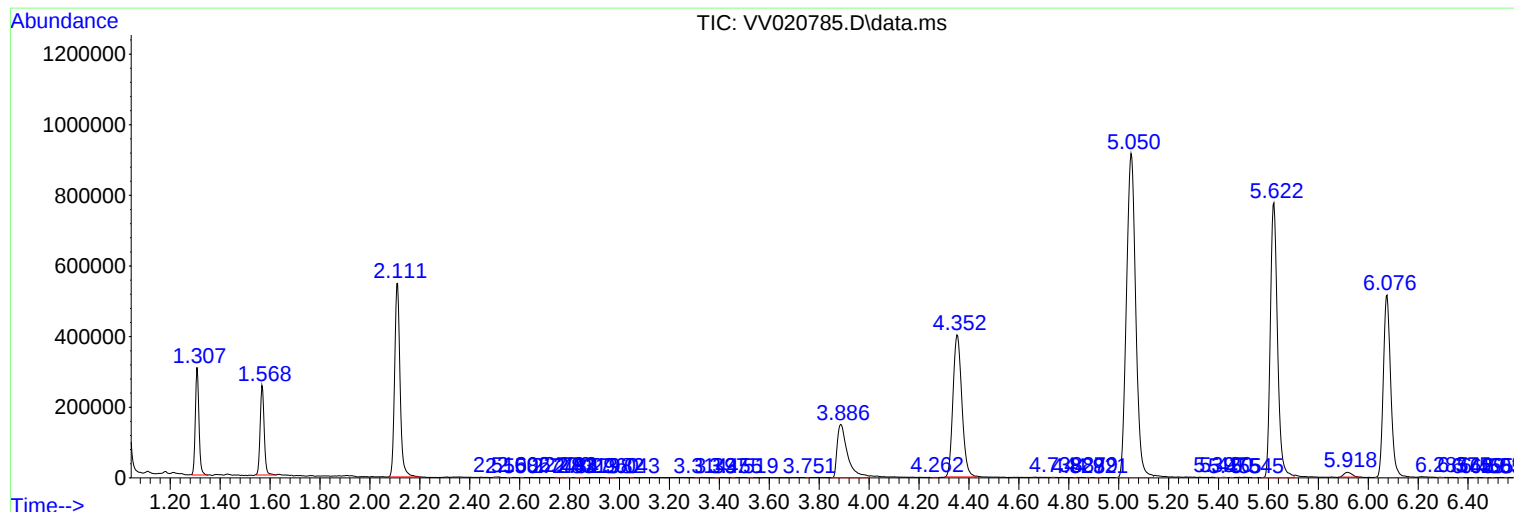

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020785.D
Acq On : 27 Mar 2021 02:47
Operator : SY/MD
Sample : M1824-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4W3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
Data File : VV020785.D
Acq On : 27 Mar 2021 02:47
Operator : SY/MD
Sample : M1824-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4W3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------