
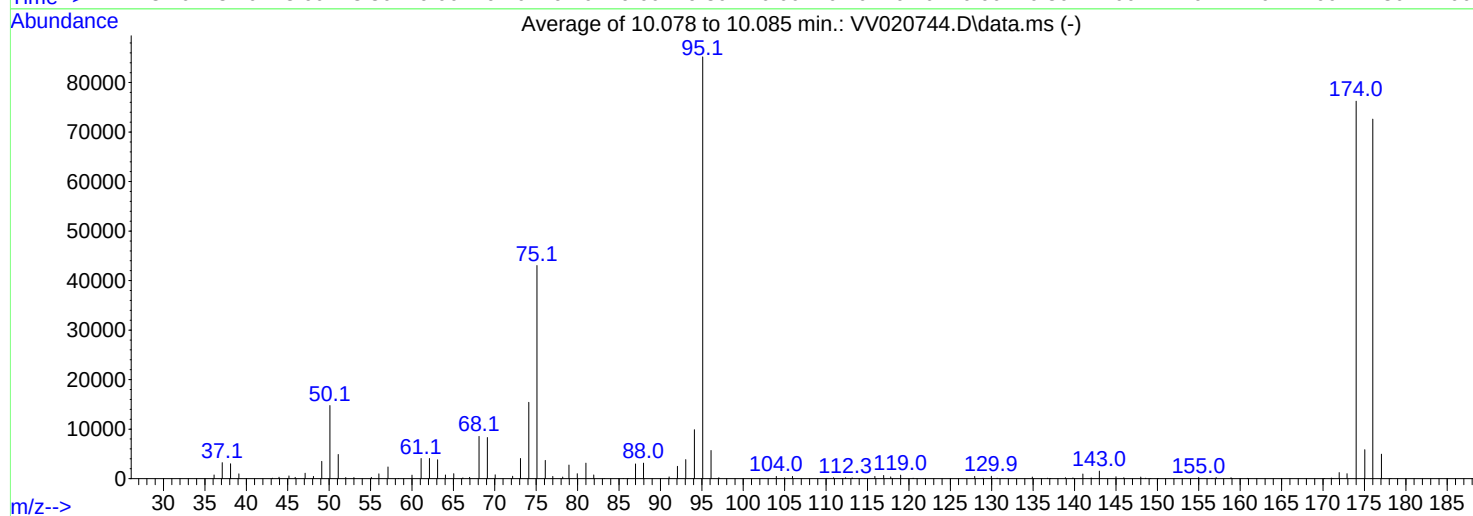


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032621\
 Data File : VV020744.D
 Acq On : 26 Mar 2021 09:56
 Operator : SY/MD
 Sample : BFB69
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB69

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis
 Last Update : Sat Mar 27 08:21:41 2021

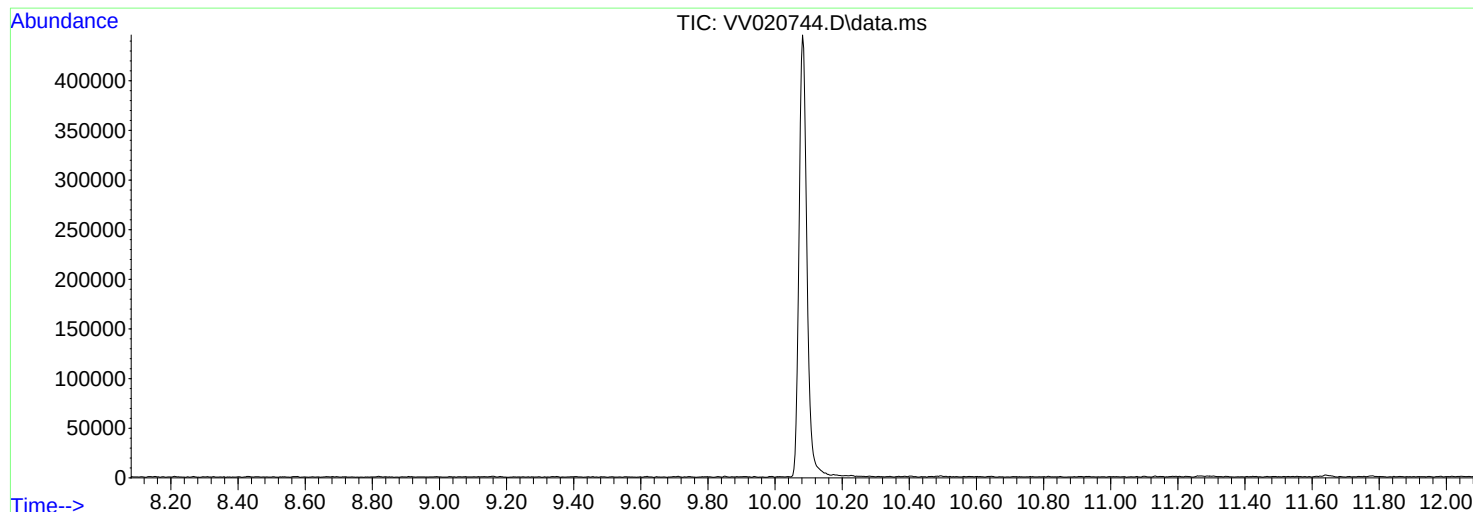

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	14762	PASS
75	95	30	80	50.5	43040	PASS
95	95	100	100	100.0	85189	PASS
96	95	5	9	6.7	5677	PASS
173	174	0.00	2	1.3	1006	PASS
174	95	50	120	89.5	76229	PASS
175	174	5	9	7.7	5851	PASS
176	174	95	101	95.3	72624	PASS
177	176	5	9	6.8	4932	PASS

m/z	Abundance
39.10	117.0
40.10	378.0
41.60	101.0
43.90	544.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

m/z	Abundance
36.10	583.0
37.10	3166.0
38.10	2731.0
39.10	917.0
40.00	276.0
43.20	105.0
44.10	766.0
45.10	506.0
45.90	235.0
47.10	1106.0
48.10	369.0
49.10	3747.0
50.10	15131.0
51.10	4718.0
52.00	264.0
53.00	199.0
55.10	326.0
56.00	1055.0
57.10	2235.0
58.40	138.0
60.00	666.0
61.10	4227.0
62.10	4068.0
63.10	3629.0
64.10	679.0
65.00	868.0
66.20	181.0
67.00	271.0
68.10	8281.0
69.10	8631.0
70.10	778.0
72.20	343.0
73.10	4082.0
74.10	15237.0
75.10	42408.0
76.10	3540.0
77.00	458.0
78.20	340.0
79.00	2723.0
80.00	995.0
81.00	3087.0
82.00	709.0
83.20	102.0
85.50	114.0
87.00	3222.0
88.00	3131.0
91.00	417.0
92.10	2304.0
93.10	4158.0
94.10	9538.0
95.10	85192.0
96.10	5635.0
97.00	132.0
104.00	422.0
105.00	109.0
105.90	470.0
110.10	128.0
110.90	193.0
112.30	244.0
113.20	206.0
115.90	532.0
116.90	699.0
117.80	416.0
119.00	628.0
120.50	124.0
127.90	407.0
129.90	413.0
130.70	138.0
134.90	402.0
136.70	176.0
138.90	178.0
139.80	202.0
141.00	1042.0
142.10	175.0
143.00	1578.0
145.00	321.0
145.90	157.0
148.00	321.0
155.00	257.0
157.10	229.0
158.90	224.0
171.20	141.0
172.00	1252.0
172.80	996.0
174.00	77168.0
175.00	5673.0
176.00	73408.0
177.00	5000.0
178.20	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

m/z	Abundance
36.10	784.0
37.10	3250.0
38.10	3045.0
39.10	1075.0
40.10	278.0
43.10	105.0
44.00	836.0
45.20	571.0
45.90	280.0
47.10	1125.0
48.10	466.0
49.10	3705.0
50.10	15275.0
51.10	5029.0
52.00	257.0
53.00	244.0
55.10	279.0
56.00	988.0
57.10	2441.0
60.00	707.0
61.10	4156.0
62.10	4214.0
63.10	4026.0
64.00	793.0
65.10	1000.0
66.20	185.0
67.00	235.0
68.10	8960.0
69.10	8461.0
70.10	771.0
72.20	482.0
73.10	4175.0
74.10	15992.0
75.10	44568.0
76.10	3727.0
77.00	448.0
78.20	331.0
79.00	2782.0
79.90	1015.0
81.00	3278.0
82.00	785.0
87.00	3041.0
87.90	3267.0
91.00	362.0
92.10	2595.0
93.00	3949.0
94.10	10169.0
95.10	87472.0
96.10	5825.0
97.00	192.0
104.00	487.0
105.00	171.0
105.90	486.0
110.10	119.0
110.90	190.0
112.30	230.0
113.20	182.0
114.70	103.0
115.90	413.0
116.90	666.0
117.80	340.0
119.00	742.0
120.50	135.0
128.00	526.0
129.00	109.0
130.00	530.0
130.60	147.0
134.90	331.0
136.80	157.0
138.90	239.0
139.80	197.0
141.00	987.0
142.00	174.0
143.00	1594.0
145.00	408.0
145.90	168.0
148.00	356.0
148.60	132.0
155.00	275.0
156.60	125.0
157.10	245.0
158.90	204.0
171.00	176.0
172.00	1243.0
172.90	999.0
174.00	78904.0
175.00	6053.0
176.00	74536.0
177.00	5024.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

m/z	Abundance
36.10	866.0
37.10	3324.0
38.10	3204.0
39.10	1277.0
40.20	295.0
43.10	114.0
44.00	940.0
45.20	562.0
45.90	219.0
47.10	1026.0
48.10	519.0
49.10	3037.0
50.10	13879.0
51.10	4910.0
52.00	204.0
53.00	219.0
55.10	187.0
56.00	890.0
57.10	2393.0
60.00	746.0
61.10	3854.0
62.10	3938.0
63.10	3803.0
64.00	746.0
65.10	1126.0
66.10	162.0
66.90	254.0
68.10	8371.0
69.10	7859.0
70.00	783.0
72.10	597.0
73.10	3955.0
74.10	15038.0
75.10	42144.0
76.10	3789.0
77.00	501.0
78.20	338.0
78.90	2720.0
80.00	1006.0
81.00	3062.0
81.90	768.0
86.10	132.0
87.00	2671.0
87.90	2992.0
91.10	288.0
92.00	2618.0
93.00	3421.0
94.10	9933.0
95.10	82904.0
96.10	5570.0
97.10	220.0
104.00	460.0
105.00	192.0
106.00	381.0
110.90	171.0
112.00	115.0
112.40	140.0
113.10	108.0
115.90	391.0
117.00	536.0
117.80	277.0
119.00	754.0
121.80	127.0
128.00	466.0
128.90	155.0
129.90	479.0
134.90	221.0
137.10	154.0
138.90	209.0
139.80	137.0
141.00	822.0
141.90	189.0
143.00	1412.0
145.00	444.0
146.00	245.0
148.00	312.0
148.60	122.0
149.20	134.0
150.10	134.0
155.00	218.0
156.60	122.0
157.10	211.0
158.90	148.0
160.90	158.0
170.20	137.0
171.00	223.0
171.90	1167.0
173.00	1023.0
174.00	72616.0
175.10	5827.0
176.00	69928.0
177.10	4772.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69