

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VW032624\  
 Data File : VW034831.D  
 Acq On : 26 Mar 2024 16:41  
 Operator : SY/MD  
 Sample : P1851-02  
 Misc : 5.0mL/MSVOA\_V/WATER  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 E0LX1

Quant Time: Mar 27 01:36:35 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM032624WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Wed Mar 27 01:34:52 2024  
 Response via : Initial Calibration


| Compound                      | R.T.    | QIon           | Response | Conc    | Units     | Dev(Min)  |
|-------------------------------|---------|----------------|----------|---------|-----------|-----------|
| -----                         |         |                |          |         |           |           |
| Internal Standards            |         |                |          |         |           |           |
| 1) 1,4-Difluorobenzene        | 5.535   | 114            | 144470   | 50.000  | ug/L      | 0.00      |
| 28) Chlorobenzene-d5          | 8.783   | 117            | 138845   | 50.000  | ug/L      | 0.00      |
| 58) 1,4-Dichlorobenzene-d4    | 11.185  | 152            | 64796    | 50.000  | ug/L      | 0.00      |
| System Monitoring Compounds   |         |                |          |         |           |           |
| 4) Vinyl Chloride-d3          | 1.278   | 65             | 136452   | 97.799  | ug/L      | 0.00      |
| Spiked Amount                 | 50.000  | Range 60 - 135 | Recovery | =       | 195.600%# |           |
| 7) Chloroethane-d5            | 1.532   | 69             | 115557   | 95.356  | ug/L      | 0.00      |
| Spiked Amount                 | 50.000  | Range 70 - 130 | Recovery | =       | 190.720%# |           |
| 11) 1,1-Dichloroethene-d2     | 2.060   | 65             | 59910    | 97.957  | ug/L      | 0.00      |
| Spiked Amount                 | 50.000  | Range 60 - 125 | Recovery | =       | 195.920%# |           |
| 21) 2-Butanone-d5             | 3.786   | 46             | 150145   | 181.449 | ug/L      | 0.00      |
| Spiked Amount                 | 100.000 | Range 40 - 130 | Recovery | =       | 181.450%# |           |
| 24) Chloroform-d              | 4.246   | 84             | 225292   | 96.040  | ug/L      | 0.00      |
| Spiked Amount                 | 50.000  | Range 70 - 125 | Recovery | =       | 192.080%# |           |
| 26) 1,2-Dichloroethane-d4     | 4.937   | 65             | 149822   | 100.596 | ug/L      | 0.00      |
| Spiked Amount                 | 50.000  | Range 70 - 125 | Recovery | =       | 201.200%# |           |
| 32) Benzene-d6                | 4.957   | 84             | 464442   | 99.583  | ug/L      | 0.00      |
| Spiked Amount                 | 50.000  | Range 70 - 125 | Recovery | =       | 199.160%# |           |
| 36) 1,2-Dichloropropane-d6    | 5.986   | 67             | 150470   | 101.600 | ug/L      | 0.00      |
| Spiked Amount                 | 50.000  | Range 70 - 120 | Recovery | =       | 203.200%# |           |
| 41) Toluene-d8                | 7.243   | 98             | 406426   | 96.763  | ug/L      | 0.00      |
| Spiked Amount                 | 50.000  | Range 80 - 120 | Recovery | =       | 193.520%# |           |
| 43) trans-1,3-Dichloroprop... | 7.551   | 79             | 66273    | 92.048  | ug/L      | 0.00      |
| Spiked Amount                 | 50.000  | Range 60 - 125 | Recovery | =       | 184.100%# |           |
| 47) 2-Hexanone-d5             | 8.024   | 63             | 97560    | 174.232 | ug/L      | 0.00      |
| Spiked Amount                 | 100.000 | Range 45 - 130 | Recovery | =       | 174.230%# |           |
| 56) 1,1,2,2-Tetrachloroeth... | 10.149  | 84             | 196417   | 96.308  | ug/L      | 0.00      |
| Spiked Amount                 | 50.000  | Range 65 - 120 | Recovery | =       | 192.620%# |           |
| 66) 1,2-Dichlorobenzene-d4    | 11.558  | 152            | 142832   | 98.179  | ug/L      | 0.00      |
| Spiked Amount                 | 50.000  | Range 80 - 120 | Recovery | =       | 196.360%# |           |
| Target Compounds              |         |                |          |         |           |           |
| 13) Acetone                   | 2.118   | 43             | 3069     | 4.040   | ug/L      | Qvalue 91 |
| -----                         |         |                |          |         |           |           |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV032624\  
Data File : VV034831.D  
Acq On : 26 Mar 2024 16:41  
Operator : SY/MD  
Sample : P1851-02  
Misc : 5.0mL/MSVOA\_V/WATER  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
E0LX1

Quant Time: Mar 27 01:36:35 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM032624WMA.M  
Quant Title : VOC Analysis  
QLast Update : Wed Mar 27 01:34:52 2024  
Response via : Initial Calibration

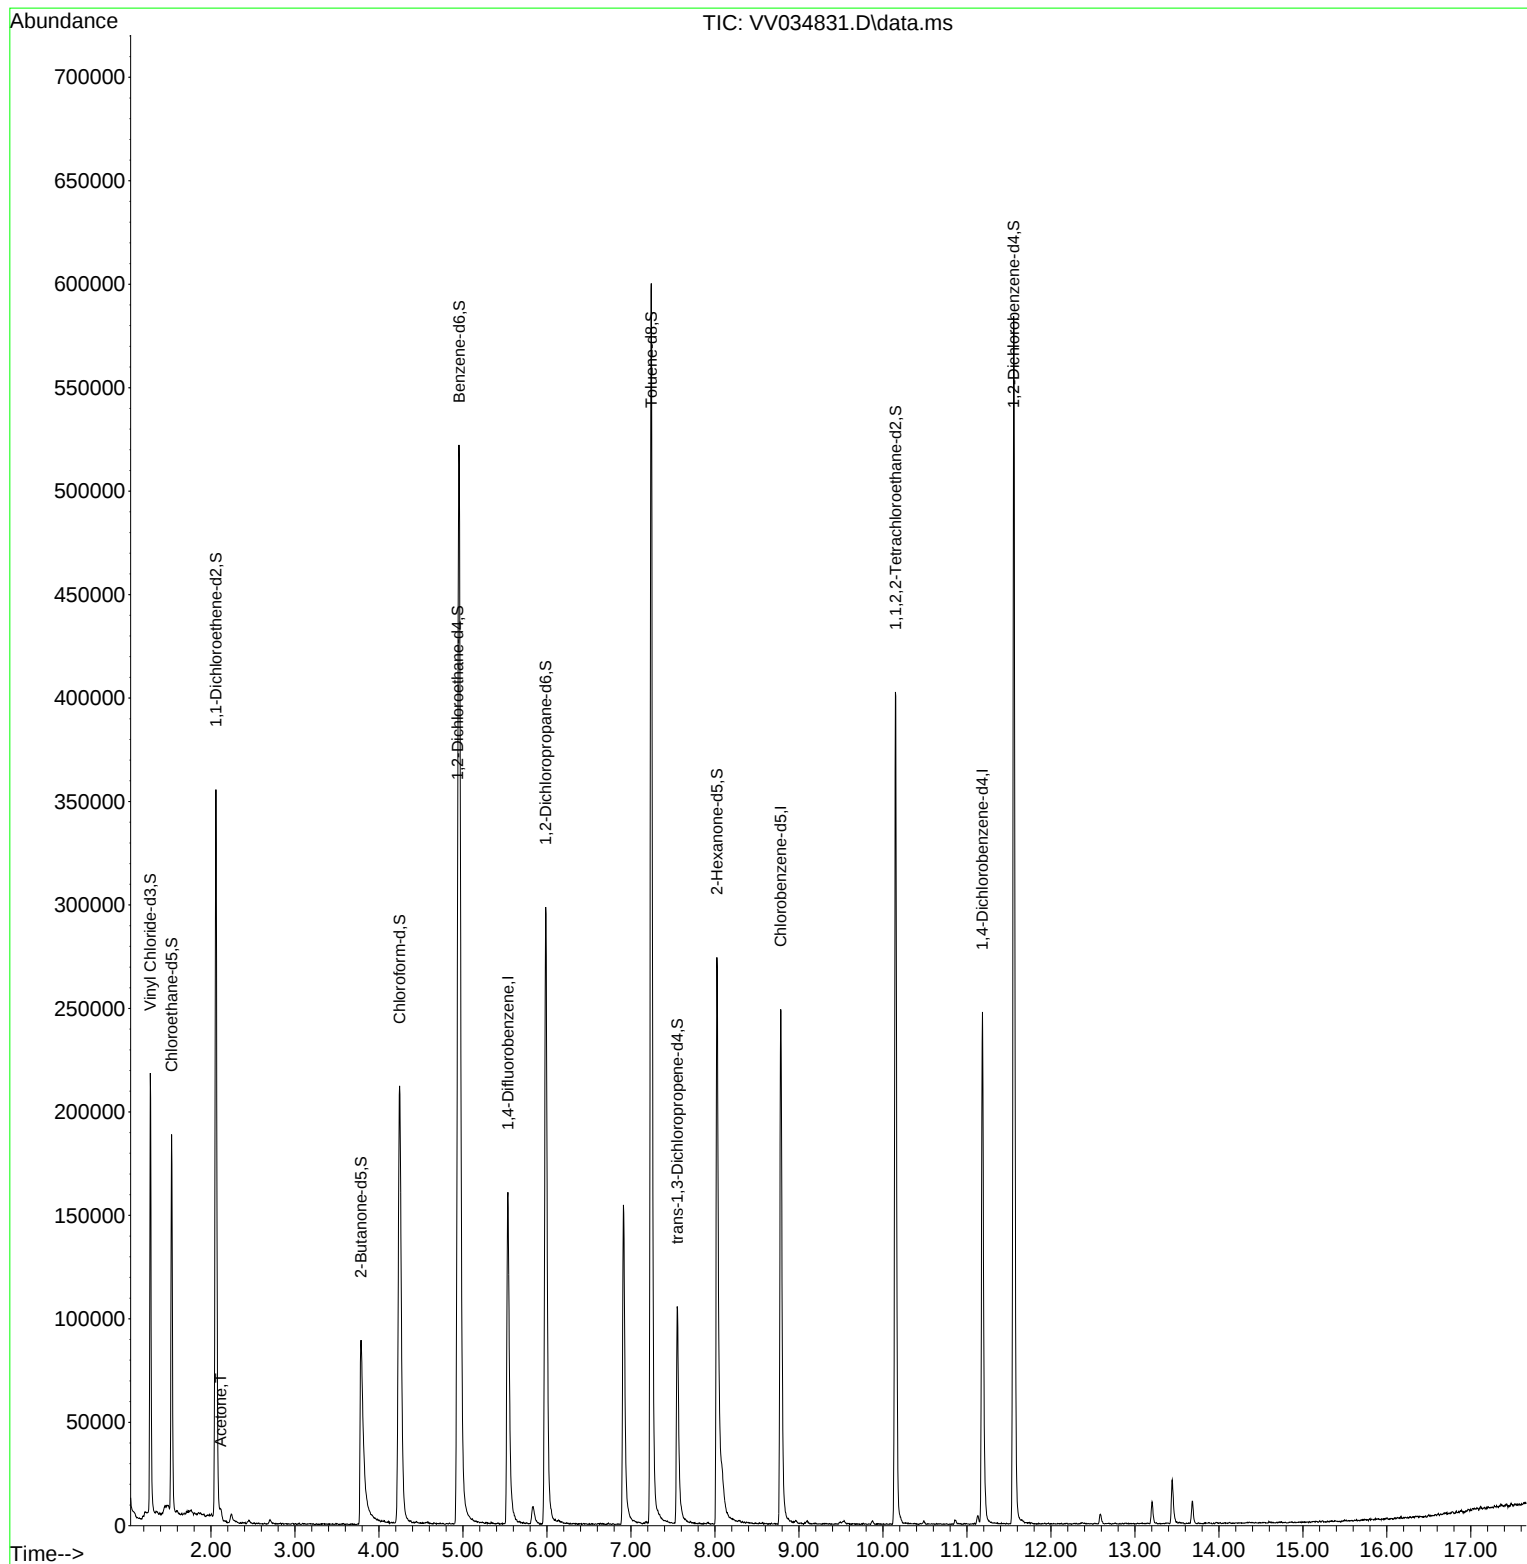

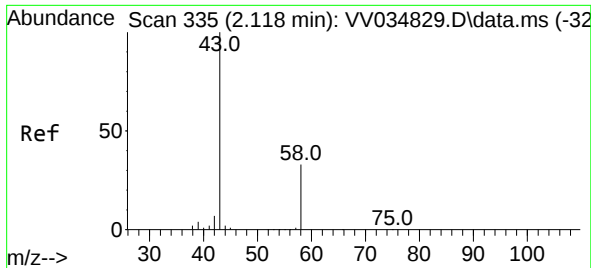

#13  
 Acetone  
 Concen: 4.040 ug/L  
 RT: 2.118 min Scan# 31  
 Delta R.T. -0.000 min  
 Lab File: VV034831.D  
 Acq: 26 Mar 2024 16:41

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 E0LX1

Tgt Ion: 43 Resp: 3069  
 Ion Ratio Lower Upper  
 43 100  
 58 28.1 0.0 66.0

