

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032624\
 Data File : VW034835.D
 Acq On : 26 Mar 2024 18:17
 Operator : SY/MD
 Sample : P1851-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LX5

Quant Time: Mar 27 01:37:36 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 27 01:34:52 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.535	114	131105	50.000	ug/L	0.00
28) Chlorobenzene-d5		8.786	117	129689	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.185	152	61394	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.278	65	109434	86.431	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	172.860%#	
7) Chloroethane-d5		1.532	69	94588	86.010	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	172.020%#	
11) 1,1-Dichloroethene-d2		2.060	65	47864	86.239	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	172.480%#	
21) 2-Butanone-d5		3.786	46	121256	161.475	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	161.470%#	
24) Chloroform-d		4.249	84	181660	85.334	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	170.660%#	
26) 1,2-Dichloroethane-d4		4.941	65	120442	89.113	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	178.220%#	
32) Benzene-d6		4.960	84	370163	84.972	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	169.940%#	
36) 1,2-Dichloropropane-d6		5.989	67	120641	87.210	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	174.420%#	
41) Toluene-d8		7.243	98	315967	80.537	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	161.080%#	
43) trans-1,3-Dichloroprop...		7.555	79	50901	75.688	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	151.380%#	
47) 2-Hexanone-d5		8.024	63	77358	147.907	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	147.910%#	
56) 1,1,2,2-Tetrachloroeth...		10.153	84	161708	84.887	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	169.780%#	
66) 1,2-Dichlorobenzene-d4		11.558	152	119638	86.793	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	173.580%#	
Target Compounds							
51) Chlorobenzene		8.822	112	6619	2.307	ug/L	Qvalue # 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
Data File : VV034835.D
Acq On : 26 Mar 2024 18:17
Operator : SY/MD
Sample : P1851-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LX5

Quant Time: Mar 27 01:37:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 27 01:34:52 2024
Response via : Initial Calibration

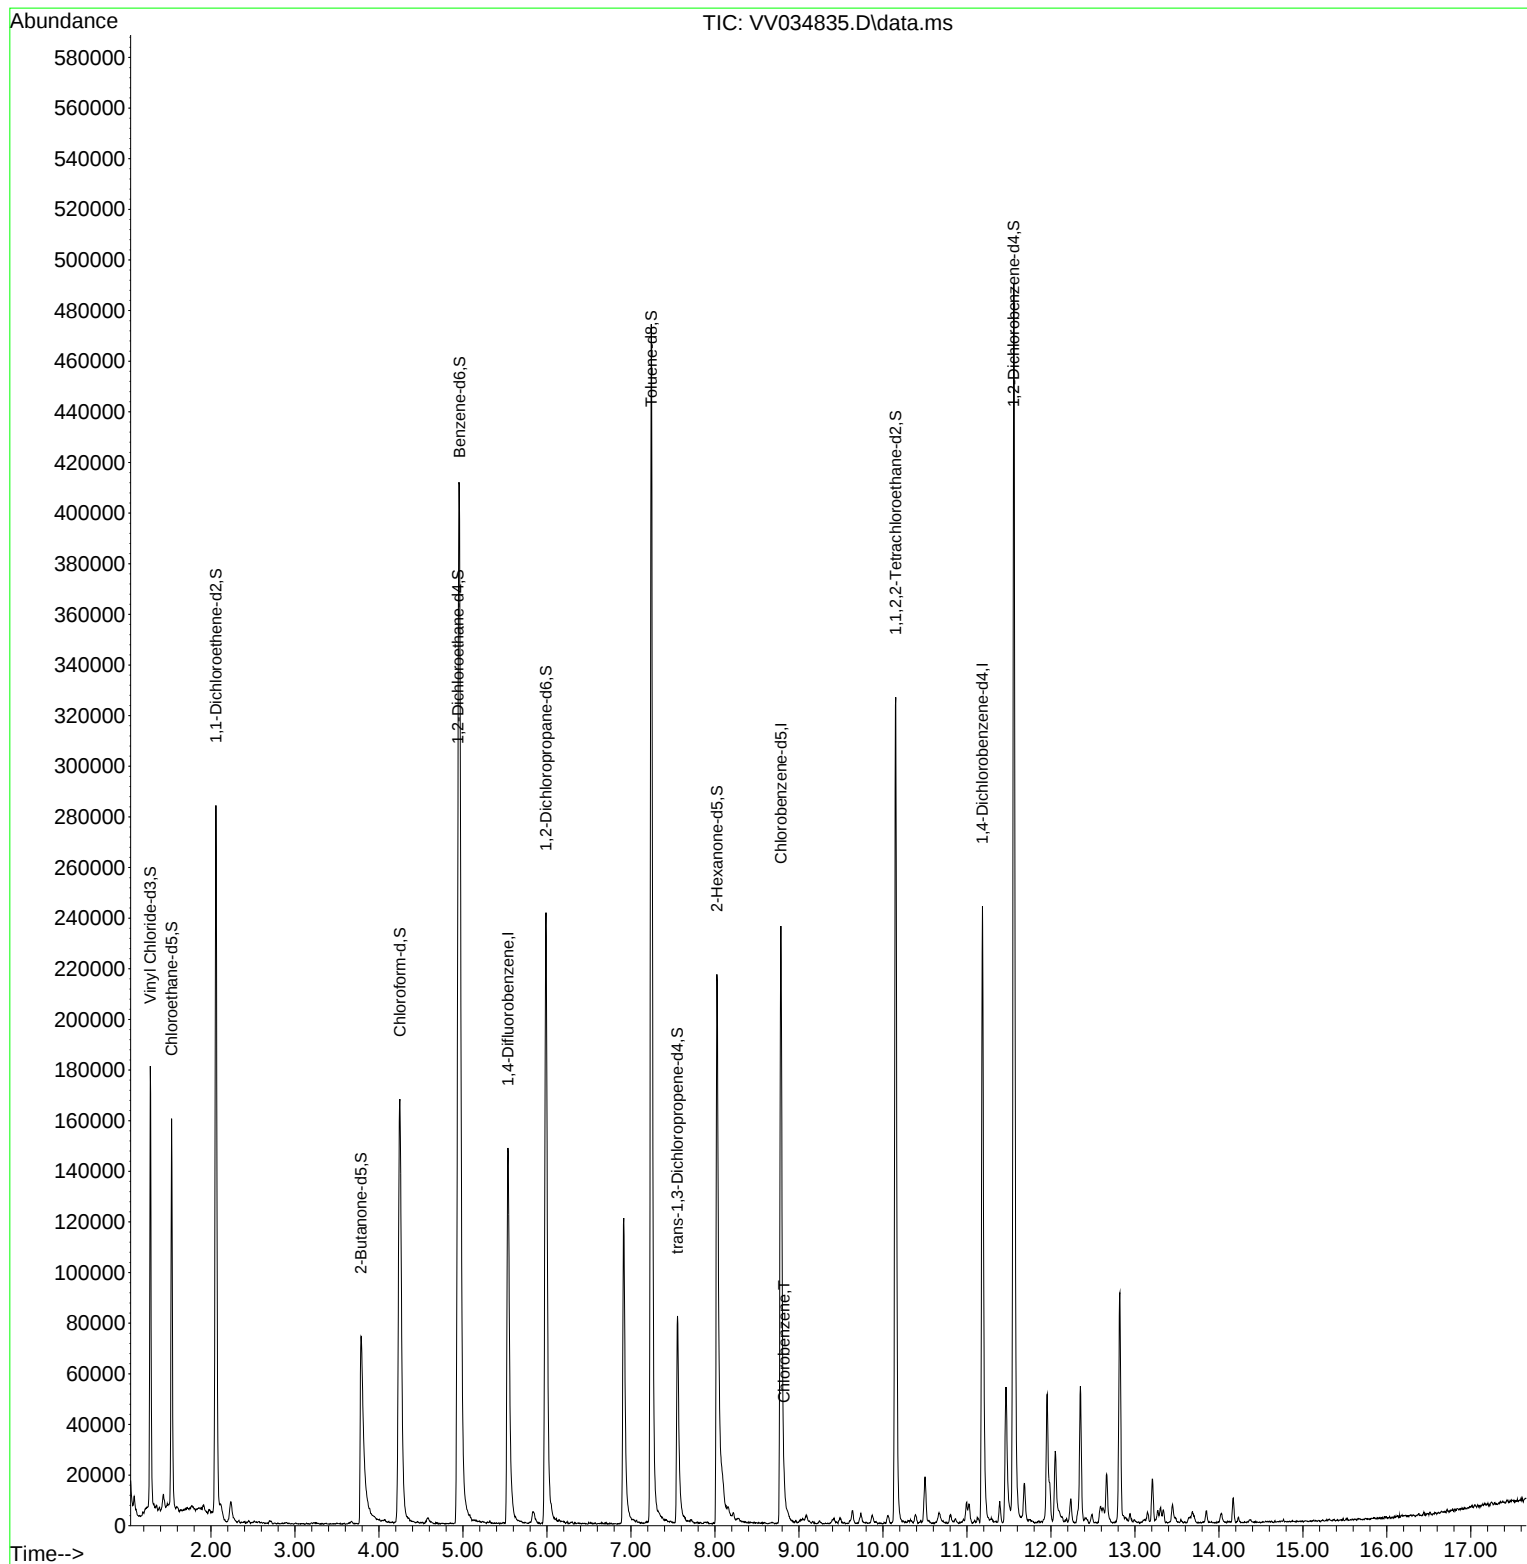

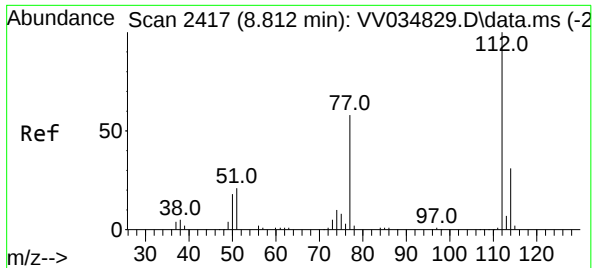

#51
 Chlorobenzene
 Concen: 2.307 ug/L
 RT: 8.822 min Scan# 2417
 Delta R.T. 0.010 min
 Lab File: VV034835.D
 Acq: 26 Mar 2024 18:17

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LX5

Tgt Ion:	112	Resp:	6619
Ion	Ratio	Lower	Upper
112	100		
114	33.6	22.0	41.0
77	71.6	47.4	71.2#

