

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032624\
 Data File : VW034836.D
 Acq On : 26 Mar 2024 18:41
 Operator : SY/MD
 Sample : P1851-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LX6

Quant Time: Mar 27 01:37:50 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 27 01:34:52 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.535	114	206543	50.000	ug/L	0.00
28) Chlorobenzene-d5		8.786	117	200165	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.185	152	94277	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.278	65	127083	63.711	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	127.420%	
7) Chloroethane-d5		1.532	69	111274	64.226	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	128.460%	
11) 1,1-Dichloroethene-d2		2.060	65	56129	64.193	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	128.380%#	
21) 2-Butanone-d5		3.790	46	146256	123.630	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	123.630%	
24) Chloroform-d		4.249	84	218296	65.091	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	130.180%#	
26) 1,2-Dichloroethane-d4		4.941	65	140207	65.848	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	131.700%#	
32) Benzene-d6		4.960	84	446017	66.336	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	132.680%#	
36) 1,2-Dichloropropane-d6		5.986	67	143338	67.135	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	134.260%#	
41) Toluene-d8		7.243	98	382872	63.230	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	126.460%#	
43) trans-1,3-Dichloroprop...		7.555	79	62950	60.648	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	121.300%	
47) 2-Hexanone-d5		8.024	63	98963	122.594	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	122.590%	
56) 1,1,2,2-Tetrachloroeth...		10.153	84	189909	64.591	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	129.180%#	
66) 1,2-Dichlorobenzene-d4		11.558	152	143470	67.779	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	135.560%#	
Target Compounds							
51) Chlorobenzene		8.818	112	6867	1.551	ug/L	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
Data File : VV034836.D
Acq On : 26 Mar 2024 18:41
Operator : SY/MD
Sample : P1851-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LX6

Quant Time: Mar 27 01:37:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 27 01:34:52 2024
Response via : Initial Calibration

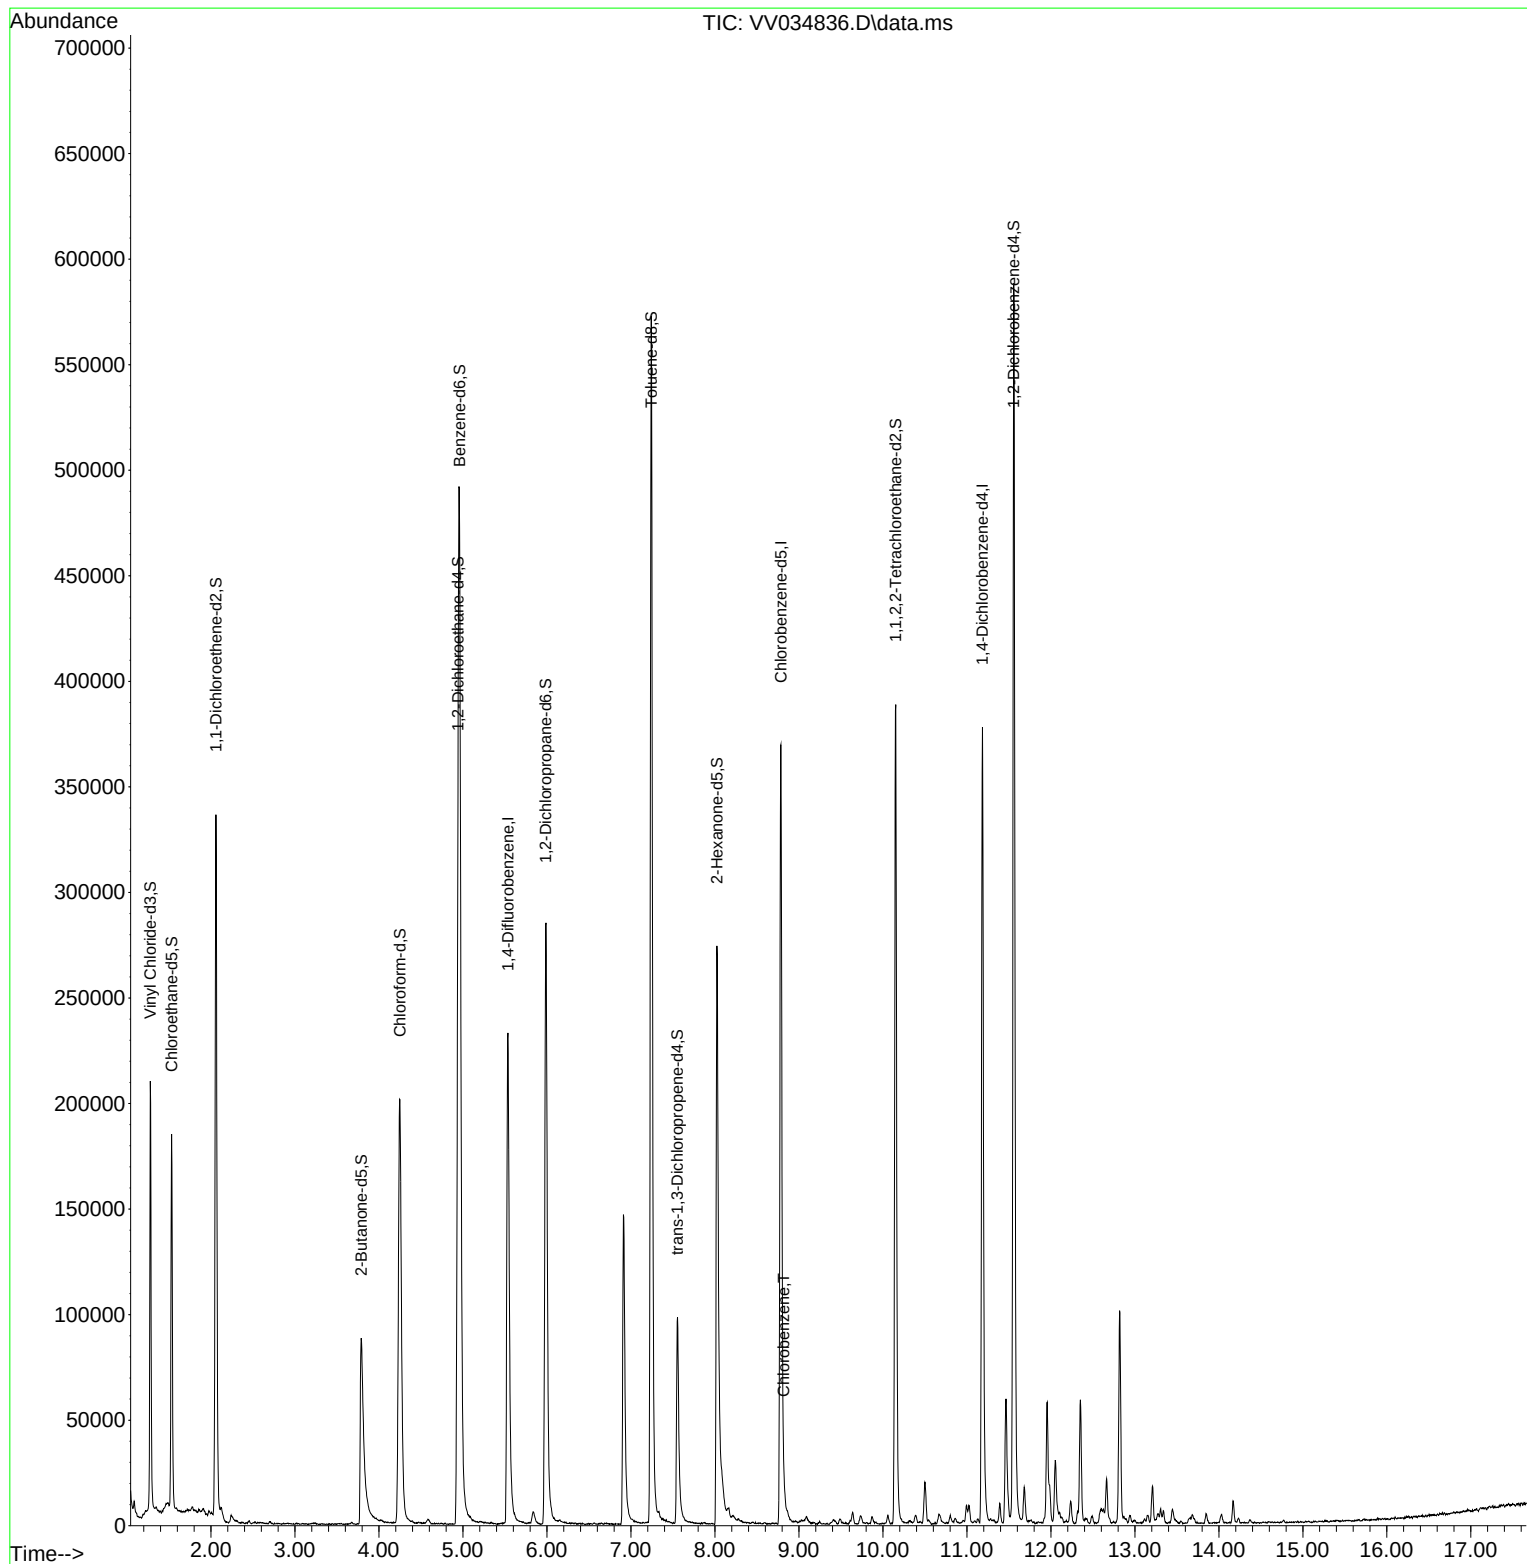

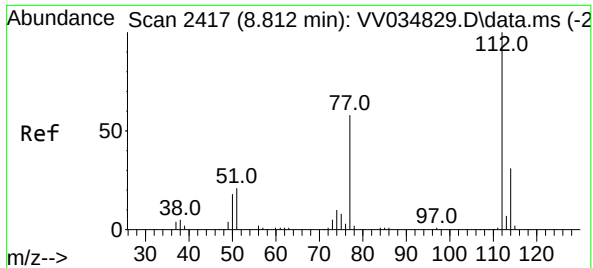

#51
 Chlorobenzene
 Concen: 1.551 ug/L
 RT: 8.818 min Scan# 2419
 Delta R.T. 0.007 min
 Lab File: VV034836.D
 Acq: 26 Mar 2024 18:41

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LX6

Tgt Ion:112	Resp:	6867
Ion	Ratio	Lower Upper
112	100	
114	27.3	22.0 41.0
77	65.3	47.4 71.2

