

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032624\
 Data File : VW034841.D
 Acq On : 26 Mar 2024 20:40
 Operator : SY/MD
 Sample : P1852-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLY2

Quant Time: Mar 27 01:39:02 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 27 01:34:52 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	167702	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	165667	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	72915	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	126849	78.322	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	= 156.640%#		
7) Chloroethane-d5	1.532	69	111328	79.140	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	= 158.280%#		
11) 1,1-Dichloroethene-d2	2.060	65	56589	79.709	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 159.420%#		
21) 2-Butanone-d5	3.786	46	140386	146.153	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	= 146.150%#		
24) Chloroform-d	4.249	84	221198	81.232	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 162.460%#		
26) 1,2-Dichloroethane-d4	4.940	65	145719	84.287	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 168.580%#		
32) Benzene-d6	4.960	84	455230	81.805	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 163.600%#		
36) 1,2-Dichloropropane-d6	5.989	67	144526	81.787	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	= 163.580%#		
41) Toluene-d8	7.243	98	395620	78.941	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 157.880%#		
43) trans-1,3-Dichloroprop...	7.554	79	62421	72.661	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 145.320%#		
47) 2-Hexanone-d5	8.024	63	91968	137.653	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	= 137.650%#		
56) 1,1,2,2-Tetrachloroeth...	10.152	84	191508	78.698	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	= 157.400%#		
66) 1,2-Dichlorobenzene-d4	11.561	152	142116	86.809	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 173.620%#		
Target Compounds						Qvalue
20) cis-1,2-Dichloroethene	3.822	96	3819	2.764	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
Data File : VV034841.D
Acq On : 26 Mar 2024 20:40
Operator : SY/MD
Sample : P1852-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LY2

Quant Time: Mar 27 01:39:02 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 27 01:34:52 2024
Response via : Initial Calibration

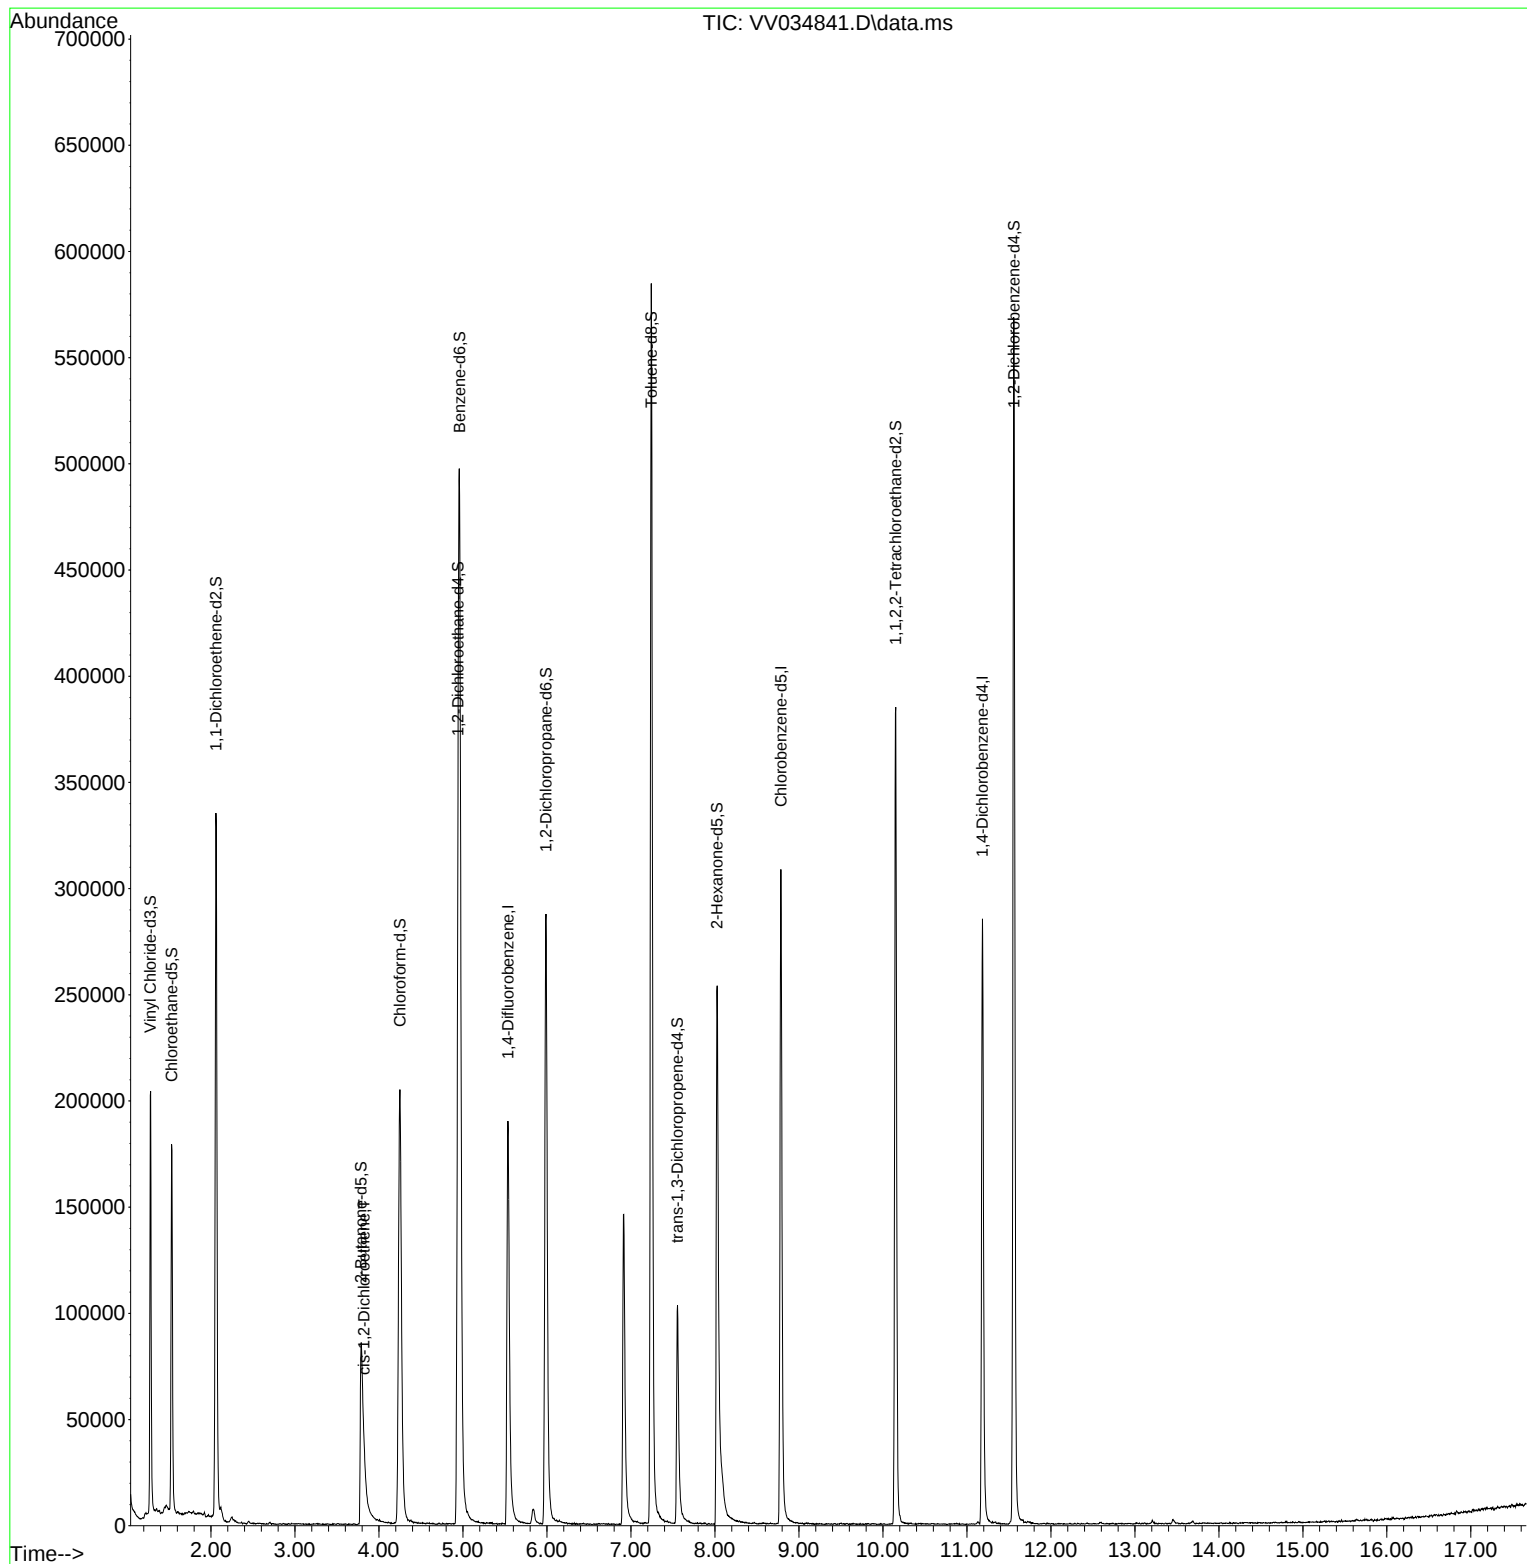

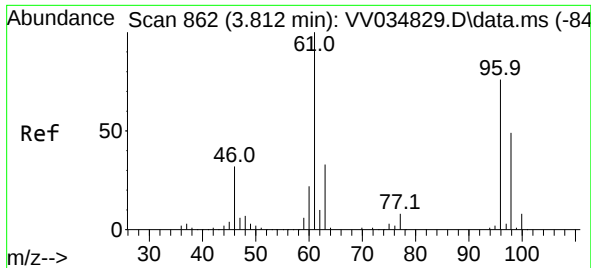

#20
 cis-1,2-Dichloroethene
 Concen: 2.764 ug/L
 RT: 3.822 min Scan# 865
 Delta R.T. 0.010 min
 Lab File: VV034841.D
 Acq: 26 Mar 2024 20:40

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLY2

Tgt Ion: 96 Resp: 3819
 Ion Ratio Lower Upper
 96 100
 61 121.3 94.9 176.3
 98 48.9 45.6 84.8

