

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
 Data File : VV034832.D
 Acq On : 26 Mar 2024 17:05
 Operator : SY/MD
 Sample : P1851-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LX2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034832.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	199953	210980	16.36%	2.395%
2	1.532	146	153	169	rVB	169757	197274	15.29%	2.239%
3	2.060	308	317	335	rBV	325523	470872	36.51%	5.345%
4	2.529	460	463	466	rBV2	556	345	0.03%	0.004%
5	2.706	513	518	526	rVB7	1518	2033	0.16%	0.023%
6	2.780	539	541	544	rBV2	297	204	0.02%	0.002%
7	2.825	553	555	559	rVB3	586	374	0.03%	0.004%
8	2.847	559	562	566	rVB3	421	279	0.02%	0.003%
9	2.931	586	588	593	rVB3	367	177	0.01%	0.002%
10	2.960	593	597	598	rBV	403	220	0.02%	0.002%
11	3.002	608	610	612	rVB2	647	244	0.02%	0.003%
12	3.088	634	637	638	rBV	404	201	0.02%	0.002%
13	3.111	642	644	645	rBV	517	252	0.02%	0.003%
14	3.153	654	657	660	rVB2	321	206	0.02%	0.002%
15	3.214	673	676	680	rBV2	283	187	0.01%	0.002%
16	3.291	698	700	703	rBV2	276	166	0.01%	0.002%
17	3.339	711	715	720	rVB3	464	368	0.03%	0.004%
18	3.394	729	732	736	rBV2	482	309	0.02%	0.004%
19	3.490	757	762	766	rBV3	255	327	0.03%	0.004%
20	3.580	785	790	791	rBV	316	255	0.02%	0.003%
21	3.783	845	853	894	rBV	86424	249448	19.34%	2.832%
22	4.249	983	998	1032	rBV	195614	509106	39.47%	5.779%
23	4.625	1113	1115	1121	rVB3	605	496	0.04%	0.006%
24	4.651	1121	1123	1127	rBV3	378	211	0.02%	0.002%
25	4.953	1202	1217	1247	rBV2	487447	1289876	100.00%	14.642%
26	5.333	1331	1335	1339	rBV4	419	387	0.03%	0.004%
27	5.423	1360	1363	1364	rBV2	428	207	0.02%	0.002%
28	5.535	1387	1398	1427	rBV	234129	488870	37.90%	5.549%
29	5.834	1481	1491	1503	rBV5	7944	18276	1.42%	0.207%
30	5.989	1524	1539	1565	rBV	279532	593484	46.01%	6.737%
31	6.230	1611	1614	1615	rBV	708	323	0.03%	0.004%
32	6.288	1626	1632	1636	rBV6	607	658	0.05%	0.007%
33	6.420	1670	1673	1675	rBV	338	183	0.01%	0.002%
34	6.439	1675	1679	1682	rVV3	537	342	0.03%	0.004%
35	6.474	1688	1690	1693	rBV2	320	215	0.02%	0.002%
36	6.664	1745	1749	1752	rBV2	408	280	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
 Data File : VV034832.D
 Acq On : 26 Mar 2024 17:05
 Operator : SY/MD
 Sample : P1851-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LX2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.683	1752	1755	1758	rBV2	342	254	0.02%	0.003%
38	6.802	1791	1792	1797	rBV2	288	200	0.02%	0.002%
39	6.841	1802	1804	1808	rVB2	403	236	0.02%	0.003%
40	6.915	1816	1827	1853	rBV	145836	286518	22.21%	3.252%
41	7.149	1896	1900	1901	rBV	319	215	0.02%	0.002%
42	7.162	1901	1904	1906	rBV2	526	364	0.03%	0.004%
43	7.243	1918	1929	1955	rBV	569693	1000627	77.58%	11.359%
44	7.555	2016	2026	2046	rBV	99896	184448	14.30%	2.094%
45	7.844	2114	2116	2119	rVB	540	216	0.02%	0.002%
46	7.870	2119	2124	2128	rBV4	665	582	0.05%	0.007%
47	7.911	2133	2137	2142	rBV3	714	914	0.07%	0.010%
48	7.950	2146	2149	2152	rBV2	408	302	0.02%	0.003%
49	8.024	2163	2172	2222	rBV	258655	555347	43.05%	6.304%
50	8.419	2292	2295	2296	rBV2	387	231	0.02%	0.003%
51	8.522	2325	2327	2331	rBV2	534	359	0.03%	0.004%
52	8.616	2353	2356	2361	rVB5	673	549	0.04%	0.006%
53	8.641	2361	2364	2368	rBV2	401	326	0.03%	0.004%
54	8.744	2393	2396	2397	rBV	395	275	0.02%	0.003%
55	8.783	2397	2408	2430	rBV	350906	607934	47.13%	6.901%
56	9.095	2501	2505	2507	rBV4	949	742	0.06%	0.008%
57	9.223	2543	2545	2548	rVB	451	247	0.02%	0.003%
58	9.259	2548	2556	2559	rBV3	414	424	0.03%	0.005%
59	9.294	2564	2567	2569	rBV	438	190	0.01%	0.002%
60	9.310	2569	2572	2577	rBV3	487	356	0.03%	0.004%
61	9.355	2583	2586	2588	rBV	243	182	0.01%	0.002%
62	9.464	2617	2620	2622	rBV3	413	298	0.02%	0.003%
63	9.519	2635	2637	2640	rVB2	577	295	0.02%	0.003%
64	9.580	2654	2656	2658	rBV	448	297	0.02%	0.003%
65	9.606	2662	2664	2668	rBV3	470	413	0.03%	0.005%
66	9.644	2673	2676	2677	rBV2	481	174	0.01%	0.002%
67	9.757	2706	2711	2714	rBV2	486	288	0.02%	0.003%
68	9.863	2740	2744	2745	rBV2	744	420	0.03%	0.005%
69	9.934	2762	2766	2771	rVB	268	186	0.01%	0.002%
70	10.085	2809	2813	2819	rVB3	600	694	0.05%	0.008%
71	10.153	2819	2834	2858	rBV	376793	609913	47.28%	6.923%
72	10.358	2894	2898	2902	rVB2	479	471	0.04%	0.005%
73	10.426	2915	2919	2923	rBV3	396	359	0.03%	0.004%
74	10.490	2931	2939	2945	rVB4	1142	1712	0.13%	0.019%
75	10.583	2966	2968	2972	rVB2	594	392	0.03%	0.004%
76	10.612	2972	2977	2980	rBV	251	248	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
 Data File : VV034832.D
 Acq On : 26 Mar 2024 17:05
 Operator : SY/MD
 Sample : P1851-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LX2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.728	3011	3013	3017	rBV2	254	185	0.01%	0.002%
78	10.792	3031	3033	3036	rBV2	358	202	0.02%	0.002%
79	10.860	3047	3054	3059	rBV4	1452	2108	0.16%	0.024%
80	10.921	3066	3073	3078	rBV4	419	574	0.04%	0.007%
81	11.130	3131	3138	3145	rBV5	2611	4365	0.34%	0.050%
82	11.185	3145	3155	3181	rVV	360145	570408	44.22%	6.475%
83	11.468	3240	3243	3245	rBV2	311	204	0.02%	0.002%
84	11.558	3259	3271	3294	rBV	543959	882032	68.38%	10.012%
85	12.001	3399	3409	3411	rBV4	846	1010	0.08%	0.011%
86	12.130	3445	3449	3450	rBV	423	255	0.02%	0.003%
87	12.284	3494	3497	3501	rBV2	307	229	0.02%	0.003%
88	12.307	3501	3504	3508	rBV	352	267	0.02%	0.003%
89	12.326	3508	3510	3513	rBV2	444	325	0.03%	0.004%
90	12.374	3520	3525	3529	rBV3	707	804	0.06%	0.009%
91	12.448	3543	3548	3549	rBV	273	229	0.02%	0.003%
92	12.590	3585	3592	3601	rBV5	3490	5755	0.45%	0.065%
93	12.754	3641	3643	3648	rVB3	590	355	0.03%	0.004%
94	12.976	3710	3712	3716	rBV2	433	213	0.02%	0.002%
95	13.046	3732	3734	3736	rBV	558	247	0.02%	0.003%
96	13.136	3760	3762	3767	rVB2	787	437	0.03%	0.005%
97	13.207	3774	3784	3799	rBV6	6634	11475	0.89%	0.130%
98	13.445	3851	3858	3873	rBV3	11750	20664	1.60%	0.235%
99	13.683	3924	3932	3942	rBV5	6651	10871	0.84%	0.123%
100	13.972	4019	4022	4023	rBV2	501	280	0.02%	0.003%




Sum of corrected areas: 8809327

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
Data File : VV034832.D
Acq On : 26 Mar 2024 17:05
Operator : SY/MD
Sample : P1851-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

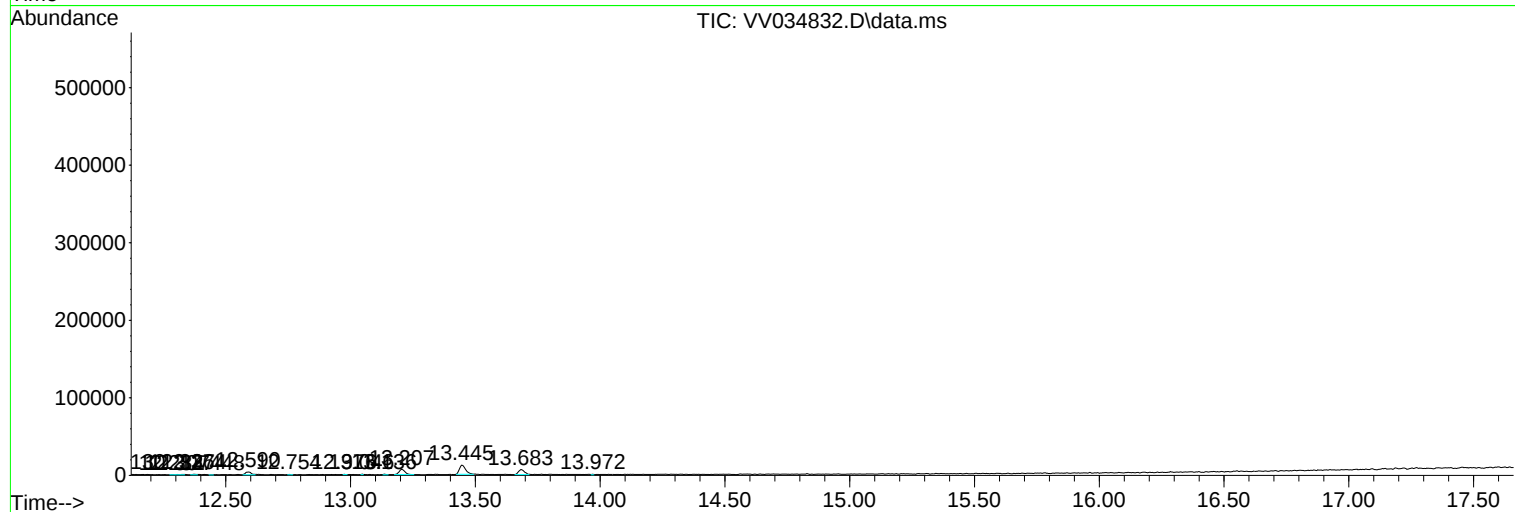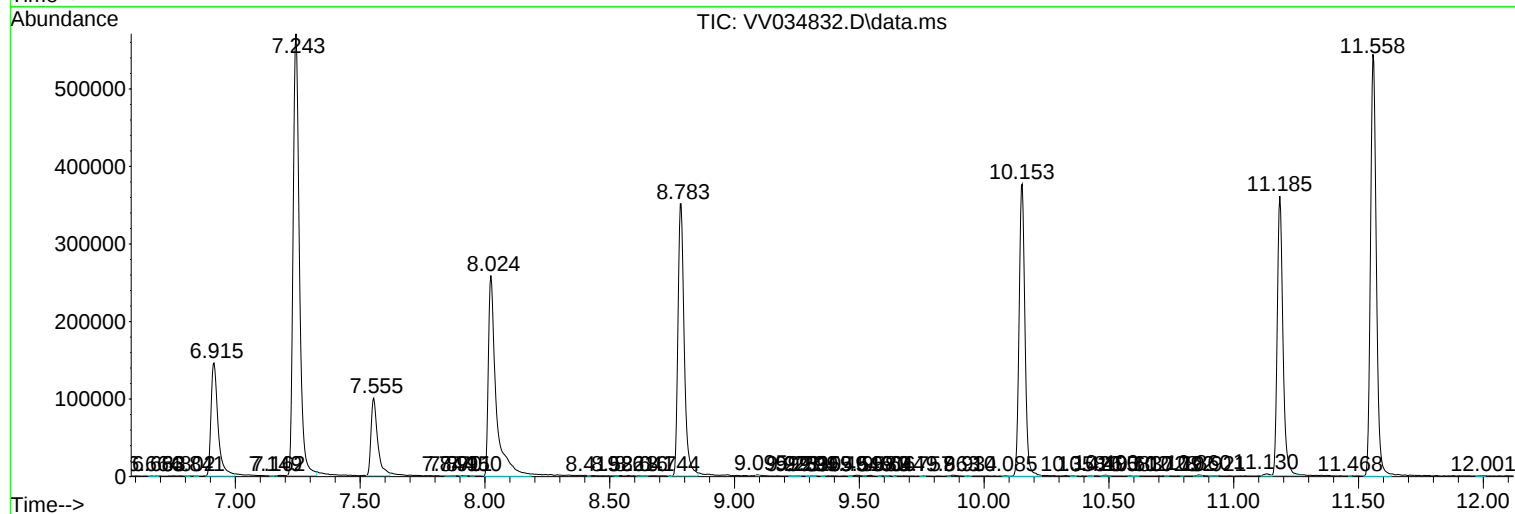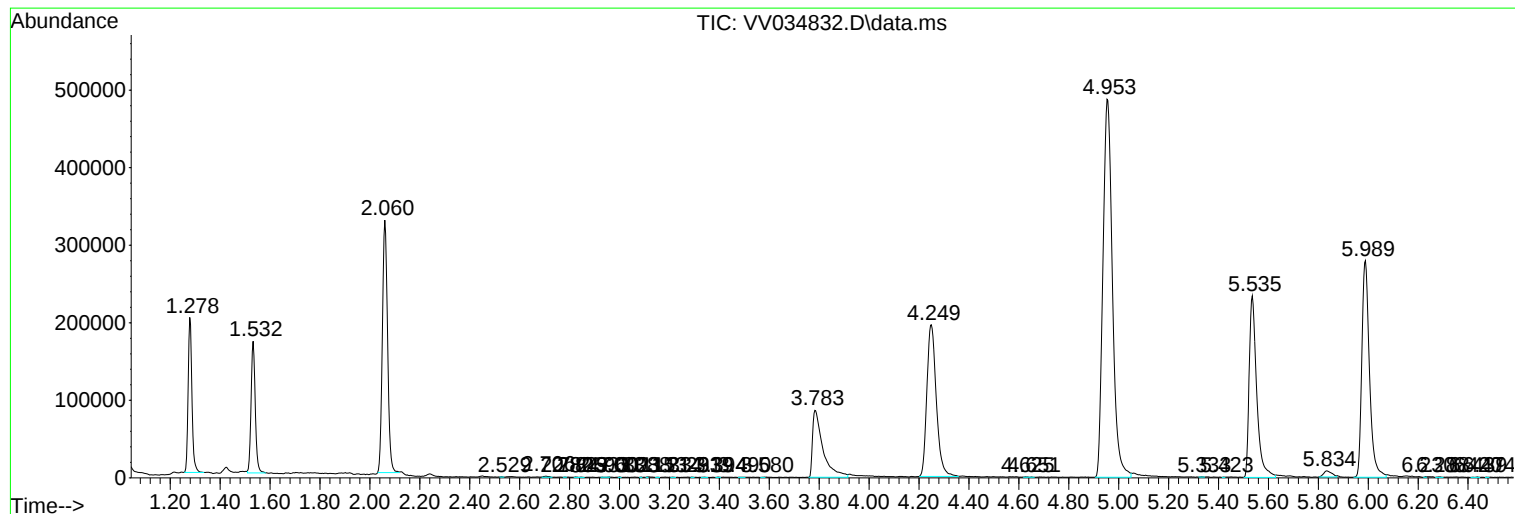

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
Data File : VV034832.D
Acq On : 26 Mar 2024 17:05
Operator : SY/MD
Sample : P1851-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
Data File : VV034832.D
Acq On : 26 Mar 2024 17:05
Operator : SY/MD
Sample : P1851-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------