

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
 Data File : VV034837.D
 Acq On : 26 Mar 2024 19:05
 Operator : SY/MD
 Sample : P1851-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LX7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034837.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	228320	242603	15.81%	2.118%
2	1.532	146	153	166	rVB	200494	232585	15.16%	2.030%
3	2.059	308	317	332	rBV	379325	548762	35.76%	4.790%
4	2.693	509	514	515	rBV2	888	621	0.04%	0.005%
5	2.751	528	532	536	rBV3	494	399	0.03%	0.003%
6	2.889	571	575	577	rBV2	921	711	0.05%	0.006%
7	2.973	600	601	605	rVB2	388	230	0.01%	0.002%
8	2.992	605	607	610	rBV2	415	308	0.02%	0.003%
9	3.024	616	617	620	rVB2	357	204	0.01%	0.002%
10	3.124	645	648	652	rBV4	437	343	0.02%	0.003%
11	3.156	656	658	665	rBV2	256	241	0.02%	0.002%
12	3.198	665	671	672	rBV2	571	538	0.04%	0.005%
13	3.275	693	695	697	rVB3	564	233	0.02%	0.002%
14	3.301	701	703	705	rBV	378	193	0.01%	0.002%
15	3.317	706	708	710	rVB	269	84	0.01%	0.001%
16	3.333	711	713	715	rBV2	279	146	0.01%	0.001%
17	3.355	718	720	722	rBV	300	115	0.01%	0.001%
18	3.407	733	736	740	rBV2	445	295	0.02%	0.003%
19	3.429	740	743	746	rBV2	350	283	0.02%	0.002%
20	3.506	765	767	770	rBV	287	188	0.01%	0.002%
21	3.526	770	773	775	rBV2	202	142	0.01%	0.001%
22	3.567	783	786	789	rVB2	469	240	0.02%	0.002%
23	3.625	801	804	807	rBV3	434	309	0.02%	0.003%
24	3.680	819	821	823	rBV	191	79	0.01%	0.001%
25	3.709	829	830	833	rVB2	365	191	0.01%	0.002%
26	3.728	833	836	838	rBV2	264	121	0.01%	0.001%
27	3.741	838	840	844	rBV3	520	333	0.02%	0.003%
28	3.786	844	854	888	rBV	113019	336885	21.95%	2.941%
29	4.249	983	998	1028	rBV	233162	598597	39.01%	5.225%
30	4.725	1143	1146	1148	rBV	295	216	0.01%	0.002%
31	4.789	1163	1166	1168	rBV4	537	370	0.02%	0.003%
32	4.860	1186	1188	1191	rBV	370	151	0.01%	0.001%
33	4.895	1196	1199	1201	rBV2	377	285	0.02%	0.002%
34	4.956	1202	1218	1264	rBV2	577237	1534540	100.00%	13.395%
35	5.532	1386	1397	1428	rBV	405114	838978	54.67%	7.323%
36	5.989	1521	1539	1564	rBV	341312	712031	46.40%	6.215%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
 Data File : VV034837.D
 Acq On : 26 Mar 2024 19:05
 Operator : SY/MD
 Sample : P1851-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LX7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.384	1660	1662	1669	rVB4	619	503	0.03%	0.004%
38	6.429	1674	1676	1681	rBV2	543	400	0.03%	0.003%
39	6.644	1741	1743	1748	rBV5	699	488	0.03%	0.004%
40	6.693	1756	1758	1760	rBV	565	305	0.02%	0.003%
41	6.718	1764	1766	1767	rBV	512	199	0.01%	0.002%
42	6.770	1780	1782	1785	rBV2	226	110	0.01%	0.001%
43	6.815	1793	1796	1798	rBV	465	273	0.02%	0.002%
44	6.844	1801	1805	1807	rVB2	243	178	0.01%	0.002%
45	6.911	1816	1826	1853	rBV	174898	334904	21.82%	2.923%
46	7.146	1896	1899	1900	rBV3	676	469	0.03%	0.004%
47	7.243	1918	1929	1954	rBV	675575	1188889	77.48%	10.378%
48	7.554	2017	2026	2061	rVB	118477	220014	14.34%	1.920%
49	7.943	2146	2147	2153	rBV2	240	182	0.01%	0.002%
50	8.024	2163	2172	2210	rBV	349067	707172	46.08%	6.173%
51	8.529	2326	2329	2332	rBV3	550	443	0.03%	0.004%
52	8.596	2346	2350	2352	rBV3	489	328	0.02%	0.003%
53	8.609	2352	2354	2356	rVV2	470	190	0.01%	0.002%
54	8.644	2363	2365	2369	rBV3	335	191	0.01%	0.002%
55	8.722	2387	2389	2393	rVB3	595	377	0.02%	0.003%
56	8.747	2393	2397	2398	rBV3	539	371	0.02%	0.003%
57	8.783	2398	2408	2430	rBV	632406	1061029	69.14%	9.261%
58	9.162	2523	2526	2527	rBV	967	541	0.04%	0.005%
59	9.262	2554	2557	2559	rBV2	605	388	0.03%	0.003%
60	9.336	2577	2580	2581	rBV2	369	180	0.01%	0.002%
61	9.377	2591	2593	2596	rBV3	455	224	0.01%	0.002%
62	9.435	2609	2611	2615	rVB3	1152	622	0.04%	0.005%
63	9.461	2616	2619	2620	rBV2	266	127	0.01%	0.001%
64	9.490	2621	2628	2635	rBV6	1746	2685	0.17%	0.023%
65	9.535	2638	2642	2644	rBV2	507	367	0.02%	0.003%
66	9.609	2660	2665	2667	rBV2	417	358	0.02%	0.003%
67	9.622	2667	2669	2671	rVV2	395	180	0.01%	0.002%
68	9.876	2742	2748	2757	rVB7	2657	3735	0.24%	0.033%
69	9.911	2757	2759	2762	rBV2	446	185	0.01%	0.002%
70	9.931	2762	2765	2766	rBV2	475	225	0.01%	0.002%
71	9.940	2766	2768	2771	rBV3	542	303	0.02%	0.003%
72	10.004	2786	2788	2790	rBV2	490	150	0.01%	0.001%
73	10.017	2790	2792	2793	rBV2	557	232	0.02%	0.002%
74	10.098	2812	2817	2819	rBV3	822	879	0.06%	0.008%
75	10.152	2822	2834	2856	rBV	465671	735613	47.94%	6.421%
76	10.342	2890	2893	2898	rBV5	801	771	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
 Data File : VV034837.D
 Acq On : 26 Mar 2024 19:05
 Operator : SY/MD
 Sample : P1851-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLX7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.461	2928	2930	2932	rBV2	731	446	0.03%	0.004%
78	10.590	2965	2970	2975	rBV4	492	566	0.04%	0.005%
79	10.622	2975	2980	2983	rBV3	755	788	0.05%	0.007%
80	10.821	3040	3042	3044	rBV	254	143	0.01%	0.001%
81	11.021	3102	3104	3109	rVB3	642	482	0.03%	0.004%
82	11.130	3129	3138	3144	rBV9	2404	4106	0.27%	0.036%
83	11.184	3144	3155	3183	rVV	636703	985433	64.22%	8.602%
84	11.467	3236	3243	3254	rVB2	20866	32417	2.11%	0.283%
85	11.557	3261	3271	3298	rVB	681377	1069117	69.67%	9.332%
86	11.959	3392	3396	3401	rBV3	1521	1528	0.10%	0.013%
87	12.191	3467	3468	3469	rBV3	296	80	0.01%	0.001%
88	12.345	3514	3516	3517	rBV2	881	416	0.03%	0.004%
89	12.506	3564	3566	3568	rBV2	616	330	0.02%	0.003%
90	12.602	3588	3596	3610	rVB2	10236	17858	1.16%	0.156%
91	12.692	3622	3624	3626	rBV3	609	317	0.02%	0.003%
92	12.824	3657	3665	3674	rVB8	3584	5981	0.39%	0.052%
93	13.181	3774	3776	3778	rBV2	443	180	0.01%	0.002%
94	13.207	3778	3784	3793	rVV7	3428	4663	0.30%	0.041%
95	13.313	3815	3817	3820	rBV3	858	522	0.03%	0.005%
96	13.393	3841	3842	3844	rBV2	416	145	0.01%	0.001%
97	13.451	3852	3860	3873	rBV3	5462	8745	0.57%	0.076%
98	13.573	3896	3898	3903	rVB3	670	418	0.03%	0.004%
99	13.654	3919	3923	3926	rBV	511	454	0.03%	0.004%
100	13.686	3926	3933	3938	rBV6	2730	3894	0.25%	0.034%




Sum of corrected areas: 11456359

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
Data File : VV034837.D
Acq On : 26 Mar 2024 19:05
Operator : SY/MD
Sample : P1851-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LX7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

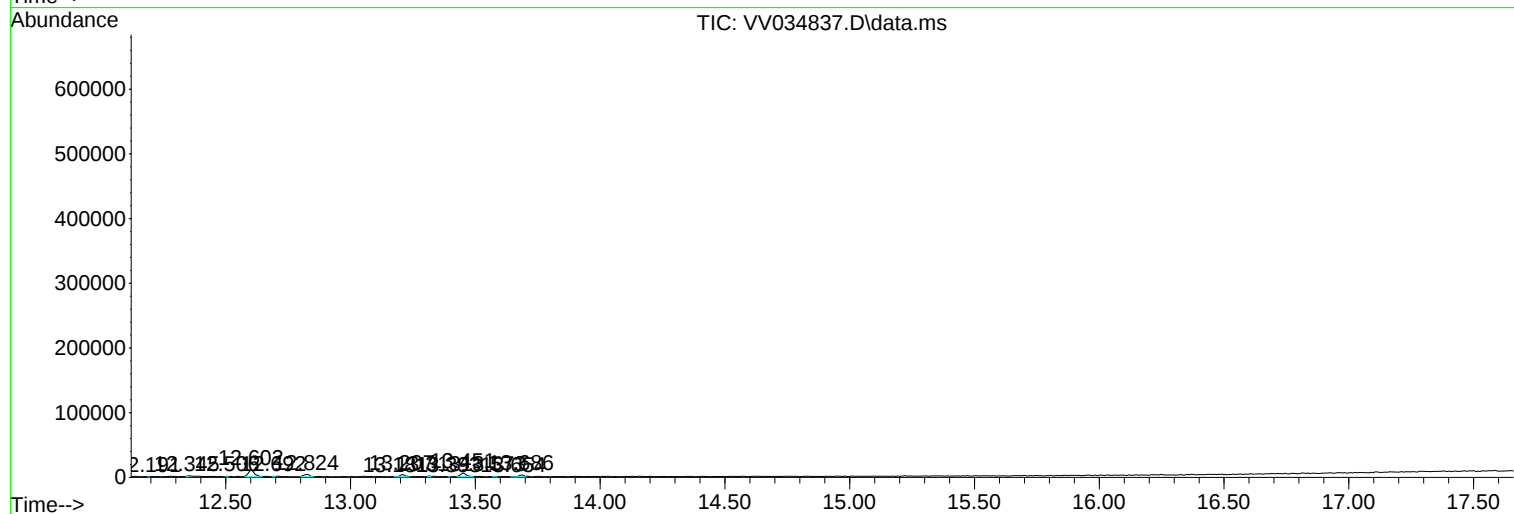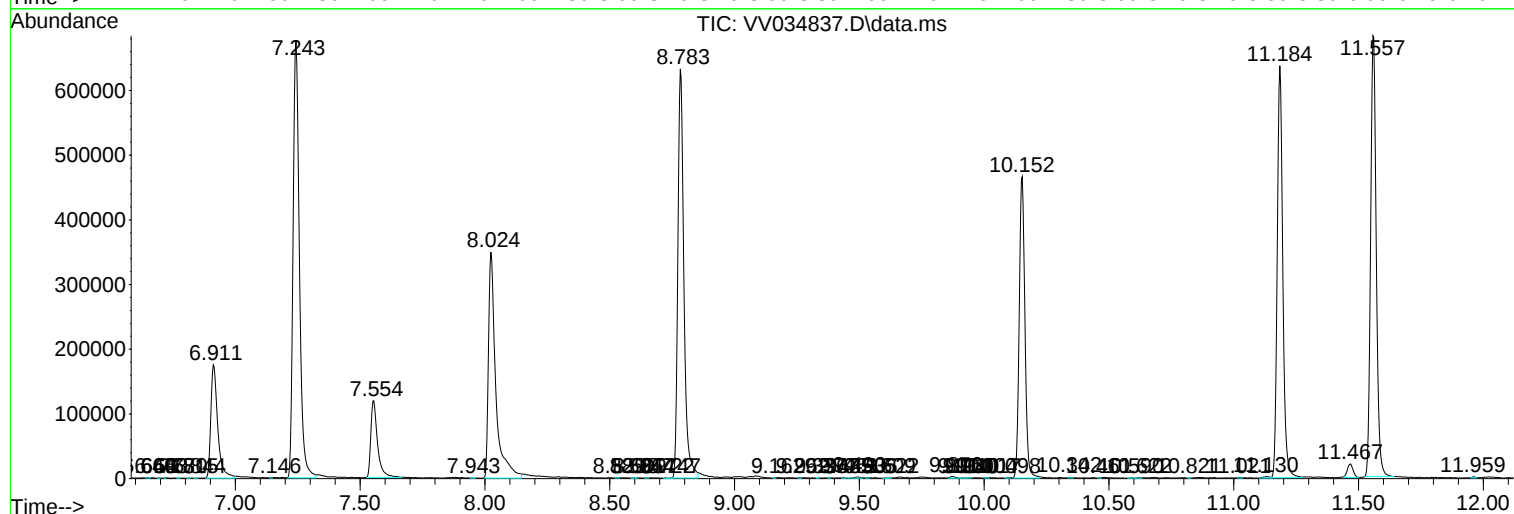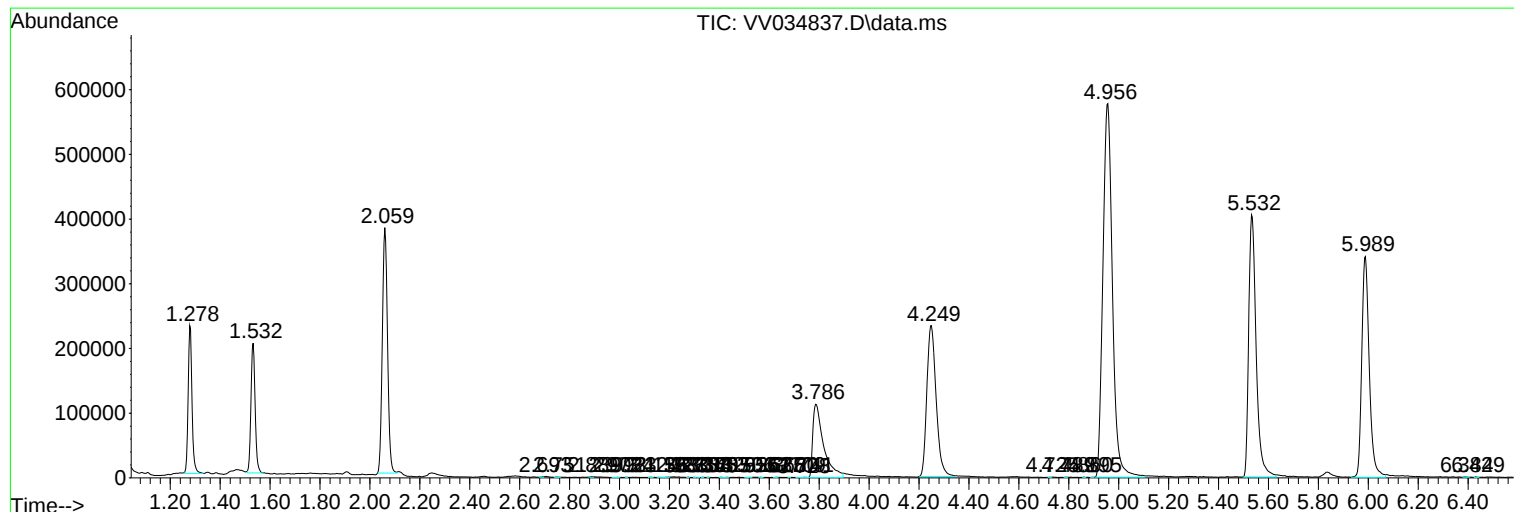

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
Data File : VV034837.D
Acq On : 26 Mar 2024 19:05
Operator : SY/MD
Sample : P1851-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LX7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
Data File : VV034837.D
Acq On : 26 Mar 2024 19:05
Operator : SY/MD
Sample : P1851-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LX7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc