

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
 Data File : VV034839.D
 Acq On : 26 Mar 2024 19:53
 Operator : SY/MD
 Sample : P1851-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034839.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	233802	247124	16.45%	2.397%
2	1.532	146	153	171	rVB	197438	235068	15.65%	2.280%
3	2.059	308	317	332	rBV	376970	542644	36.12%	5.263%
4	2.378	413	416	419	rVB3	516	370	0.02%	0.004%
5	2.555	467	471	472	rBV	412	225	0.01%	0.002%
6	2.764	532	536	542	rVB3	410	366	0.02%	0.004%
7	2.809	546	550	553	rVB2	427	260	0.02%	0.003%
8	2.822	553	554	560	rVB	402	190	0.01%	0.002%
9	2.883	571	573	577	rBV3	312	180	0.01%	0.002%
10	3.008	605	612	617	rBV3	571	656	0.04%	0.006%
11	3.098	639	640	644	rBV	327	227	0.02%	0.002%
12	3.166	659	661	663	rBV	295	195	0.01%	0.002%
13	3.288	696	699	702	rBV	303	173	0.01%	0.002%
14	3.494	757	763	765	rBV	348	371	0.02%	0.004%
15	3.555	779	782	785	rVV3	523	362	0.02%	0.004%
16	3.603	795	797	802	rVB2	395	271	0.02%	0.003%
17	3.670	815	818	827	rVB4	433	439	0.03%	0.004%
18	3.715	827	832	838	rBV2	388	496	0.03%	0.005%
19	3.786	846	854	883	rBV	98266	277083	18.44%	2.687%
20	4.249	982	998	1032	rBV	230227	598768	39.85%	5.807%
21	4.622	1108	1114	1116	rBV3	608	522	0.03%	0.005%
22	4.686	1132	1134	1136	rBV3	297	169	0.01%	0.002%
23	4.857	1184	1187	1189	rBV2	331	193	0.01%	0.002%
24	4.956	1201	1218	1246	rBV2	567752	1502480	100.00%	14.573%
25	5.432	1363	1366	1372	rVB4	724	624	0.04%	0.006%
26	5.471	1377	1378	1380	rBV2	422	166	0.01%	0.002%
27	5.535	1387	1398	1427	rBV	285231	595706	39.65%	5.778%
28	5.773	1465	1472	1477	rBV5	1015	1162	0.08%	0.011%
29	5.796	1477	1479	1482	rBV	425	240	0.02%	0.002%
30	5.834	1482	1491	1508	rVV4	9384	19838	1.32%	0.192%
31	5.989	1525	1539	1574	rBV	329425	691665	46.03%	6.708%
32	6.214	1607	1609	1612	rBV3	573	203	0.01%	0.002%
33	6.355	1649	1653	1655	rBV3	569	345	0.02%	0.003%
34	6.452	1680	1683	1685	rVB2	378	238	0.02%	0.002%
35	6.519	1699	1704	1707	rVV2	322	309	0.02%	0.003%
36	6.538	1707	1710	1712	rVV4	524	348	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
 Data File : VV034839.D
 Acq On : 26 Mar 2024 19:53
 Operator : SY/MD
 Sample : P1851-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.593	1725	1727	1730	rBV2	314	172	0.01%	0.002%
38	6.786	1784	1787	1791	rVV3	364	260	0.02%	0.003%
39	6.834	1800	1802	1805	rVB	296	179	0.01%	0.002%
40	6.915	1816	1827	1856	rBV	170045	328527	21.87%	3.186%
41	7.243	1918	1929	1965	rBV	671468	1185128	78.88%	11.495%
42	7.551	2016	2025	2051	rBV	114189	217327	14.46%	2.108%
43	7.818	2106	2108	2111	rVB2	422	210	0.01%	0.002%
44	7.847	2114	2117	2120	rVB3	555	330	0.02%	0.003%
45	7.866	2120	2123	2124	rBV	373	242	0.02%	0.002%
46	8.024	2162	2172	2215	rBV	314683	649048	43.20%	6.295%
47	8.413	2290	2293	2295	rBV2	563	346	0.02%	0.003%
48	8.464	2306	2309	2311	rBV3	511	325	0.02%	0.003%
49	8.741	2393	2395	2398	rVB3	537	331	0.02%	0.003%
50	8.786	2398	2409	2441	rBV	435615	748571	49.82%	7.260%
51	9.056	2489	2493	2495	rBV3	420	266	0.02%	0.003%
52	9.220	2541	2544	2547	rBV2	369	252	0.02%	0.002%
53	9.268	2555	2559	2560	rBV	360	215	0.01%	0.002%
54	9.320	2573	2575	2577	rBV	313	173	0.01%	0.002%
55	9.397	2596	2599	2604	rVB3	349	295	0.02%	0.003%
56	9.458	2614	2618	2620	rBV2	267	200	0.01%	0.002%
57	9.513	2633	2635	2639	rBV2	295	204	0.01%	0.002%
58	9.532	2639	2641	2643	rBV	316	184	0.01%	0.002%
59	9.574	2650	2654	2657	rVB3	810	554	0.04%	0.005%
60	9.648	2674	2677	2679	rBV	435	206	0.01%	0.002%
61	9.699	2690	2693	2695	rBV	365	180	0.01%	0.002%
62	9.731	2699	2703	2707	rVB2	366	266	0.02%	0.003%
63	9.776	2714	2717	2720	rBV3	289	199	0.01%	0.002%
64	9.805	2720	2726	2728	rBV2	443	324	0.02%	0.003%
65	9.873	2742	2747	2749	rBV2	397	382	0.03%	0.004%
66	9.895	2752	2754	2756	rVB3	516	196	0.01%	0.002%
67	9.985	2780	2782	2785	rVB2	444	179	0.01%	0.002%
68	10.005	2785	2788	2792	rVB3	291	175	0.01%	0.002%
69	10.033	2792	2797	2800	rBV2	186	219	0.01%	0.002%
70	10.101	2814	2818	2822	rVB3	396	386	0.03%	0.004%
71	10.152	2822	2834	2853	rBV	444414	707416	47.08%	6.861%
72	10.413	2912	2915	2917	rBV2	255	164	0.01%	0.002%
73	10.699	2998	3004	3006	rBV2	343	384	0.03%	0.004%
74	10.786	3030	3031	3035	rBV3	389	252	0.02%	0.002%
75	10.831	3042	3045	3047	rVB2	326	176	0.01%	0.002%
76	10.911	3064	3070	3075	rBV2	474	554	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
 Data File : VV034839.D
 Acq On : 26 Mar 2024 19:53
 Operator : SY/MD
 Sample : P1851-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	11.133	3133	3139	3144	rBV4	1605	1873	0.12%	0.018%
78	11.185	3144	3155	3181	rBV	426283	677330	45.08%	6.569%
79	11.561	3252	3272	3300	rBV	651488	1051118	69.96%	10.195%
80	11.818	3349	3352	3354	rBV3	578	330	0.02%	0.003%
81	11.889	3371	3374	3378	rVB4	583	408	0.03%	0.004%
82	12.056	3424	3426	3429	rVB2	445	183	0.01%	0.002%
83	12.091	3433	3437	3438	rBV2	255	182	0.01%	0.002%
84	12.127	3446	3448	3451	rVB2	352	174	0.01%	0.002%
85	12.146	3451	3454	3456	rBV	468	238	0.02%	0.002%
86	12.403	3531	3534	3536	rBV2	296	211	0.01%	0.002%
87	12.551	3576	3580	3582	rBV2	392	296	0.02%	0.003%
88	12.590	3590	3592	3601	rVB4	1287	1131	0.08%	0.011%
89	12.699	3624	3626	3628	rBV2	529	283	0.02%	0.003%
90	12.795	3651	3656	3658	rBV	466	371	0.02%	0.004%
91	12.930	3696	3698	3702	rVB	293	198	0.01%	0.002%
92	13.043	3729	3733	3735	rBV2	251	206	0.01%	0.002%
93	13.056	3735	3737	3739	rBV	417	223	0.01%	0.002%
94	13.210	3780	3785	3798	rVB4	1870	2462	0.16%	0.024%
95	13.374	3834	3836	3839	rBV	511	322	0.02%	0.003%
96	13.455	3854	3861	3875	rVB4	3413	5296	0.35%	0.051%
97	13.577	3895	3899	3901	rBV2	452	307	0.02%	0.003%
98	13.689	3928	3934	3938	rBV4	1948	1878	0.12%	0.018%
99	14.130	4067	4071	4073	rBV	509	413	0.03%	0.004%
100	14.483	4179	4181	4182	rBV	523	199	0.01%	0.002%




Sum of corrected areas: 10310305

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
Data File : VV034839.D
Acq On : 26 Mar 2024 19:53
Operator : SY/MD
Sample : P1851-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOLY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

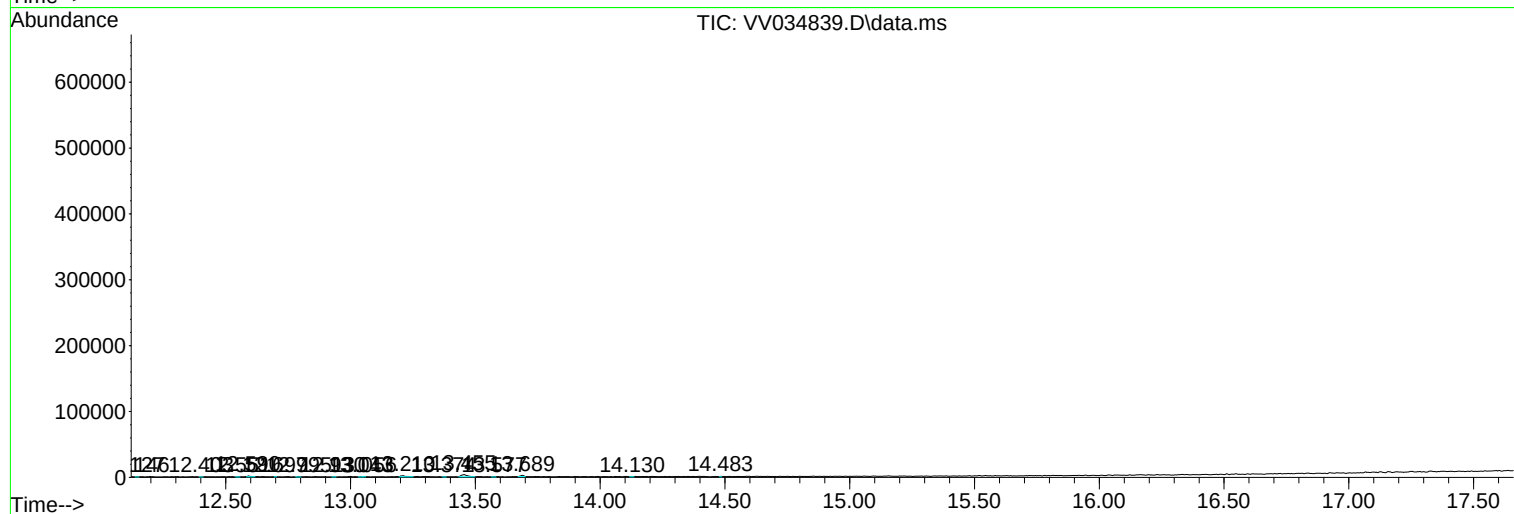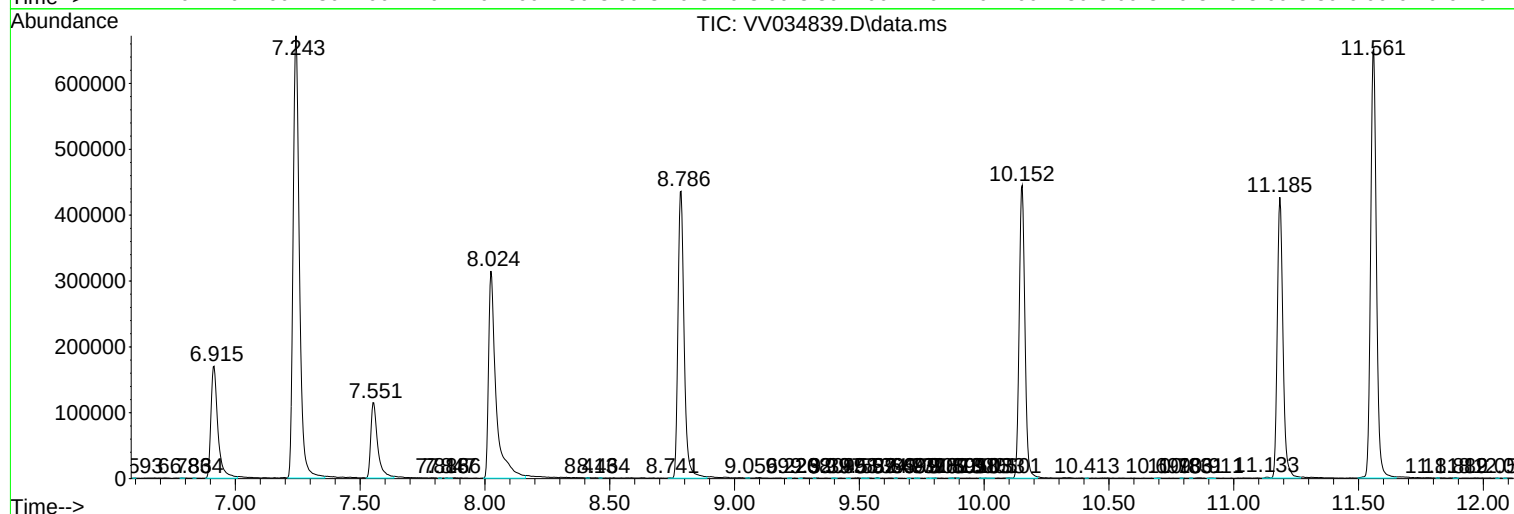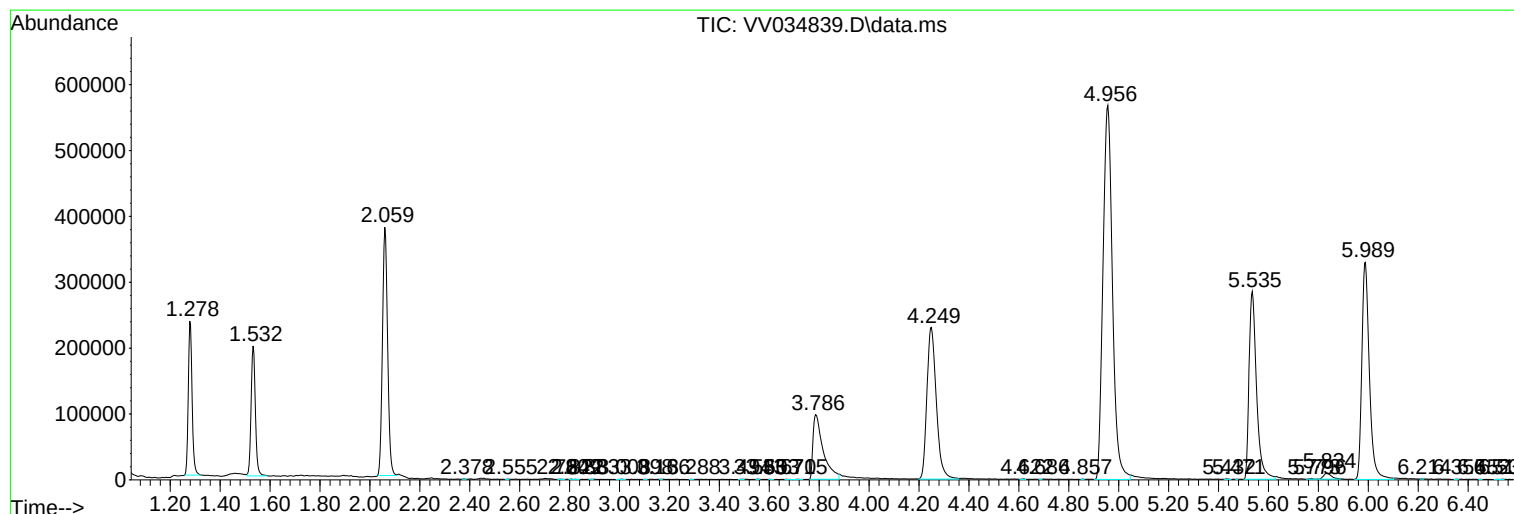

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
Data File : VV034839.D
Acq On : 26 Mar 2024 19:53
Operator : SY/MD
Sample : P1851-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
Data File : VV034839.D
Acq On : 26 Mar 2024 19:53
Operator : SY/MD
Sample : P1851-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------