

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
 Data File : VV034841.D
 Acq On : 26 Mar 2024 20:40
 Operator : SY/MD
 Sample : P1852-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034841.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	88	rBV	197379	207739	15.70%	2.414%
2	1.532	146	153	172	rVB	173528	207714	15.70%	2.413%
3	2.060	308	317	331	rBV	329773	479499	36.24%	5.571%
4	2.391	416	420	424	rBV4	455	525	0.04%	0.006%
5	2.449	431	438	443	rBV5	1340	1813	0.14%	0.021%
6	2.539	463	466	468	rBV2	308	255	0.02%	0.003%
7	2.693	511	514	515	rBV2	536	311	0.02%	0.004%
8	2.725	523	524	528	rBV2	389	290	0.02%	0.003%
9	2.863	560	567	572	rBV4	454	562	0.04%	0.007%
10	2.928	584	587	591	rVB3	426	284	0.02%	0.003%
11	2.957	593	596	599	rBV2	410	231	0.02%	0.003%
12	3.143	651	654	658	rVB	245	137	0.01%	0.002%
13	3.166	658	661	663	rBV	343	169	0.01%	0.002%
14	3.285	696	698	701	rVB3	343	184	0.01%	0.002%
15	3.387	727	730	731	rBV	253	156	0.01%	0.002%
16	3.452	747	750	753	rVB3	506	208	0.02%	0.002%
17	3.471	753	756	760	rBV3	354	305	0.02%	0.004%
18	3.506	763	767	768	rBV	349	271	0.02%	0.003%
19	3.545	776	779	783	rBV3	284	210	0.02%	0.002%
20	3.603	795	797	800	rVB2	361	201	0.02%	0.002%
21	3.693	823	825	828	rBV	434	330	0.02%	0.004%
22	3.754	837	844	847	rBV2	376	380	0.03%	0.004%
23	3.789	847	855	910	rBV	85408	275922	20.85%	3.206%
24	4.143	963	965	966	rBV	424	147	0.01%	0.002%
25	4.185	976	978	981	rBV2	430	275	0.02%	0.003%
26	4.249	983	998	1027	rVV	203853	520972	39.37%	6.053%
27	4.760	1155	1157	1161	rVB	441	213	0.02%	0.002%
28	4.805	1168	1171	1173	rVB2	399	211	0.02%	0.002%
29	4.818	1173	1175	1177	rBV2	245	147	0.01%	0.002%
30	4.957	1202	1218	1246	rBV2	496793	1323247	100.00%	15.375%
31	5.423	1359	1363	1364	rBV	385	224	0.02%	0.003%
32	5.468	1375	1377	1379	rBV2	380	166	0.01%	0.002%
33	5.535	1388	1398	1428	rBV	189840	405347	30.63%	4.710%
34	5.834	1481	1491	1492	rBV3	6642	7797	0.59%	0.091%
35	5.989	1526	1539	1565	rBV2	287245	601909	45.49%	6.994%
36	6.265	1619	1625	1628	rBV4	439	496	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
 Data File : VV034841.D
 Acq On : 26 Mar 2024 20:40
 Operator : SY/MD
 Sample : P1852-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.307	1636	1638	1641	rBV	535	298	0.02%	0.003%
38	6.326	1641	1644	1648	rVB3	674	375	0.03%	0.004%
39	6.484	1689	1693	1699	rVB3	359	384	0.03%	0.004%
40	6.561	1714	1717	1720	rVB3	401	201	0.02%	0.002%
41	6.609	1730	1732	1734	rVV2	381	174	0.01%	0.002%
42	6.622	1734	1736	1740	rVB3	330	187	0.01%	0.002%
43	6.731	1768	1770	1773	rBV3	378	190	0.01%	0.002%
44	6.767	1778	1781	1783	rVB	366	186	0.01%	0.002%
45	6.783	1783	1786	1788	rBV	317	231	0.02%	0.003%
46	6.915	1816	1827	1863	rBV	145953	288556	21.81%	3.353%
47	7.153	1898	1901	1903	rBV3	591	435	0.03%	0.005%
48	7.243	1918	1929	1955	rBV	583528	1021985	77.23%	11.875%
49	7.554	2017	2026	2043	rBV	102354	183329	13.85%	2.130%
50	7.812	2104	2106	2111	rBV5	387	247	0.02%	0.003%
51	7.831	2111	2112	2116	rVB2	658	330	0.02%	0.004%
52	7.854	2116	2119	2121	rBV3	301	216	0.02%	0.003%
53	7.915	2135	2138	2140	rBV2	350	226	0.02%	0.003%
54	7.960	2149	2152	2156	rBV2	298	198	0.01%	0.002%
55	7.992	2159	2162	2164	rVB	512	301	0.02%	0.003%
56	8.027	2164	2173	2211	rBV	253735	551998	41.72%	6.414%
57	8.538	2327	2332	2335	rBV4	469	392	0.03%	0.005%
58	8.622	2355	2358	2361	rBV	393	242	0.02%	0.003%
59	8.786	2398	2409	2436	rBV	308060	510919	38.61%	5.937%
60	9.072	2495	2498	2500	rBV3	544	398	0.03%	0.005%
61	9.165	2523	2527	2528	rBV2	405	213	0.02%	0.002%
62	9.204	2536	2539	2541	rBV2	370	191	0.01%	0.002%
63	9.323	2573	2576	2577	rBV	318	179	0.01%	0.002%
64	9.349	2581	2584	2586	rBV2	232	137	0.01%	0.002%
65	9.432	2605	2610	2614	rVB5	486	461	0.03%	0.005%
66	9.455	2614	2617	2619	rBV	278	147	0.01%	0.002%
67	9.503	2626	2632	2634	rBV4	528	482	0.04%	0.006%
68	9.532	2639	2641	2644	rVB	313	185	0.01%	0.002%
69	9.564	2647	2651	2652	rBV	451	318	0.02%	0.004%
70	9.603	2660	2663	2666	rBV2	372	232	0.02%	0.003%
71	9.644	2674	2676	2679	rVB	378	143	0.01%	0.002%
72	9.689	2687	2690	2694	rBV2	324	224	0.02%	0.003%
73	9.757	2709	2711	2717	rVB3	338	271	0.02%	0.003%
74	9.789	2717	2721	2722	rBV	355	177	0.01%	0.002%
75	9.969	2774	2777	2778	rVV2	330	145	0.01%	0.002%
76	10.152	2822	2834	2857	rBV	384616	621902	47.00%	7.226%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
 Data File : VV034841.D
 Acq On : 26 Mar 2024 20:40
 Operator : SY/MD
 Sample : P1852-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.529	2946	2951	2952	rBV3	288	235	0.02%	0.003%
78	10.574	2963	2965	2968	rBV2	296	173	0.01%	0.002%
79	10.654	2987	2990	2995	rVB2	398	260	0.02%	0.003%
80	10.792	3023	3033	3036	rBV	382	520	0.04%	0.006%
81	10.812	3037	3039	3043	rVV2	248	151	0.01%	0.002%
82	11.185	3145	3155	3175	rBV	284978	459460	34.72%	5.339%
83	11.304	3190	3192	3196	rBV3	657	358	0.03%	0.004%
84	11.474	3243	3245	3247	rBV2	285	155	0.01%	0.002%
85	11.503	3251	3254	3255	rBV2	341	224	0.02%	0.003%
86	11.558	3255	3271	3296	rBV	568049	912704	68.97%	10.605%
87	11.950	3391	3393	3395	rBV2	395	158	0.01%	0.002%
88	11.979	3399	3402	3408	rVB3	397	246	0.02%	0.003%
89	12.004	3408	3410	3412	rBV	270	177	0.01%	0.002%
90	12.284	3494	3497	3501	rVB2	443	323	0.02%	0.004%
91	12.316	3505	3507	3509	rBV	315	141	0.01%	0.002%
92	12.361	3518	3521	3525	rBV2	424	313	0.02%	0.004%
93	12.992	3714	3717	3720	rBV3	262	218	0.02%	0.003%
94	13.014	3720	3724	3726	rBV2	509	315	0.02%	0.004%
95	13.143	3762	3764	3765	rBV2	356	130	0.01%	0.002%
96	13.252	3794	3798	3801	rVB2	434	338	0.03%	0.004%
97	13.284	3806	3808	3810	rBV2	341	179	0.01%	0.002%
98	13.455	3852	3861	3864	rBV4	2229	2814	0.21%	0.033%
99	13.728	3944	3946	3949	rBV2	447	314	0.02%	0.004%
100	14.464	4173	4175	4177	rBV2	487	211	0.02%	0.002%




Sum of corrected areas: 8606369

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
Data File : VV034841.D
Acq On : 26 Mar 2024 20:40
Operator : SY/MD
Sample : P1852-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOLY2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

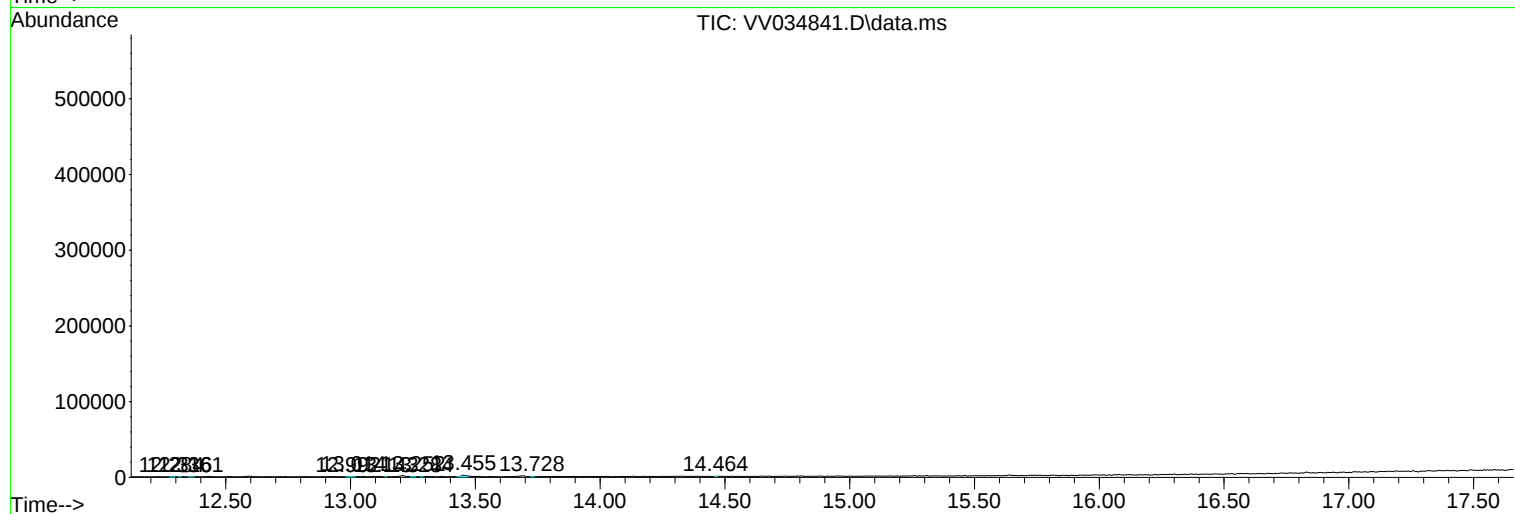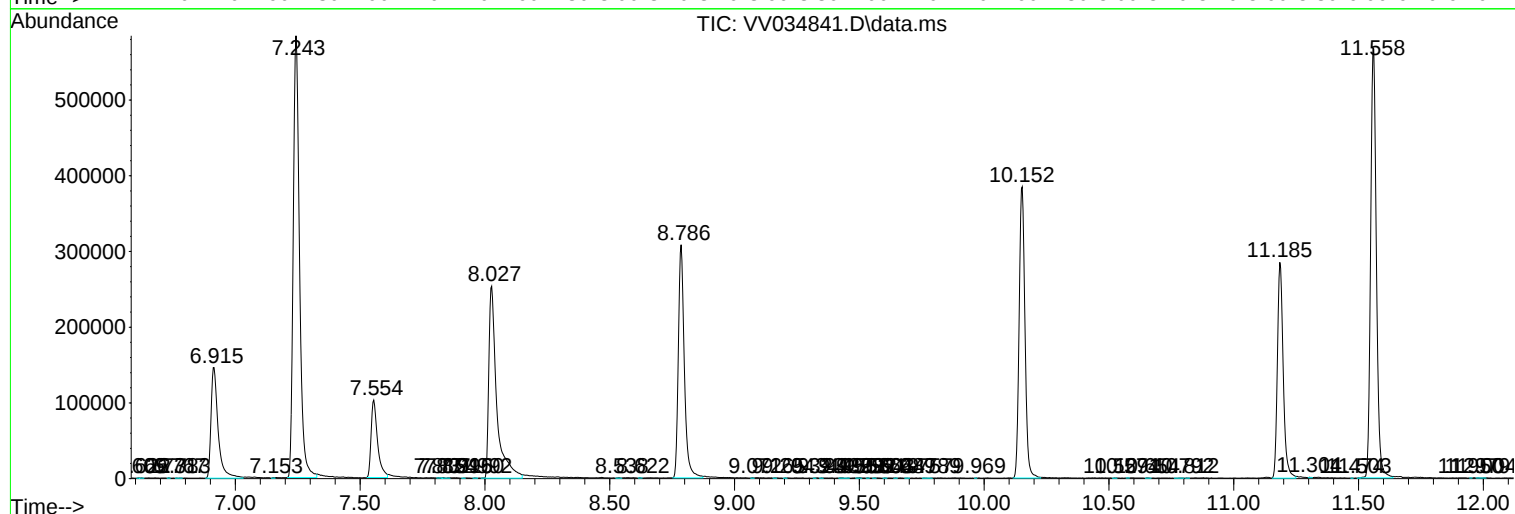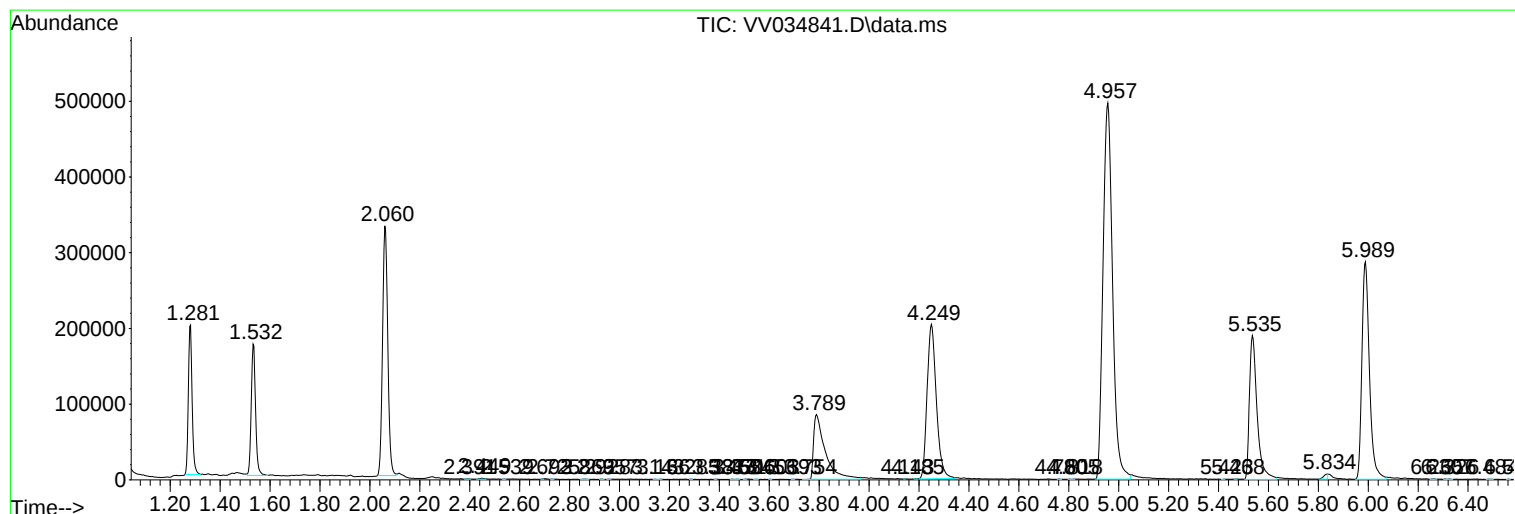

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
Data File : VV034841.D
Acq On : 26 Mar 2024 20:40
Operator : SY/MD
Sample : P1852-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LY2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
Data File : VV034841.D
Acq On : 26 Mar 2024 20:40
Operator : SY/MD
Sample : P1852-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LY2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
