

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
 Data File : VV034843.D
 Acq On : 26 Mar 2024 21:28
 Operator : SY/MD
 Sample : P1852-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLY4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034843.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	90	rVB2	221870	237714	19.03%	2.589%
2	1.532	147	153	168	rVB	164052	189801	15.20%	2.067%
3	2.059	308	317	331	rBV	304806	442888	35.46%	4.823%
4	2.230	367	370	371	rBV2	1005	602	0.05%	0.007%
5	2.683	506	511	513	rBV3	882	667	0.05%	0.007%
6	2.703	514	517	522	rVV6	1282	1266	0.10%	0.014%
7	2.870	567	569	573	rBV2	223	173	0.01%	0.002%
8	2.889	573	575	578	rBV2	373	284	0.02%	0.003%
9	2.973	599	601	604	rVB2	263	163	0.01%	0.002%
10	2.998	604	609	610	rBV2	395	321	0.03%	0.003%
11	3.043	620	623	627	rBV3	250	221	0.02%	0.002%
12	3.172	658	663	664	rBV2	278	210	0.02%	0.002%
13	3.339	711	715	718	rBV2	320	293	0.02%	0.003%
14	3.394	726	732	735	rBV3	384	287	0.02%	0.003%
15	3.423	738	741	744	rBV2	266	174	0.01%	0.002%
16	3.442	744	747	749	rBV2	311	163	0.01%	0.002%
17	3.481	756	759	762	rBV2	249	193	0.02%	0.002%
18	3.625	802	804	806	rBV	291	158	0.01%	0.002%
19	3.670	810	818	819	rBV3	1321	1413	0.11%	0.015%
20	3.728	834	836	838	rVB2	422	181	0.01%	0.002%
21	3.793	846	856	888	rBV2	84130	307099	24.59%	3.344%
22	4.249	981	998	1027	rBV	190340	498368	39.90%	5.427%
23	4.468	1064	1066	1069	rVB4	632	279	0.02%	0.003%
24	4.545	1088	1090	1091	rBV	486	217	0.02%	0.002%
25	4.645	1117	1121	1123	rBV2	285	181	0.01%	0.002%
26	4.725	1143	1146	1150	rVB2	359	261	0.02%	0.003%
27	4.754	1152	1155	1158	rBV4	434	262	0.02%	0.003%
28	4.802	1166	1170	1171	rBV	276	157	0.01%	0.002%
29	4.821	1174	1176	1181	rBV2	336	220	0.02%	0.002%
30	4.847	1181	1184	1186	rVB2	447	294	0.02%	0.003%
31	4.879	1191	1194	1196	rBV2	513	332	0.03%	0.004%
32	4.956	1201	1218	1253	rBV2	466303	1248979	100.00%	13.601%
33	5.394	1351	1354	1357	rBV2	577	394	0.03%	0.004%
34	5.452	1368	1372	1377	rBV2	323	314	0.03%	0.003%
35	5.535	1387	1398	1431	rBV	309331	651049	52.13%	7.090%
36	5.837	1483	1492	1519	rVB5	7801	18461	1.48%	0.201%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032624\
 Data File : VW034843.D
 Acq On : 26 Mar 2024 21:28
 Operator : SY/MD
 Sample : P1852-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLY4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.989	1526	1539	1565	rBV	272101	564279	45.18%	6.145%
38	6.381	1659	1661	1666	rVB3	414	251	0.02%	0.003%
39	6.529	1703	1707	1708	rBV	248	191	0.02%	0.002%
40	6.654	1742	1746	1750	rVV2	377	365	0.03%	0.004%
41	6.786	1784	1787	1789	rBV2	353	189	0.02%	0.002%
42	6.799	1789	1791	1796	rVB	245	164	0.01%	0.002%
43	6.870	1809	1813	1815	rBV2	304	253	0.02%	0.003%
44	6.915	1816	1827	1863	rVV	136732	268633	21.51%	2.925%
45	7.243	1918	1929	1957	rBV	533235	940824	75.33%	10.245%
46	7.513	2010	2013	2015	rBV2	360	241	0.02%	0.003%
47	7.554	2016	2026	2056	rVV	92942	176687	14.15%	1.924%
48	7.786	2096	2098	2101	rBV3	579	420	0.03%	0.005%
49	7.831	2109	2112	2113	rVB	418	176	0.01%	0.002%
50	7.863	2118	2122	2125	rBV6	534	462	0.04%	0.005%
51	7.915	2134	2138	2141	rBV2	603	464	0.04%	0.005%
52	7.976	2153	2157	2159	rBV2	448	233	0.02%	0.003%
53	7.992	2159	2162	2164	rVB2	397	180	0.01%	0.002%
54	8.027	2164	2173	2213	rBV	237509	513591	41.12%	5.593%
55	8.561	2336	2339	2342	rBV3	439	328	0.03%	0.004%
56	8.661	2367	2370	2372	rBV2	714	526	0.04%	0.006%
57	8.734	2392	2393	2398	rVB3	692	356	0.03%	0.004%
58	8.783	2398	2408	2432	rBV	482545	826645	66.19%	9.002%
59	9.062	2493	2495	2499	rBV3	594	384	0.03%	0.004%
60	9.178	2529	2531	2536	rVB4	509	378	0.03%	0.004%
61	9.259	2550	2556	2558	rBV3	546	367	0.03%	0.004%
62	9.361	2586	2588	2592	rVB2	501	304	0.02%	0.003%
63	9.387	2592	2596	2598	rBV2	518	460	0.04%	0.005%
64	9.400	2598	2600	2602	rVV	468	169	0.01%	0.002%
65	9.487	2621	2627	2629	rBV4	827	704	0.06%	0.008%
66	9.590	2657	2659	2661	rBV2	357	157	0.01%	0.002%
67	9.751	2703	2709	2712	rVV3	492	553	0.04%	0.006%
68	9.824	2730	2732	2735	rVB3	573	256	0.02%	0.003%
69	9.873	2740	2747	2759	rVB4	2570	4180	0.33%	0.046%
70	10.030	2793	2796	2801	rBV2	403	297	0.02%	0.003%
71	10.066	2804	2807	2811	rVB4	430	295	0.02%	0.003%
72	10.152	2821	2834	2862	rBV	364344	583843	46.75%	6.358%
73	10.468	2926	2932	2934	rBV3	734	721	0.06%	0.008%
74	10.731	3011	3014	3016	rBV	345	202	0.02%	0.002%
75	10.789	3026	3032	3034	rBV2	568	527	0.04%	0.006%
76	10.840	3045	3048	3051	rBV2	314	194	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
 Data File : VV034843.D
 Acq On : 26 Mar 2024 21:28
 Operator : SY/MD
 Sample : P1852-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LY4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.869	3051	3057	3059	rBV4	480	509	0.04%	0.006%
78	10.953	3079	3083	3086	rBV2	345	246	0.02%	0.003%
79	11.130	3131	3138	3144	rBV5	1592	1828	0.15%	0.020%
80	11.185	3144	3155	3178	rBV	488836	758051	60.69%	8.255%
81	11.394	3214	3220	3222	rBV5	1077	1072	0.09%	0.012%
82	11.467	3235	3243	3258	rVB4	9055	16058	1.29%	0.175%
83	11.558	3258	3271	3295	rBV	528677	854873	68.45%	9.309%
84	11.918	3382	3383	3385	rBV	413	205	0.02%	0.002%
85	11.959	3388	3396	3403	rVV3	5742	9541	0.76%	0.104%
86	12.056	3418	3426	3435	rBV6	4011	6173	0.49%	0.067%
87	12.162	3456	3459	3462	rBV	264	165	0.01%	0.002%
88	12.236	3479	3482	3485	rBV3	1176	774	0.06%	0.008%
89	12.281	3494	3496	3500	rBV2	261	183	0.01%	0.002%
90	12.352	3510	3518	3527	rBV3	6747	10256	0.82%	0.112%
91	12.432	3540	3543	3546	rBV2	598	321	0.03%	0.003%
92	12.448	3546	3548	3551	rBV	492	271	0.02%	0.003%
93	12.477	3554	3557	3559	rBV3	588	420	0.03%	0.005%
94	12.583	3587	3590	3597	rBV5	1494	1314	0.11%	0.014%
95	12.741	3636	3639	3645	rVB3	486	413	0.03%	0.004%
96	12.770	3645	3648	3649	rBV3	436	172	0.01%	0.002%
97	12.821	3654	3664	3674	rBV5	13358	21345	1.71%	0.232%
98	12.940	3695	3701	3705	rBV4	667	989	0.08%	0.011%
99	13.033	3728	3730	3734	rBV	307	190	0.02%	0.002%
100	13.207	3777	3784	3795	rVB7	2712	3991	0.32%	0.043%




Sum of corrected areas: 9182848

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
Data File : VV034843.D
Acq On : 26 Mar 2024 21:28
Operator : SY/MD
Sample : P1852-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOLY4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

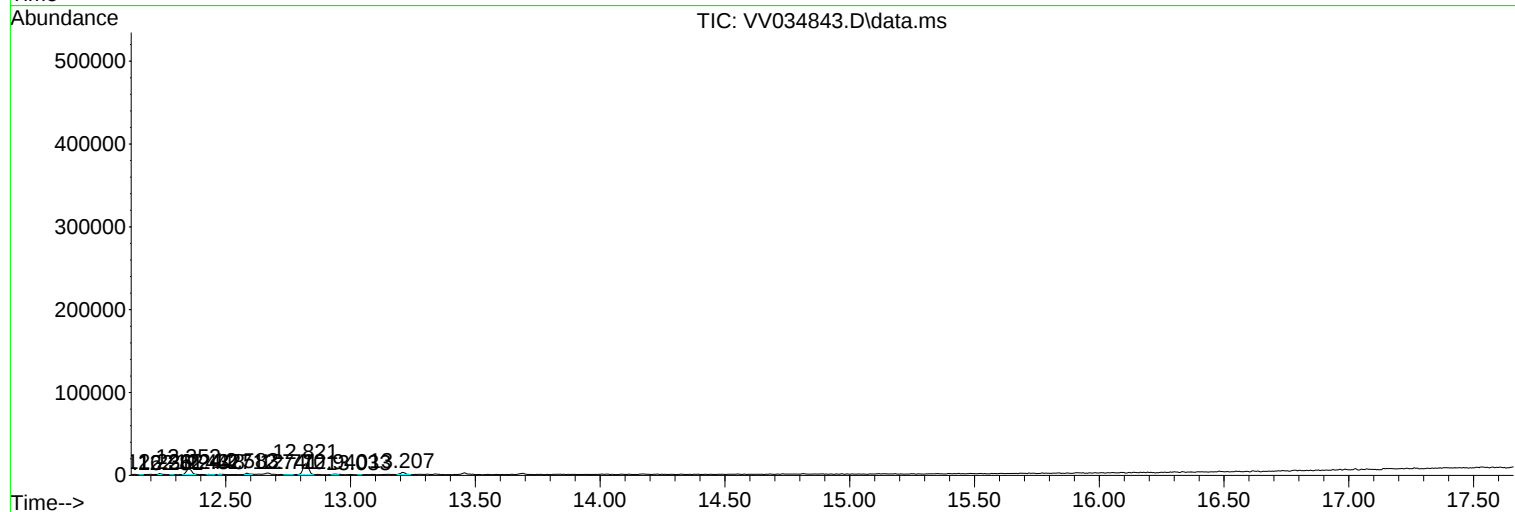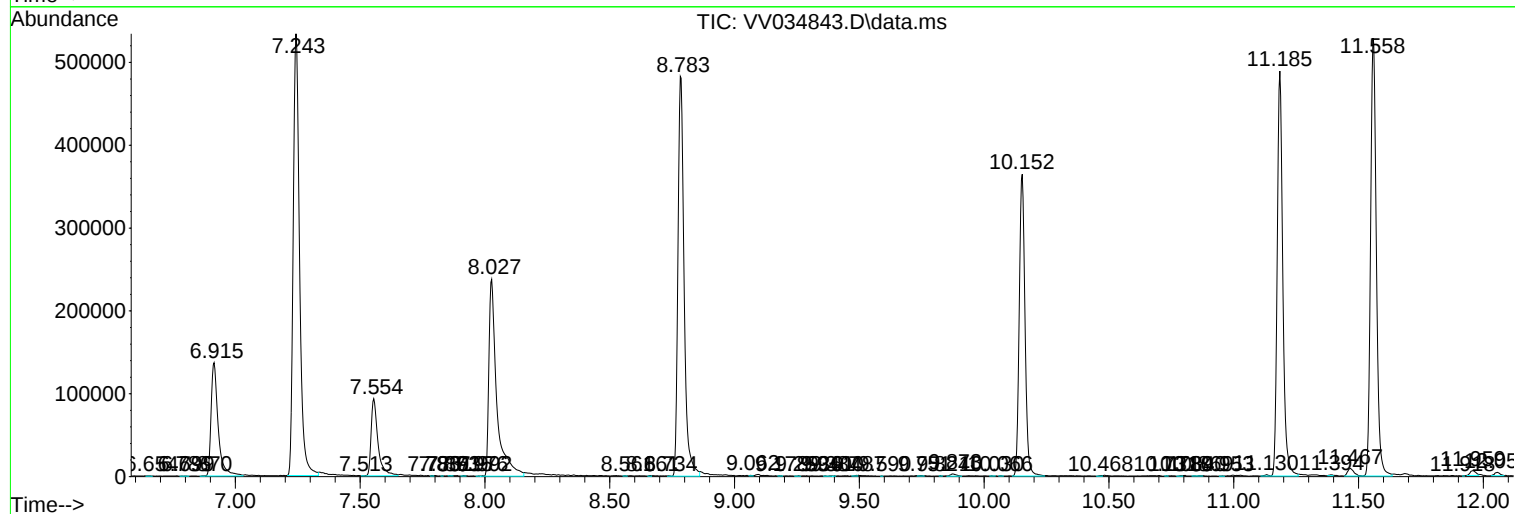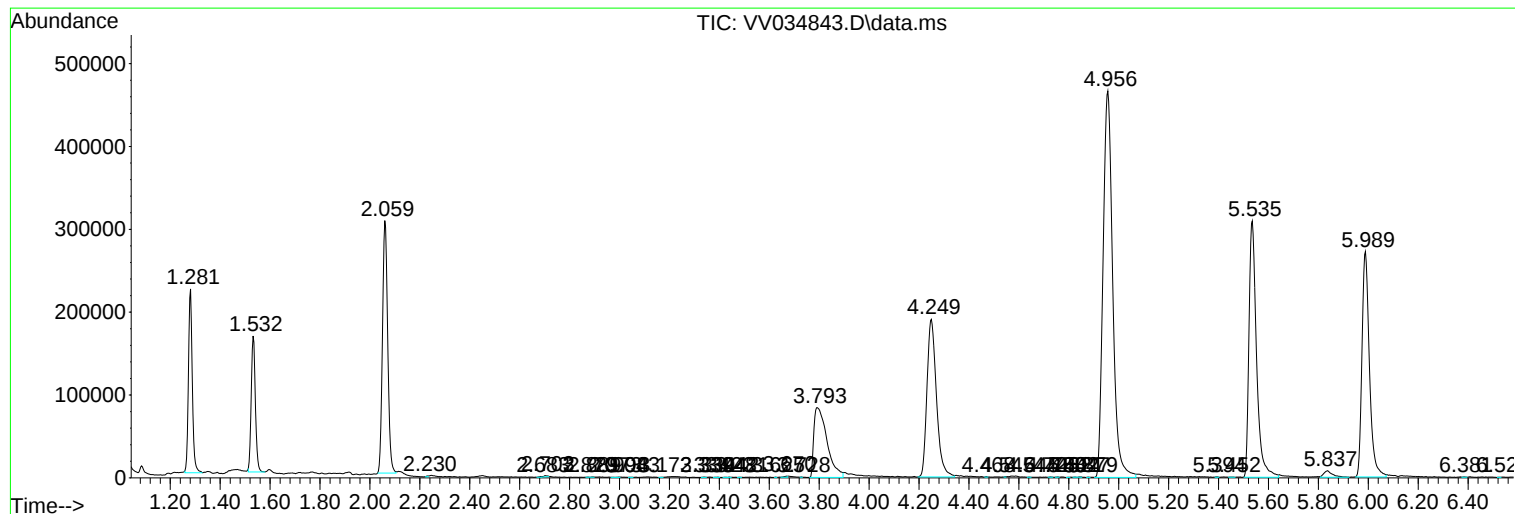

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
Data File : VV034843.D
Acq On : 26 Mar 2024 21:28
Operator : SY/MD
Sample : P1852-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LY4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
Data File : VV034843.D
Acq On : 26 Mar 2024 21:28
Operator : SY/MD
Sample : P1852-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LY4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc