

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
 Data File : VV034845.D
 Acq On : 26 Mar 2024 22:16
 Operator : SY/MD
 Sample : P1852-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034845.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	207496	216158	15.11%	2.067%
2	1.532	146	153	169	rVB	188329	221817	15.50%	2.121%
3	2.060	308	317	330	rBV	351236	501814	35.07%	4.798%
4	2.503	450	455	456	rBV2	493	379	0.03%	0.004%
5	2.555	469	471	473	rBV	412	163	0.01%	0.002%
6	2.651	499	501	503	rBV3	343	172	0.01%	0.002%
7	2.667	503	506	511	rVV2	616	572	0.04%	0.005%
8	2.744	527	530	534	rBV2	417	274	0.02%	0.003%
9	2.883	571	573	575	rBV2	594	309	0.02%	0.003%
10	2.982	600	604	606	rBV	308	232	0.02%	0.002%
11	3.121	643	647	650	rVB	678	424	0.03%	0.004%
12	3.162	656	660	661	rBV2	402	178	0.01%	0.002%
13	3.246	681	686	690	rBV4	352	377	0.03%	0.004%
14	3.301	699	703	705	rVB	278	152	0.01%	0.001%
15	3.416	735	739	744	rVB2	408	312	0.02%	0.003%
16	3.445	744	748	751	rBV2	366	332	0.02%	0.003%
17	3.465	751	754	755	rBV2	458	277	0.02%	0.003%
18	3.590	790	793	795	rBV2	419	178	0.01%	0.002%
19	3.664	813	816	822	rBV2	198	169	0.01%	0.002%
20	3.786	840	854	891	rBV	90678	269385	18.83%	2.576%
21	4.249	982	998	1027	rBV	220909	565812	39.55%	5.410%
22	4.526	1079	1084	1087	rBV5	857	661	0.05%	0.006%
23	4.683	1127	1133	1134	rBV	719	527	0.04%	0.005%
24	4.953	1199	1217	1263	rBV2	534122	1430777	100.00%	13.681%
25	5.387	1350	1352	1356	rBV3	604	279	0.02%	0.003%
26	5.532	1386	1397	1432	rBV	383060	795913	55.63%	7.611%
27	5.831	1480	1490	1502	rBV4	10681	24063	1.68%	0.230%
28	5.989	1519	1539	1570	rBV	310573	656715	45.90%	6.280%
29	6.304	1632	1637	1639	rBV5	555	433	0.03%	0.004%
30	6.455	1681	1684	1686	rBV3	372	256	0.02%	0.002%
31	6.503	1694	1699	1702	rBV6	578	538	0.04%	0.005%
32	6.532	1707	1708	1712	rVB	533	300	0.02%	0.003%
33	6.561	1712	1717	1720	rBV2	317	213	0.01%	0.002%
34	6.612	1730	1733	1735	rBV3	285	154	0.01%	0.001%
35	6.625	1735	1737	1741	rBV2	366	279	0.02%	0.003%
36	6.686	1752	1756	1757	rBV2	380	187	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
 Data File : VV034845.D
 Acq On : 26 Mar 2024 22:16
 Operator : SY/MD
 Sample : P1852-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.719	1764	1766	1769	rVB2	302	167	0.01%	0.002%
38	6.776	1782	1784	1787	rBV	404	162	0.01%	0.002%
39	6.805	1790	1793	1797	rVB2	227	155	0.01%	0.001%
40	6.844	1803	1805	1808	rVB2	350	174	0.01%	0.002%
41	6.915	1816	1827	1857	rBV	158013	306883	21.45%	2.935%
42	7.175	1905	1908	1910	rBV	657	421	0.03%	0.004%
43	7.243	1918	1929	1954	rBV	623098	1097538	76.71%	10.495%
44	7.516	2012	2014	2015	rBV	550	235	0.02%	0.002%
45	7.555	2016	2026	2050	rVV	108277	202277	14.14%	1.934%
46	7.854	2115	2119	2121	rBV2	633	447	0.03%	0.004%
47	7.972	2154	2156	2159	rBV2	337	194	0.01%	0.002%
48	7.992	2159	2162	2163	rBV2	491	315	0.02%	0.003%
49	8.024	2163	2172	2217	rBV2	275483	593318	41.47%	5.673%
50	8.551	2334	2336	2338	rBV	446	274	0.02%	0.003%
51	8.657	2366	2369	2373	rBV3	508	380	0.03%	0.004%
52	8.783	2397	2408	2434	rBV	603158	991866	69.32%	9.484%
53	9.005	2475	2477	2479	rVB3	671	307	0.02%	0.003%
54	9.079	2497	2500	2503	rBV3	572	412	0.03%	0.004%
55	9.117	2510	2512	2518	rVB4	710	540	0.04%	0.005%
56	9.149	2518	2522	2523	rBV	414	319	0.02%	0.003%
57	9.210	2536	2541	2544	rBV3	437	399	0.03%	0.004%
58	9.236	2547	2549	2554	rVB4	540	408	0.03%	0.004%
59	9.355	2582	2586	2587	rBV2	413	248	0.02%	0.002%
60	9.442	2610	2613	2618	rVB3	577	498	0.03%	0.005%
61	9.490	2624	2628	2630	rBV3	713	450	0.03%	0.004%
62	9.522	2637	2638	2642	rBV2	330	163	0.01%	0.002%
63	9.593	2658	2660	2664	rVB	354	223	0.02%	0.002%
64	9.670	2682	2684	2690	rVB2	448	311	0.02%	0.003%
65	9.702	2690	2694	2696	rBV	177	156	0.01%	0.001%
66	9.731	2699	2703	2704	rBV3	283	208	0.01%	0.002%
67	9.876	2742	2748	2750	rBV5	783	735	0.05%	0.007%
68	9.982	2777	2781	2785	rVB3	449	370	0.03%	0.004%
69	10.152	2822	2834	2860	rBV	418491	667589	46.66%	6.384%
70	10.361	2897	2899	2903	rVB3	622	407	0.03%	0.004%
71	10.381	2903	2905	2907	rBV	369	197	0.01%	0.002%
72	10.525	2948	2950	2955	rVB3	300	204	0.01%	0.002%
73	10.686	2996	3000	3005	rVB2	312	214	0.01%	0.002%
74	10.940	3077	3079	3084	rVB2	372	240	0.02%	0.002%
75	10.992	3091	3095	3099	rBV2	359	246	0.02%	0.002%
76	11.014	3099	3102	3105	rBV2	278	226	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
 Data File : VV034845.D
 Acq On : 26 Mar 2024 22:16
 Operator : SY/MD
 Sample : P1852-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	11.046	3110	3112	3113	rBV	478	162	0.01%	0.002%
78	11.127	3131	3137	3139	rBV6	791	774	0.05%	0.007%
79	11.185	3144	3155	3180	rBV	580411	912366	63.77%	8.724%
80	11.426	3229	3230	3233	rBV	447	218	0.02%	0.002%
81	11.558	3254	3271	3293	rBV	617453	977748	68.34%	9.349%
82	11.744	3327	3329	3332	rBV2	579	343	0.02%	0.003%
83	11.847	3359	3361	3364	rVB2	387	175	0.01%	0.002%
84	11.966	3396	3398	3400	rVB2	467	196	0.01%	0.002%
85	12.220	3474	3477	3479	rBV2	401	267	0.02%	0.003%
86	12.268	3489	3492	3493	rBV2	438	187	0.01%	0.002%
87	12.416	3535	3538	3541	rBV3	326	269	0.02%	0.003%
88	12.471	3552	3555	3558	rBV2	335	217	0.02%	0.002%
89	12.593	3586	3593	3594	rBV2	659	664	0.05%	0.006%
90	12.779	3647	3651	3652	rBV2	357	220	0.02%	0.002%
91	12.853	3671	3674	3680	rBV2	471	449	0.03%	0.004%
92	12.898	3684	3688	3690	rBV	331	214	0.01%	0.002%
93	13.069	3739	3741	3745	rBV2	283	154	0.01%	0.001%
94	13.249	3794	3797	3800	rBV2	268	203	0.01%	0.002%
95	13.320	3816	3819	3821	rBV2	397	217	0.02%	0.002%
96	13.596	3903	3905	3908	rBV2	410	181	0.01%	0.002%
97	13.689	3930	3934	3938	rBV3	796	641	0.04%	0.006%
98	13.824	3974	3976	3979	rBV	577	414	0.03%	0.004%
99	13.988	4024	4027	4029	rBV2	408	307	0.02%	0.003%
100	15.168	4392	4394	4398	rBV3	775	515	0.04%	0.005%




Sum of corrected areas: 10457758

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
Data File : VV034845.D
Acq On : 26 Mar 2024 22:16
Operator : SY/MD
Sample : P1852-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOLY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

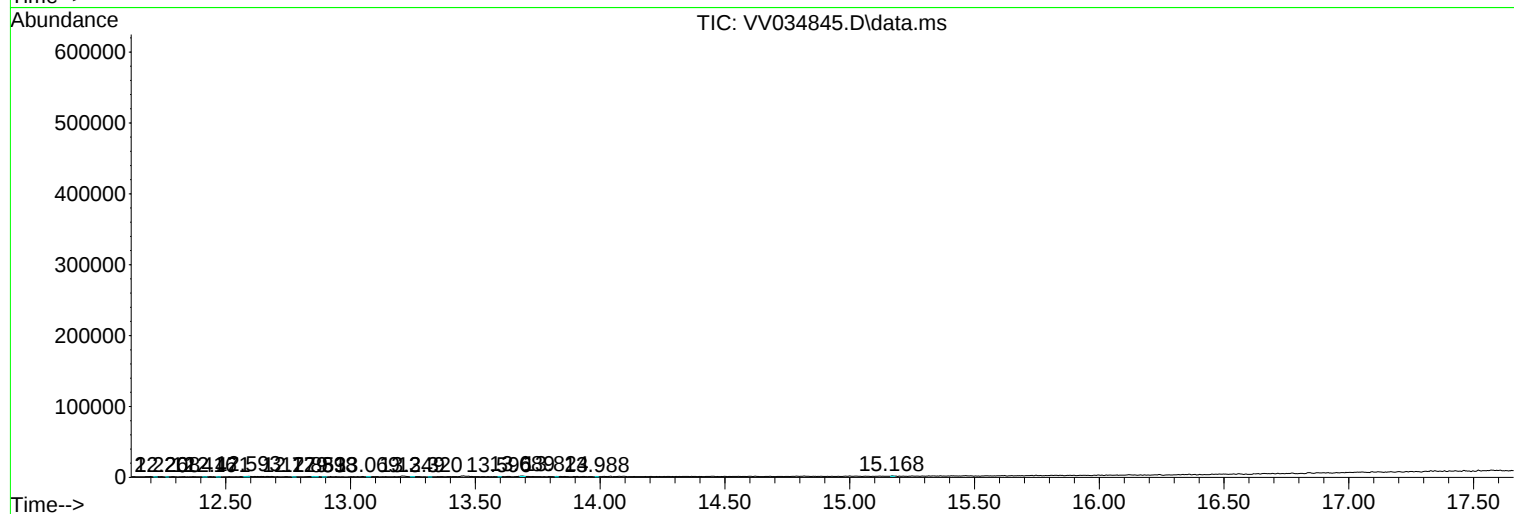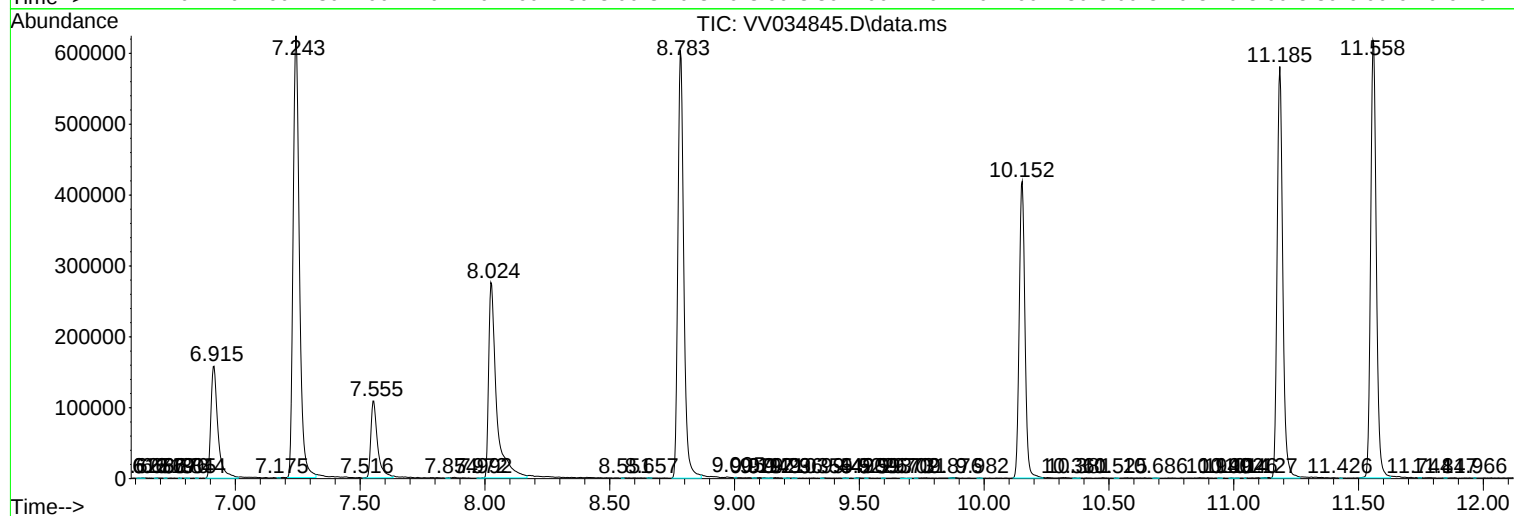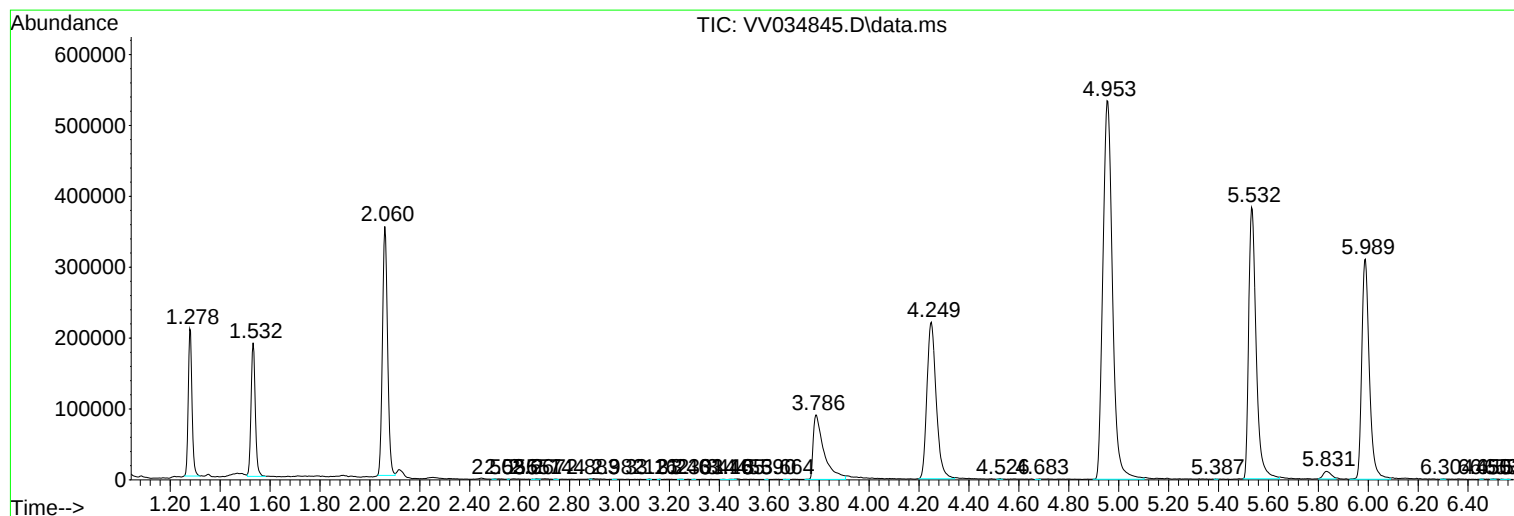

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
Data File : VV034845.D
Acq On : 26 Mar 2024 22:16
Operator : SY/MD
Sample : P1852-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
Data File : VV034845.D
Acq On : 26 Mar 2024 22:16
Operator : SY/MD
Sample : P1852-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc