

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
 Data File : VV034846.D
 Acq On : 26 Mar 2024 22:40
 Operator : SY/MD
 Sample : P1851-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LX9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV034846.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	202486	213728	15.22%	2.035%
2	1.532	146	153	168	rVB	190346	224238	15.96%	2.135%
3	2.060	308	317	331	rBV	343482	496555	35.35%	4.727%
4	2.249	367	376	381	rBV5	2337	4560	0.32%	0.043%
5	2.510	451	457	458	rBV2	531	520	0.04%	0.005%
6	2.709	510	519	529	rVB8	2684	4905	0.35%	0.047%
7	2.786	541	543	549	rVB4	407	281	0.02%	0.003%
8	2.844	558	561	563	rBV2	513	367	0.03%	0.003%
9	2.870	566	569	570	rBV2	686	382	0.03%	0.004%
10	3.073	628	632	635	rBV2	368	217	0.02%	0.002%
11	3.214	668	676	678	rBV5	1213	1630	0.12%	0.016%
12	3.285	696	698	700	rBV2	454	161	0.01%	0.002%
13	3.298	700	702	706	rVB2	398	244	0.02%	0.002%
14	3.352	714	719	721	rBV3	361	370	0.03%	0.004%
15	3.391	729	731	735	rBV2	274	217	0.02%	0.002%
16	3.423	738	741	743	rBV	271	161	0.01%	0.002%
17	3.455	745	751	754	rVB2	273	266	0.02%	0.003%
18	3.494	758	763	766	rBV2	278	276	0.02%	0.003%
19	3.552	779	781	786	rVB3	361	239	0.02%	0.002%
20	3.635	803	807	809	rBV3	249	179	0.01%	0.002%
21	3.651	809	812	816	rVV	362	314	0.02%	0.003%
22	3.680	818	821	824	rVV	319	193	0.01%	0.002%
23	3.719	829	833	834	rBV	380	209	0.01%	0.002%
24	3.790	843	855	886	rBV3	111594	340507	24.24%	3.242%
25	4.246	982	997	1028	rBV	218891	566669	40.34%	5.395%
26	4.564	1094	1096	1098	rBV2	524	239	0.02%	0.002%
27	4.751	1150	1154	1156	rVV3	545	379	0.03%	0.004%
28	4.783	1162	1164	1167	rVB2	753	370	0.03%	0.004%
29	4.806	1167	1171	1173	rBV2	566	410	0.03%	0.004%
30	4.863	1188	1189	1194	rVB2	528	272	0.02%	0.003%
31	4.957	1202	1218	1256	rBV2	526284	1404688	100.00%	13.373%
32	5.532	1386	1397	1432	rBV	367538	767341	54.63%	7.305%
33	5.928	1516	1520	1523	rBV4	621	570	0.04%	0.005%
34	5.989	1524	1539	1565	rBV	307805	651533	46.38%	6.203%
35	6.230	1612	1614	1621	rBV4	786	659	0.05%	0.006%
36	6.301	1631	1636	1640	rBV5	1086	1222	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
 Data File : VV034846.D
 Acq On : 26 Mar 2024 22:40
 Operator : SY/MD
 Sample : P1851-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LX9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.384	1660	1662	1664	rBV3	479	281	0.02%	0.003%
38	6.474	1687	1690	1691	rBV	495	320	0.02%	0.003%
39	6.593	1724	1727	1729	rBV2	532	229	0.02%	0.002%
40	6.732	1765	1770	1771	rBV	317	258	0.02%	0.002%
41	6.912	1816	1826	1858	rBV	157151	305812	21.77%	2.911%
42	7.243	1918	1929	1952	rBV	609854	1074841	76.52%	10.233%
43	7.555	2016	2026	2052	rBV	107629	200460	14.27%	1.908%
44	7.757	2087	2089	2091	rBV4	511	193	0.01%	0.002%
45	7.799	2098	2102	2111	rVB5	613	837	0.06%	0.008%
46	7.841	2111	2115	2116	rBV	432	224	0.02%	0.002%
47	7.976	2155	2157	2159	rBV2	372	180	0.01%	0.002%
48	8.024	2163	2172	2209	rBV	323689	671962	47.84%	6.397%
49	8.712	2382	2386	2388	rBV3	493	369	0.03%	0.004%
50	8.783	2397	2408	2431	rBV	583414	973551	69.31%	9.269%
51	9.149	2519	2522	2526	rBV3	649	611	0.04%	0.006%
52	9.204	2537	2539	2544	rBV3	926	735	0.05%	0.007%
53	9.239	2548	2550	2552	rBV	440	220	0.02%	0.002%
54	9.323	2571	2576	2578	rBV	313	233	0.02%	0.002%
55	9.339	2579	2581	2587	rVB3	435	365	0.03%	0.003%
56	9.375	2588	2592	2594	rVV3	543	338	0.02%	0.003%
57	9.432	2606	2610	2611	rBV2	379	266	0.02%	0.003%
58	9.468	2617	2621	2624	rBV4	726	579	0.04%	0.006%
59	9.484	2624	2626	2628	rBV2	923	544	0.04%	0.005%
60	9.551	2642	2647	2650	rVB3	757	576	0.04%	0.005%
61	9.584	2650	2657	2661	rBV3	281	308	0.02%	0.003%
62	9.661	2680	2681	2685	rBV	303	196	0.01%	0.002%
63	9.709	2692	2696	2700	rVB4	435	382	0.03%	0.004%
64	9.748	2703	2708	2710	rBV4	1695	1806	0.13%	0.017%
65	9.879	2745	2749	2752	rBV3	1363	882	0.06%	0.008%
66	9.918	2759	2761	2763	rBV2	440	209	0.01%	0.002%
67	9.950	2766	2771	2774	rBB2	529	421	0.03%	0.004%
68	9.976	2777	2779	2784	rVB3	271	242	0.02%	0.002%
69	10.014	2787	2791	2793	rVB2	540	320	0.02%	0.003%
70	10.095	2812	2816	2818	rBV3	572	338	0.02%	0.003%
71	10.149	2822	2833	2856	rBV	430956	692293	49.28%	6.591%
72	10.326	2885	2888	2890	rBV4	968	635	0.05%	0.006%
73	10.436	2919	2922	2925	rVB2	425	301	0.02%	0.003%
74	10.455	2925	2928	2932	rVB3	624	429	0.03%	0.004%
75	10.484	2933	2937	2945	rBV4	842	805	0.06%	0.008%
76	10.548	2953	2957	2959	rBV2	637	408	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
 Data File : VV034846.D
 Acq On : 26 Mar 2024 22:40
 Operator : SY/MD
 Sample : P1851-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LX9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.735	3011	3015	3018	rBV2	411	360	0.03%	0.003%
78	10.821	3037	3042	3046	rBV4	787	726	0.05%	0.007%
79	10.908	3066	3069	3071	rBV	304	197	0.01%	0.002%
80	10.982	3090	3092	3096	rBV3	442	305	0.02%	0.003%
81	11.005	3096	3099	3101	rBV4	572	333	0.02%	0.003%
82	11.034	3106	3108	3112	rBV2	471	393	0.03%	0.004%
83	11.108	3126	3131	3132	rBV3	463	305	0.02%	0.003%
84	11.120	3132	3135	3138	rBV4	996	766	0.05%	0.007%
85	11.185	3144	3155	3179	rBV	556540	876058	62.37%	8.341%
86	11.429	3228	3231	3234	rBV4	869	812	0.06%	0.008%
87	11.464	3235	3242	3253	rVB2	16329	24135	1.72%	0.230%
88	11.558	3261	3271	3293	rBV	617555	972568	69.24%	9.259%
89	11.905	3376	3379	3380	rBV	591	342	0.02%	0.003%
90	12.227	3477	3479	3486	rVB5	957	809	0.06%	0.008%
91	12.690	3621	3623	3628	rBV3	406	281	0.02%	0.003%
92	12.754	3641	3643	3644	rBV3	381	165	0.01%	0.002%
93	12.950	3700	3704	3707	rBV3	550	455	0.03%	0.004%
94	13.082	3743	3745	3750	rVB3	712	389	0.03%	0.004%
95	13.207	3779	3784	3790	rBV7	1044	1551	0.11%	0.015%
96	13.458	3854	3862	3865	rBV4	1824	2353	0.17%	0.022%
97	13.503	3874	3876	3880	rBV2	494	361	0.03%	0.003%
98	13.853	3983	3985	3988	rBV2	409	187	0.01%	0.002%
99	14.130	4069	4071	4073	rVB2	503	190	0.01%	0.002%
100	14.615	4218	4222	4225	rBB4	758	537	0.04%	0.005%




Sum of corrected areas: 10503608

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
Data File : VV034846.D
Acq On : 26 Mar 2024 22:40
Operator : SY/MD
Sample : P1851-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LX9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

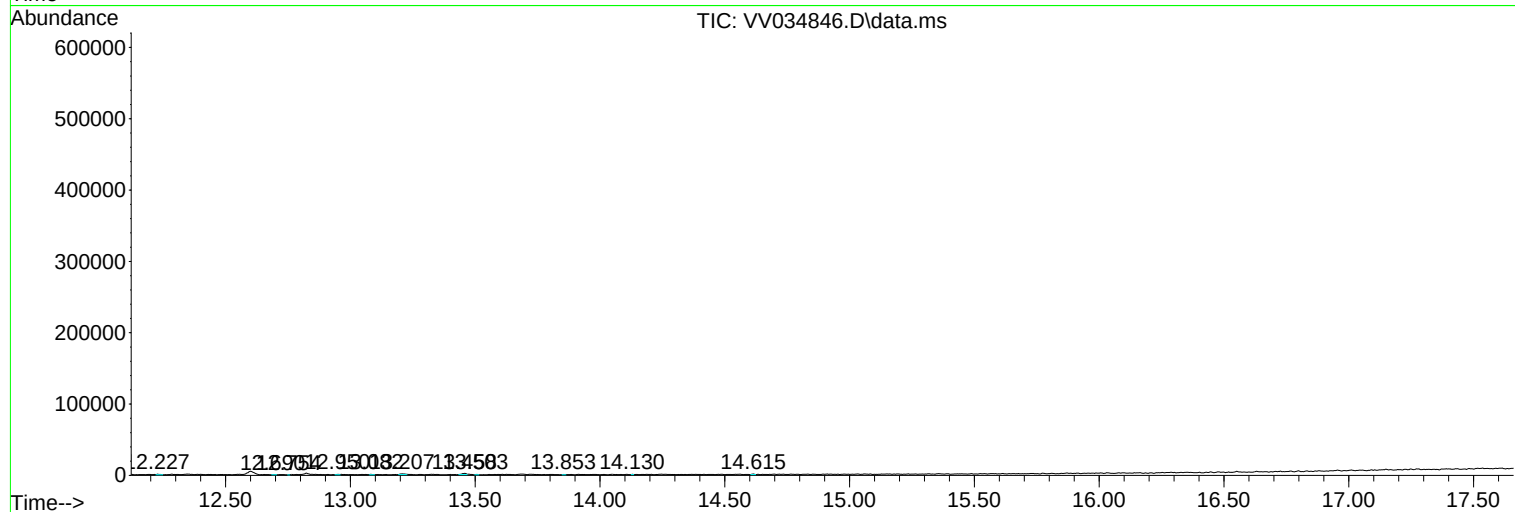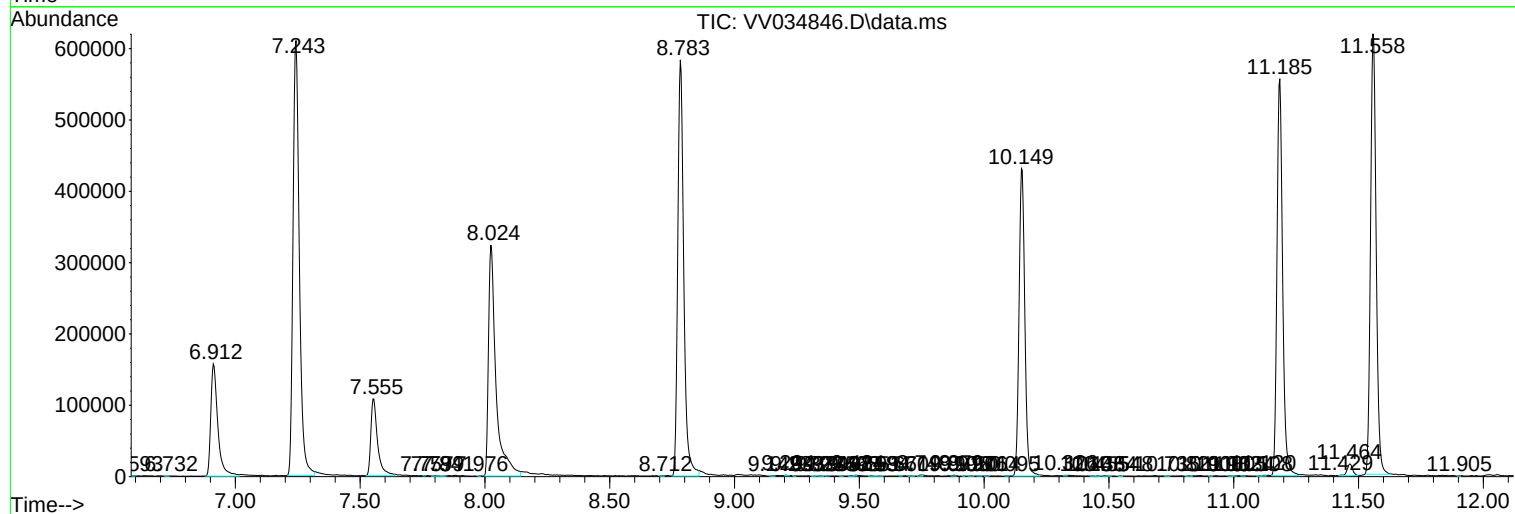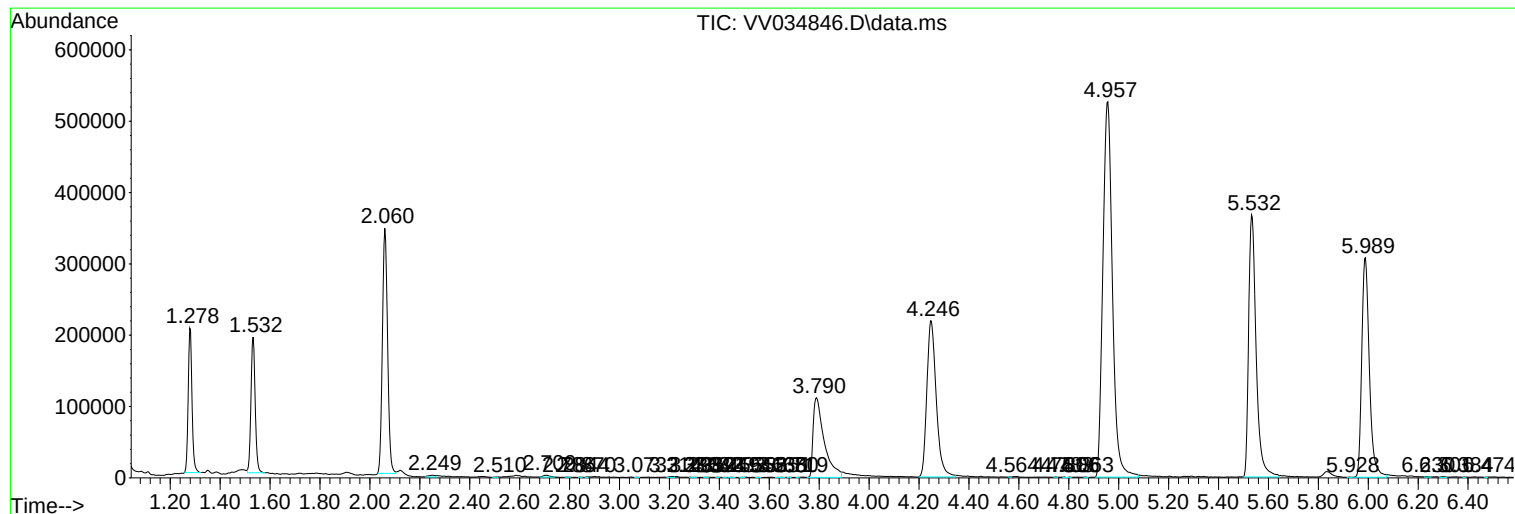

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
Data File : VV034846.D
Acq On : 26 Mar 2024 22:40
Operator : SY/MD
Sample : P1851-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LX9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
Data File : VV034846.D
Acq On : 26 Mar 2024 22:40
Operator : SY/MD
Sample : P1851-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LX9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc