

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
 Data File : VV034851.D
 Acq On : 27 Mar 2024 00:39
 Operator : SY/MD
 Sample : VIBLK275
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK275

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034851.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	256442	273034	15.88%	2.136%
2	1.532	146	153	172	rVB	246568	278400	16.19%	2.178%
3	2.060	307	317	333	rBV	435821	639220	37.18%	5.001%
4	2.532	462	464	465	rBV	306	163	0.01%	0.001%
5	2.635	492	496	497	rBV3	460	322	0.02%	0.003%
6	2.703	510	517	526	rBV5	1755	3519	0.20%	0.028%
7	2.790	540	544	547	rBV2	423	443	0.03%	0.003%
8	2.867	565	568	571	rVB2	270	185	0.01%	0.001%
9	2.915	581	583	584	rBV2	385	204	0.01%	0.002%
10	2.944	590	592	596	rVB	434	259	0.02%	0.002%
11	2.963	596	598	600	rBV2	484	251	0.01%	0.002%
12	2.976	600	602	604	rBV	396	155	0.01%	0.001%
13	3.069	627	631	634	rVB3	440	339	0.02%	0.003%
14	3.124	643	648	653	rVB4	784	781	0.05%	0.006%
15	3.163	657	660	664	rBV3	583	430	0.03%	0.003%
16	3.256	685	689	692	rBV3	522	461	0.03%	0.004%
17	3.282	695	697	700	rVB	474	201	0.01%	0.002%
18	3.320	700	709	713	rBV4	439	571	0.03%	0.004%
19	3.391	730	731	736	rBV2	236	164	0.01%	0.001%
20	3.426	740	742	744	rBV2	251	159	0.01%	0.001%
21	3.645	805	810	814	rBV2	488	398	0.02%	0.003%
22	3.786	843	854	892	rBV	111532	339970	19.78%	2.660%
23	4.246	982	997	1026	rBV	262264	676308	39.34%	5.291%
24	4.465	1062	1065	1069	rBV2	456	318	0.02%	0.002%
25	4.728	1144	1147	1151	rBV3	743	651	0.04%	0.005%
26	4.847	1181	1184	1187	rBV2	409	295	0.02%	0.002%
27	4.953	1201	1217	1248	rBV2	648598	1719096	100.00%	13.449%
28	5.317	1325	1330	1331	rBV3	648	591	0.03%	0.005%
29	5.532	1387	1397	1436	rBV	421952	872498	50.75%	6.826%
30	5.834	1480	1491	1513	rBV5	13849	34189	1.99%	0.267%
31	5.986	1524	1538	1567	rBV	372640	783499	45.58%	6.130%
32	6.317	1638	1641	1643	rBV2	457	231	0.01%	0.002%
33	6.384	1657	1662	1669	rBV2	559	659	0.04%	0.005%
34	6.433	1673	1677	1678	rBV	368	252	0.01%	0.002%
35	6.580	1718	1723	1724	rBV2	477	325	0.02%	0.003%
36	6.635	1735	1740	1742	rBV4	483	452	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032624\
 Data File : VW034851.D
 Acq On : 27 Mar 2024 00:39
 Operator : SY/MD
 Sample : VIBLK275
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK275

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.741	1769	1773	1774	rBV2	386	248	0.01%	0.002%
38	6.912	1811	1826	1864	rBV	197257	380606	22.14%	2.978%
39	7.243	1918	1929	1955	rBV	779307	1356060	78.88%	10.609%
40	7.551	2016	2025	2056	rBV	132651	250040	14.54%	1.956%
41	7.789	2097	2099	2103	rBV3	814	462	0.03%	0.004%
42	7.915	2131	2138	2139	rBV3	1667	1770	0.10%	0.014%
43	8.024	2162	2172	2216	rBV	348519	742617	43.20%	5.810%
44	8.625	2357	2359	2363	rVB4	507	368	0.02%	0.003%
45	8.680	2373	2376	2378	rBV2	468	314	0.02%	0.002%
46	8.722	2386	2389	2390	rBV2	307	187	0.01%	0.001%
47	8.783	2397	2408	2439	rBV	646344	1075591	62.57%	8.415%
48	9.259	2554	2556	2559	rBV	313	174	0.01%	0.001%
49	9.288	2563	2565	2567	rBV	273	157	0.01%	0.001%
50	9.455	2613	2617	2619	rBV2	361	190	0.01%	0.001%
51	9.487	2619	2627	2629	rBV5	3327	3593	0.21%	0.028%
52	9.722	2696	2700	2701	rBV2	390	271	0.02%	0.002%
53	9.757	2707	2711	2714	rBV2	485	393	0.02%	0.003%
54	9.873	2736	2747	2755	rBV3	3470	5617	0.33%	0.044%
55	9.947	2766	2770	2771	rBV	428	268	0.02%	0.002%
56	9.979	2778	2780	2784	rBV	394	247	0.01%	0.002%
57	10.034	2795	2797	2802	rVB3	354	248	0.01%	0.002%
58	10.088	2810	2814	2816	rBV2	415	294	0.02%	0.002%
59	10.149	2821	2833	2865	rBV	500950	803966	46.77%	6.290%
60	10.355	2895	2897	2899	rBV	370	165	0.01%	0.001%
61	10.387	2904	2907	2909	rVB	481	248	0.01%	0.002%
62	10.413	2909	2915	2918	rVB3	477	518	0.03%	0.004%
63	10.432	2918	2921	2922	rBV	243	145	0.01%	0.001%
64	10.458	2927	2929	2930	rBV	371	167	0.01%	0.001%
65	10.590	2967	2970	2972	rBV	227	154	0.01%	0.001%
66	10.725	3007	3012	3016	rBV2	496	409	0.02%	0.003%
67	10.786	3026	3031	3035	rBV4	423	347	0.02%	0.003%
68	10.825	3041	3043	3046	rVB2	399	177	0.01%	0.001%
69	10.860	3046	3054	3066	rBV3	4791	7663	0.45%	0.060%
70	10.924	3069	3074	3077	rBV2	418	323	0.02%	0.003%
71	10.998	3092	3097	3100	rVB3	231	214	0.01%	0.002%
72	11.024	3100	3105	3108	rVB2	530	398	0.02%	0.003%
73	11.053	3111	3114	3117	rBV	246	191	0.01%	0.001%
74	11.082	3120	3123	3128	rBV3	600	552	0.03%	0.004%
75	11.127	3129	3137	3144	rBV2	8178	12157	0.71%	0.095%
76	11.185	3144	3155	3187	rVB	655459	1041896	60.61%	8.151%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
 Data File : VV034851.D
 Acq On : 27 Mar 2024 00:39
 Operator : SY/MD
 Sample : VIBLK275
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK275

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	11.365	3208	3211	3214	rBV3	645	346	0.02%	0.003%
78	11.461	3239	3241	3242	rBV2	469	191	0.01%	0.001%
79	11.509	3252	3256	3258	rBV2	680	459	0.03%	0.004%
80	11.558	3260	3271	3293	rBV	763993	1209652	70.37%	9.464%
81	11.850	3360	3362	3366	rVV2	544	377	0.02%	0.003%
82	11.992	3404	3406	3408	rBV2	435	156	0.01%	0.001%
83	12.178	3462	3464	3472	rVB4	395	352	0.02%	0.003%
84	12.210	3472	3474	3476	rBV2	449	267	0.02%	0.002%
85	12.371	3518	3524	3533	rVB4	2394	3241	0.19%	0.025%
86	12.490	3559	3561	3564	rBV2	382	198	0.01%	0.002%
87	12.516	3564	3569	3573	rBV2	438	447	0.03%	0.003%
88	12.587	3584	3591	3603	rVB2	11181	17266	1.00%	0.135%
89	12.786	3651	3653	3654	rBV	345	158	0.01%	0.001%
90	12.837	3667	3669	3673	rVB	516	317	0.02%	0.002%
91	12.863	3673	3677	3679	rBV2	264	203	0.01%	0.002%
92	12.882	3680	3683	3685	rVB2	315	184	0.01%	0.001%
93	12.898	3685	3688	3690	rBV	369	224	0.01%	0.002%
94	12.950	3701	3704	3707	rBV2	307	192	0.01%	0.002%
95	12.995	3715	3718	3724	rVB2	570	327	0.02%	0.003%
96	13.046	3731	3734	3737	rBV	291	206	0.01%	0.002%
97	13.172	3770	3773	3774	rBV	332	167	0.01%	0.001%
98	13.201	3774	3782	3796	rVV2	25708	39559	2.30%	0.309%
99	13.442	3845	3857	3874	rBV	81555	136368	7.93%	1.067%
100	13.683	3922	3932	3947	rBV2	32255	52687	3.06%	0.412%




Sum of corrected areas: 12781942

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
Data File : VV034851.D
Acq On : 27 Mar 2024 00:39
Operator : SY/MD
Sample : VIBLK275
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK275

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

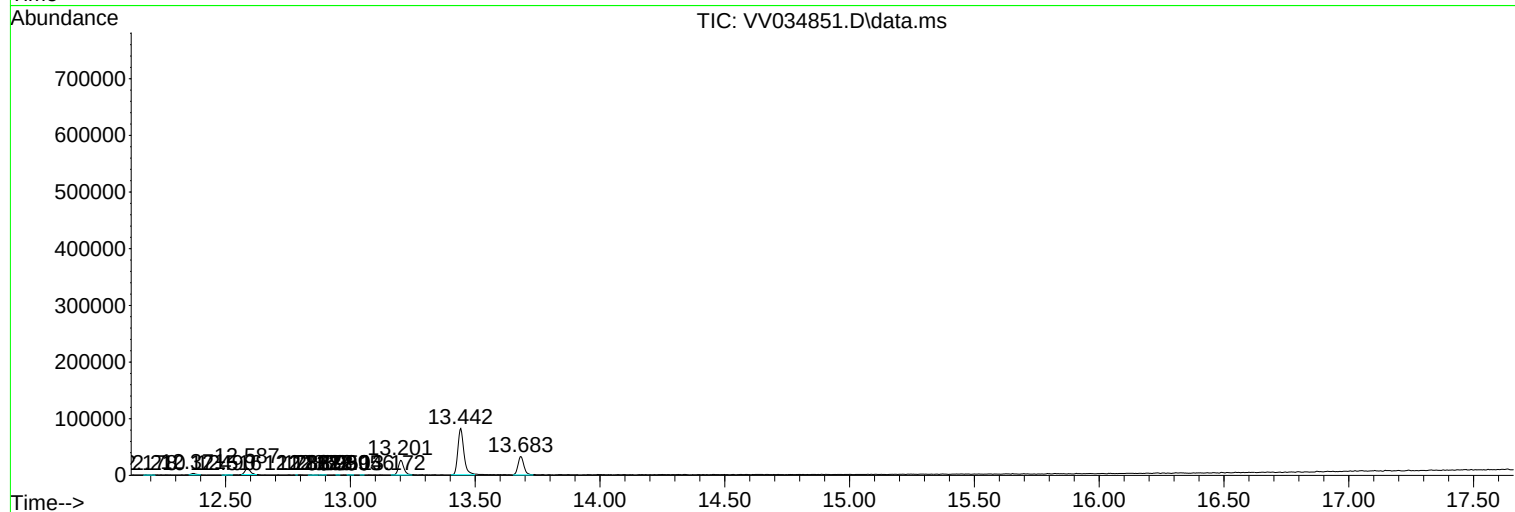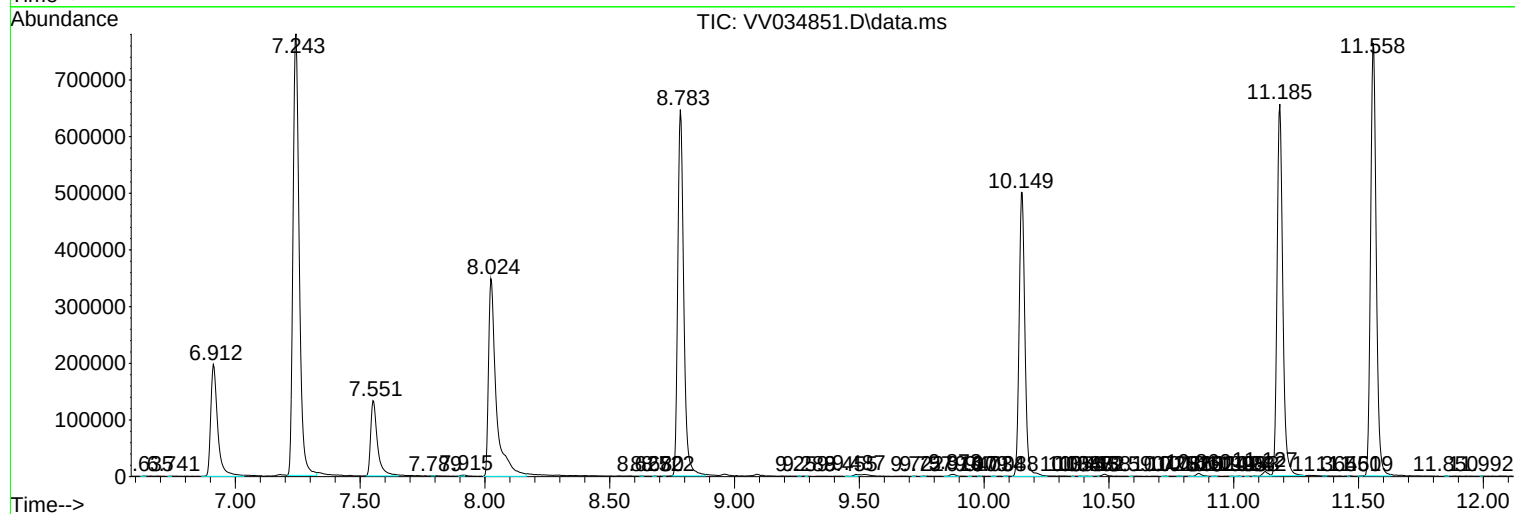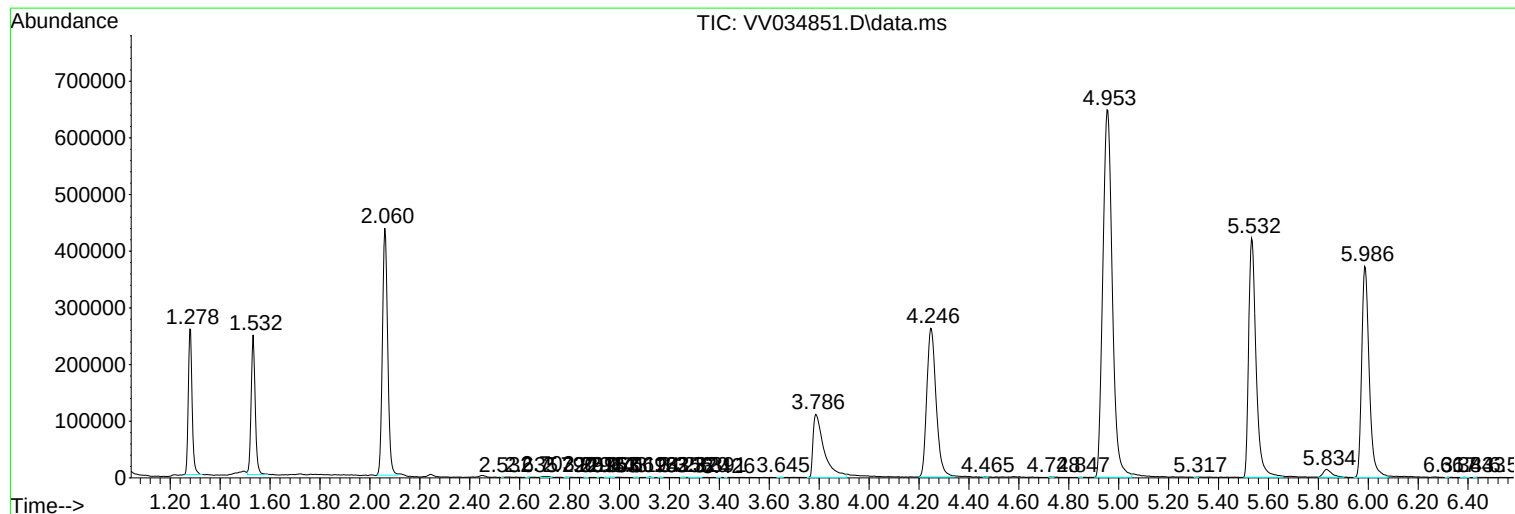

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
Data File : VV034851.D
Acq On : 27 Mar 2024 00:39
Operator : SY/MD
Sample : VIBLK275
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK275

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
Data File : VV034851.D
Acq On : 27 Mar 2024 00:39
Operator : SY/MD
Sample : VIBLK275
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK275

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------