
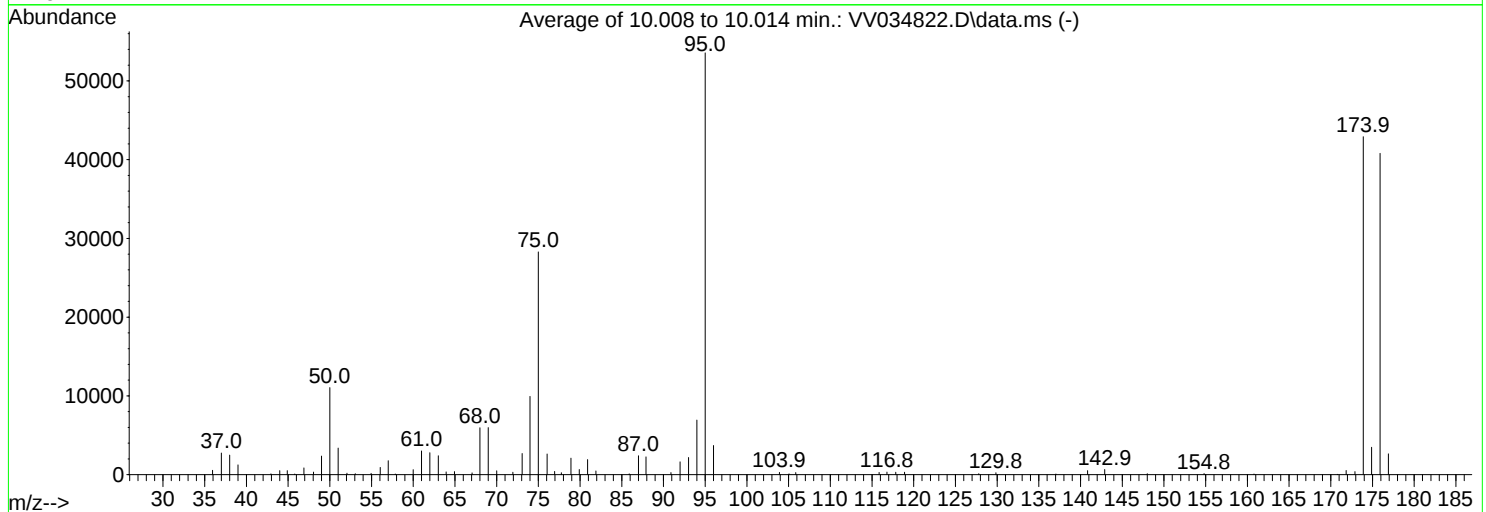


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032624\
Data File : VV034822.D
Acq On : 26 Mar 2024 11:48
Operator : SY/MD
Sample : BFB275
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB275

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Title : VOC Analysis
Last Update : Thu Mar 28 01:53:40 2024

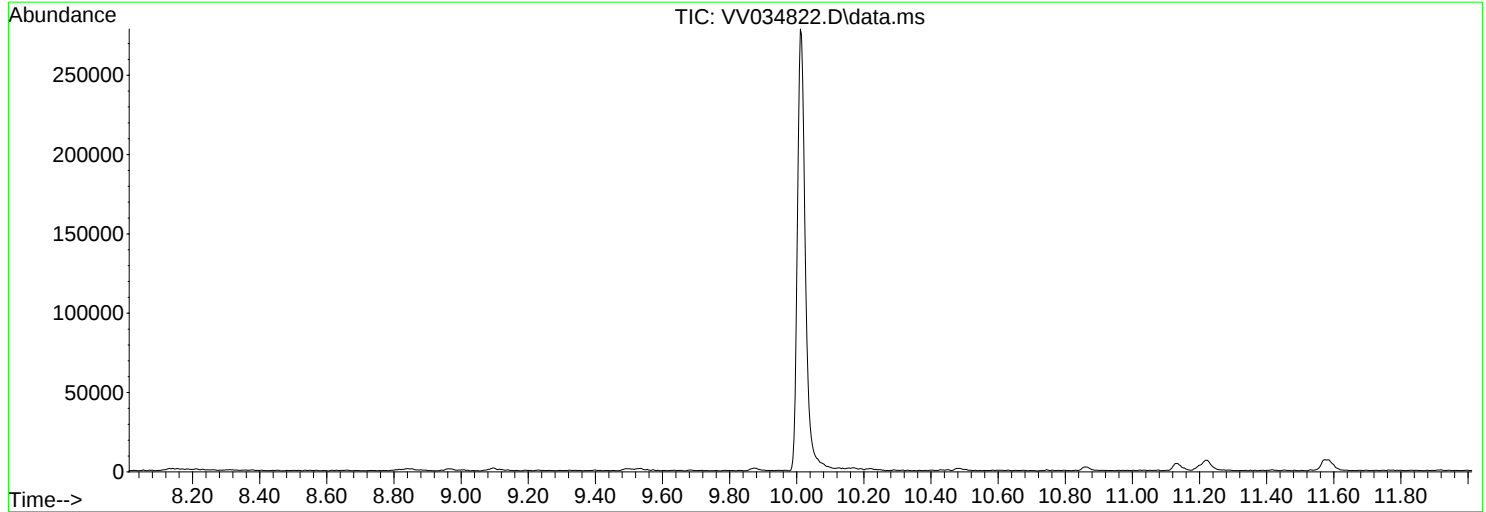

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	11063	PASS
75	95	30	80	52.8	28291	PASS
95	95	100	100	100.0	53565	PASS
96	95	5	9	6.9	3702	PASS
173	174	0.00	2	0.9	387	PASS
174	95	50	120	80.1	42909	PASS
175	174	5	9	8.1	3476	PASS
176	174	95	105	95.1	40792	PASS
177	176	5	10	6.5	2640	PASS

Scan 2779 (9.976 min): VV034822.D\data.ms
BFB275

m/z	Abundance
39.90	359.0
44.10	359.0

Instrument :
MSVOA_V
ClientSampleId :
BFB275

m/z	Abundance
35.90	537.0
37.00	2554.0
38.00	2398.0
39.00	1262.0
40.00	339.0
43.00	103.0
44.00	785.0
44.90	500.0
45.80	119.0
46.90	787.0
48.10	323.0
49.00	2223.0
50.00	10538.0
51.00	3309.0
52.10	201.0
53.00	100.0
55.00	177.0
56.00	963.0
57.00	1705.0
57.80	134.0
60.00	598.0
61.00	2812.0
62.00	2671.0
63.00	2206.0
64.00	372.0
64.90	377.0
67.00	224.0
68.00	5770.0
69.00	5699.0
70.00	480.0
72.00	334.0
73.00	2506.0
74.00	9548.0
75.00	27096.0
76.10	2483.0
76.90	357.0
77.70	182.0
78.90	1886.0
79.90	670.0
80.90	1851.0
81.90	483.0
85.90	106.0
87.00	2149.0
87.90	2362.0
90.90	261.0
92.00	1468.0
93.00	2187.0
94.00	6769.0
95.00	50984.0
96.00	3548.0
103.90	293.0
105.10	102.0
105.80	253.0
115.90	285.0
116.80	298.0
117.90	312.0
118.90	217.0
127.90	117.0
130.00	237.0
137.00	115.0
140.90	467.0
142.90	614.0
148.00	103.0
154.80	130.0
170.80	102.0
171.80	496.0
172.90	552.0
173.90	38960.0
174.90	3199.0
175.90	37496.0
176.90	2465.0

Instrument :
MSVOA_V
ClientSampleId :
BFB275

m/z	Abundance
35.90	574.0
37.00	2860.0
38.00	2571.0
39.00	1288.0
40.00	313.0
42.90	107.0
44.00	868.0
44.90	519.0
45.80	124.0
46.90	959.0
48.10	344.0
49.00	2446.0
50.00	11452.0
51.00	3498.0
52.10	183.0
53.00	125.0
54.90	173.0
56.10	915.0
57.00	1848.0
57.90	101.0
60.00	655.0
61.00	3099.0
62.00	2788.0
63.00	2473.0
64.00	357.0
65.00	402.0
67.10	232.0
68.00	6220.0
69.00	6141.0
70.00	505.0
71.90	320.0
73.10	2747.0
74.00	10195.0
75.00	29312.0
76.00	2762.0
77.00	394.0
77.80	255.0
78.90	2161.0
79.90	681.0
80.90	2001.0
81.90	503.0
85.90	111.0
87.00	2457.0
87.90	2299.0
90.90	265.0
92.00	1700.0
93.00	2187.0
94.00	7248.0
95.00	55288.0
96.00	3869.0
103.90	311.0
105.10	114.0
105.90	282.0
115.90	302.0
116.80	343.0
117.90	323.0
118.90	294.0
127.80	123.0
129.80	267.0
137.10	114.0
140.80	524.0
142.90	682.0
148.00	145.0
154.80	135.0
160.80	104.0
171.90	535.0
172.90	609.0
173.90	44472.0
174.90	3610.0
175.90	42248.0
176.90	2708.0

Instrument :
MSVOA_V
ClientSampleId :
BFB275

m/z	Abundance
36.00	523.0
37.00	2838.0
38.00	2462.0
39.00	1152.0
39.90	307.0
42.90	101.0
44.00	944.0
44.90	482.0
46.90	839.0
48.00	306.0
49.00	2409.0
50.00	11198.0
51.00	3338.0
52.00	139.0
53.10	117.0
54.90	158.0
56.00	882.0
57.00	1759.0
60.00	626.0
61.00	3140.0
62.00	2881.0
63.00	2502.0
63.90	310.0
65.00	395.0
67.10	208.0
68.00	5905.0
69.00	6106.0
70.00	484.0
71.90	273.0
73.00	2775.0
74.00	10062.0
75.00	28464.0
76.00	2648.0
77.00	444.0
77.80	311.0
78.90	2216.0
79.90	615.0
80.90	1906.0
81.90	439.0
85.90	100.0
87.00	2569.0
87.90	2110.0
90.90	281.0
92.00	1691.0
93.00	2169.0
94.00	6778.0
95.00	54424.0
96.00	3688.0
103.90	270.0
104.90	103.0
105.90	261.0
115.80	295.0
116.80	342.0
117.80	287.0
118.90	376.0
127.70	133.0
129.80	259.0
140.80	543.0
142.90	666.0
148.00	132.0
154.80	156.0
160.80	125.0
171.90	532.0
173.90	45296.0
174.90	3618.0
175.90	42632.0
176.90	2747.0

Instrument :
MSVOA_V
ClientSampleId :
BFB275