
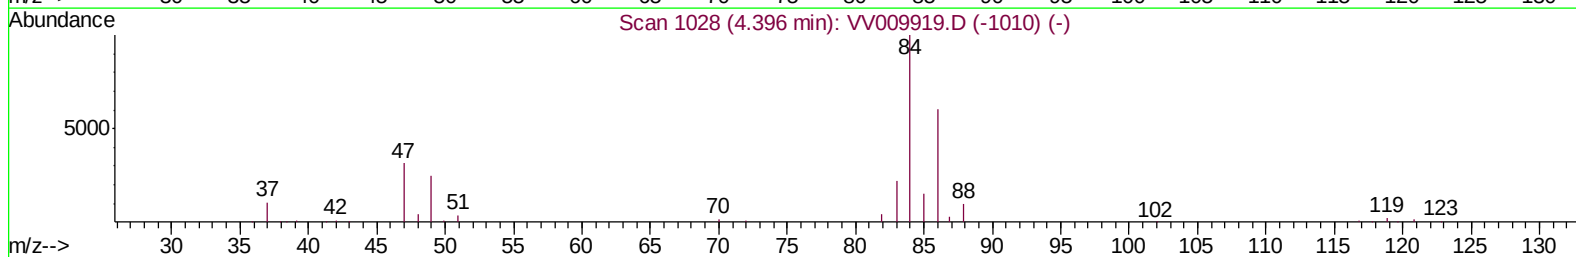
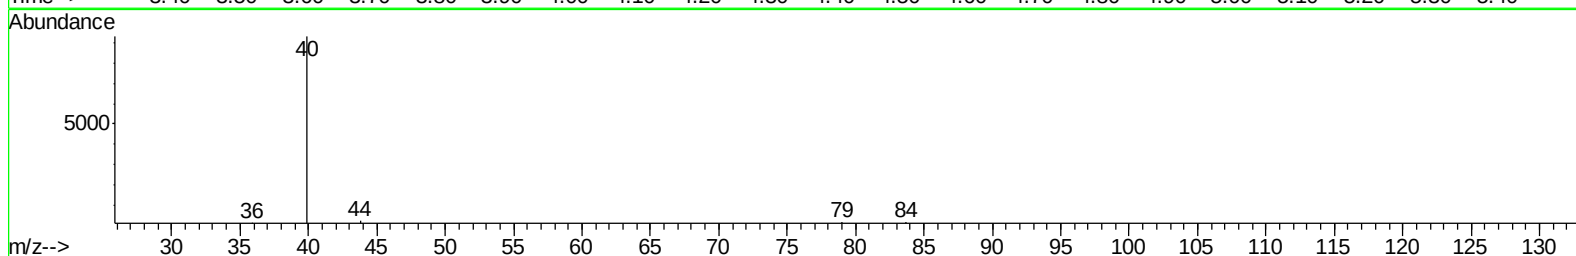


Data File : VV009925.D
Acq On : 27 Mar 2019 13:59
Operator : SY/MD
Sample : K2085-03
Misc : 4.89G/10mL/MSVOA_V/SOIL
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Mar 28 05:16:10 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM032619S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 28 05:12:38 2019
Response via : Initial Calibration

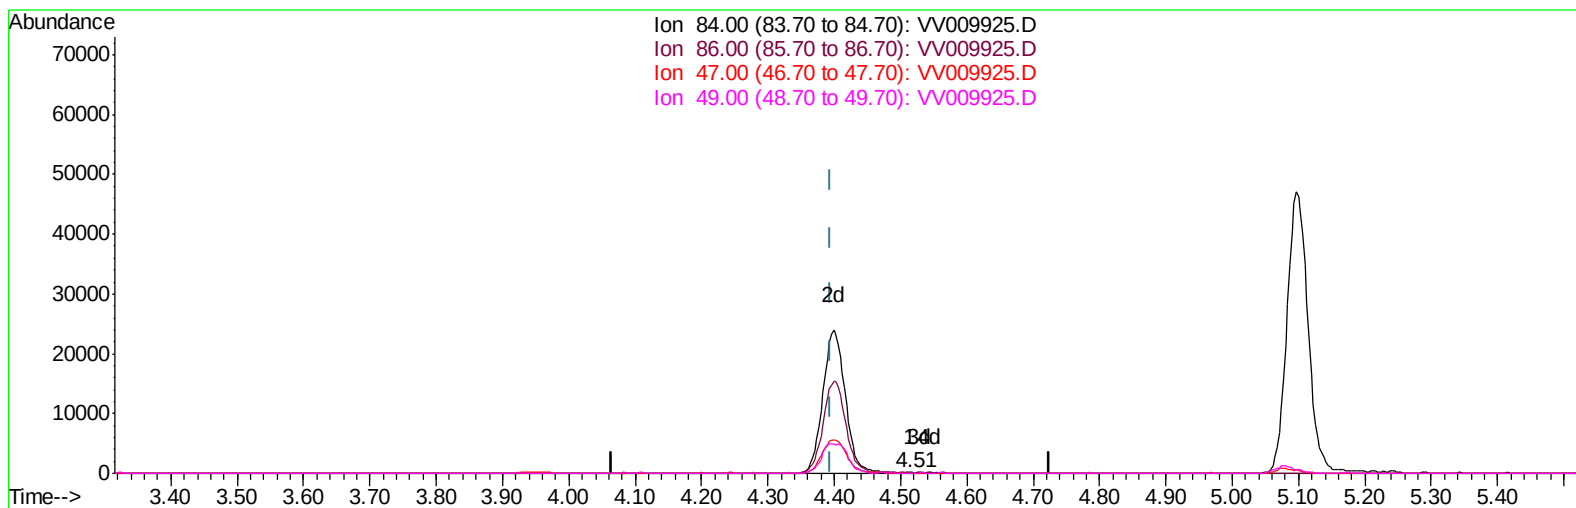

TIC: VV009925.D

(24) Chloroform-d (S)

4.515min (+0.119) 0.09ug/L

response 155

Ion	Exp%	Act%
84.00	100	100
86.00	61.50	49.68
47.00	49.10	46.45
49.00	31.70	29.68