

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV032719\

Quantitation Report (QT/LSC Reviewed)

Data File : VV009941.D

Acq On : 27 Mar 2019 22:10

Operator : SY/MD

Sample : K2128-03

Misc : 5.75G/10mL/MSVOA_V/SOIL

ALS Vial : 22 Sample Multiplier: 1

Quant Time: Mar 29 13:19:11 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM032619S.M

Quant Title : VOC Analysis

QLast Update : Thu Mar 28 07:17:22 2019

Response via : Initial Calibration

Instrument :

MSVOA_V

ClientSampleId :


BF0L8

Manual Integrations

APPROVED

MMDadoda

3/29/2019 1:12:39 PM

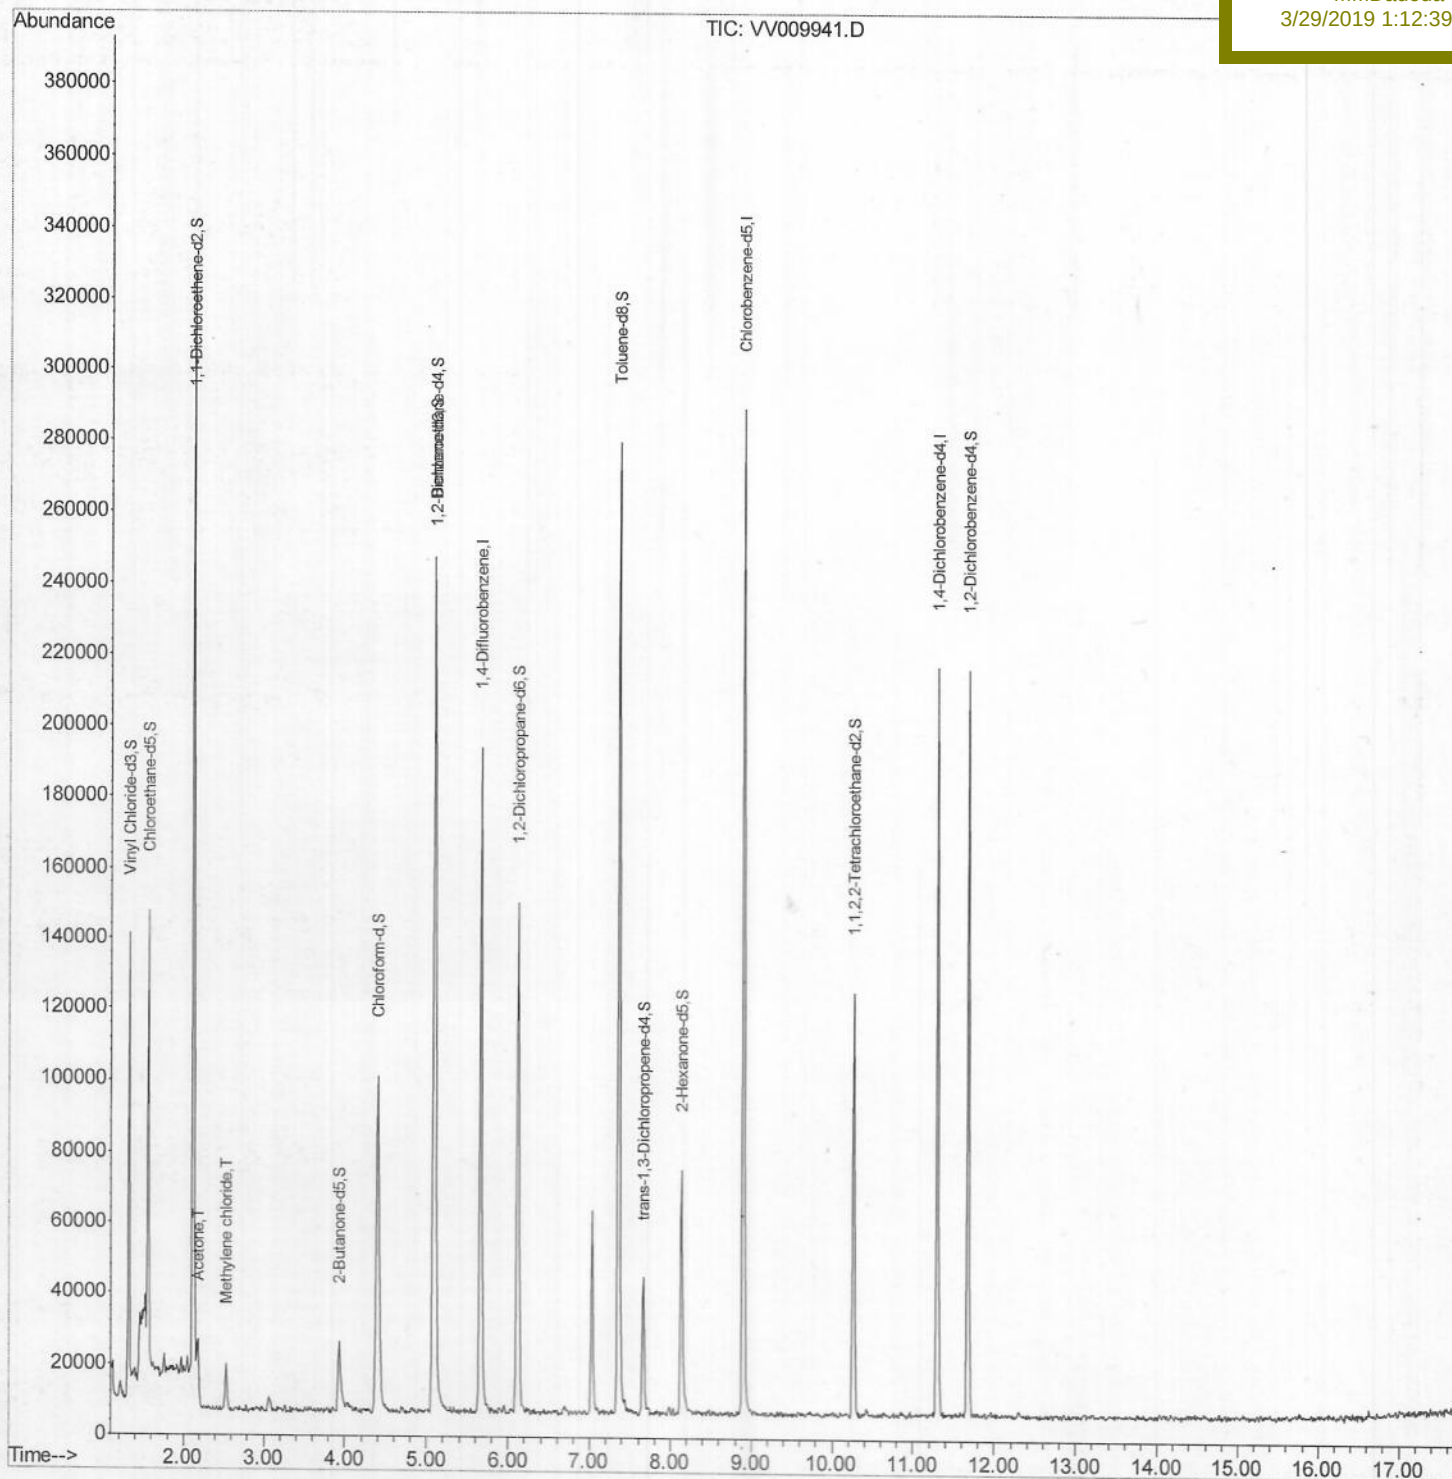

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV032719\
Quantitation Report (Qedit)




Data File : VV009941.D
Acq On : 27 Mar 2019 22:10
Operator : SY/MD
Sample : K2128-03
Misc : 5.75G/10mL/MSVOA_V/SOIL
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Mar 28 07:20:38 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM032619S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 28 07:17:22 2019
Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampleId :
BF0L8

Manual Integrations
APPROVED

MMDadoda
3/29/2019 1:12:39 PM

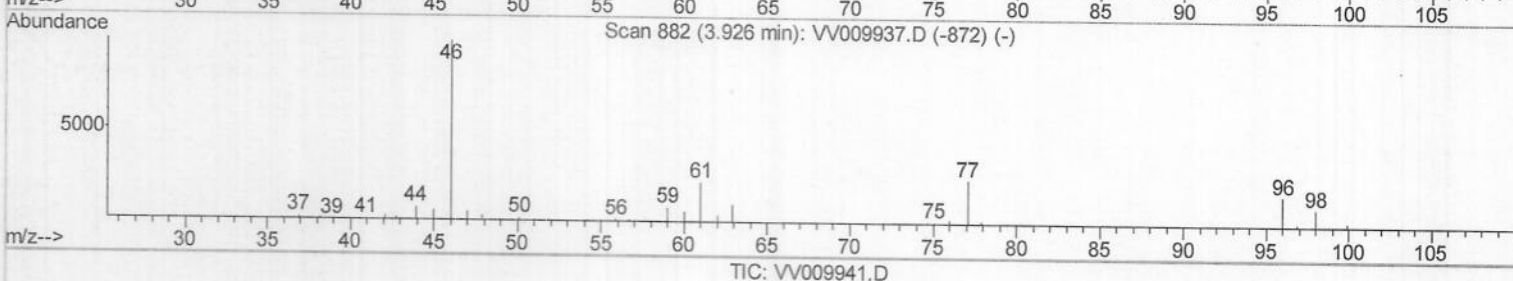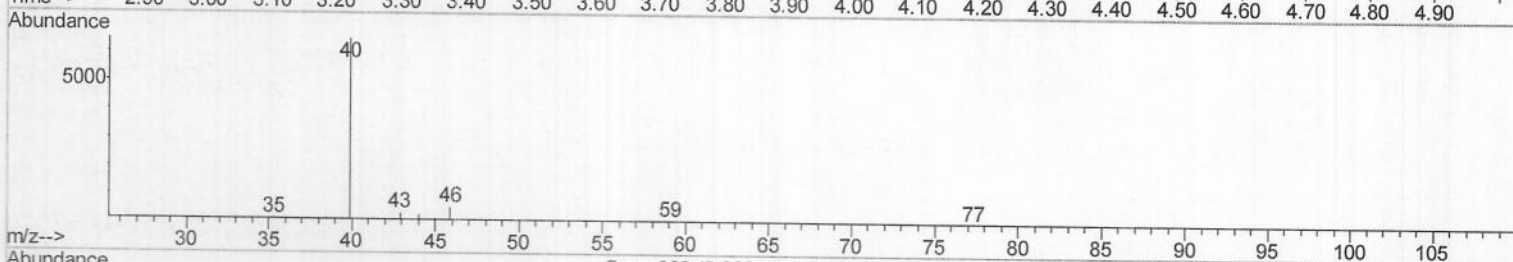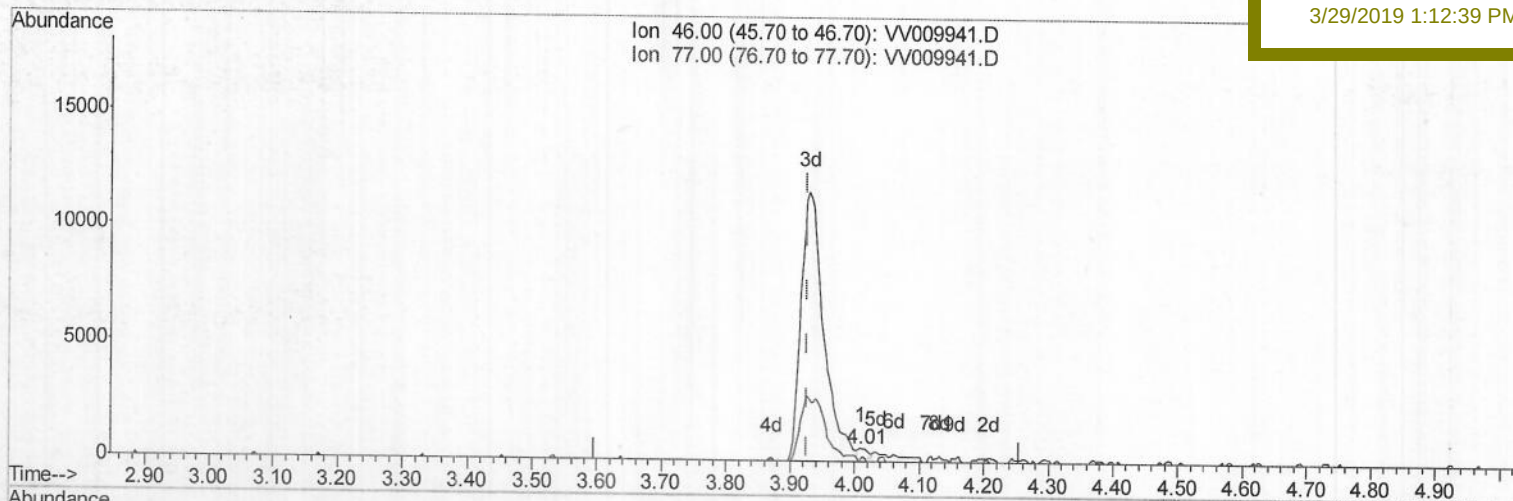

(20) 2-Butanone-d5 (S)

4.010min (+0.083) 0.83ug/L

response 463

Ion	Exp%	Act%
46.00	100	100
77.00	23.10	18.14
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV032719\
Quantitation Report (Qedit)




Data File : VV009941.D
Acq On : 27 Mar 2019 22:10
Operator : SY/MD
Sample : K2128-03
Misc : 5.75G/10mL/MSVOA_V/SOIL
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Mar 28 07:20:38 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM032619S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 28 07:17:22 2019
Response via : Initial Calibration

Instrument :
MSVOA_V
Client Sampled :
BF0L8

Manual Integrations
APPROVED

MMDadoda
3/29/2019 1:12:39 PM

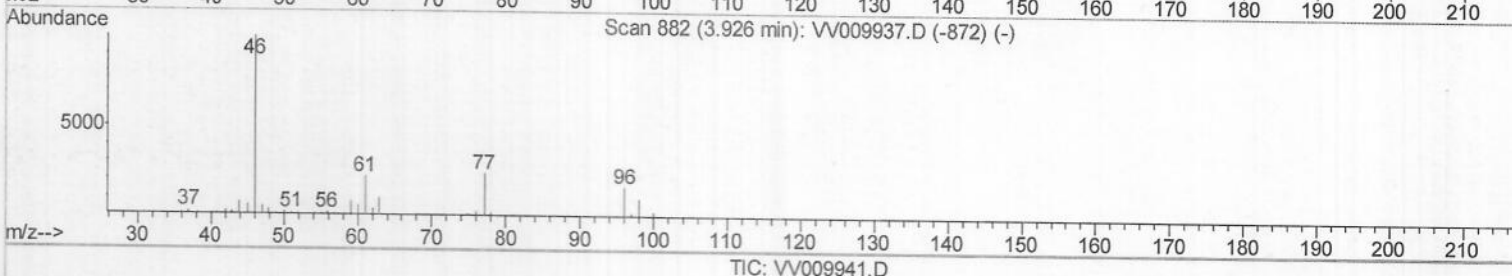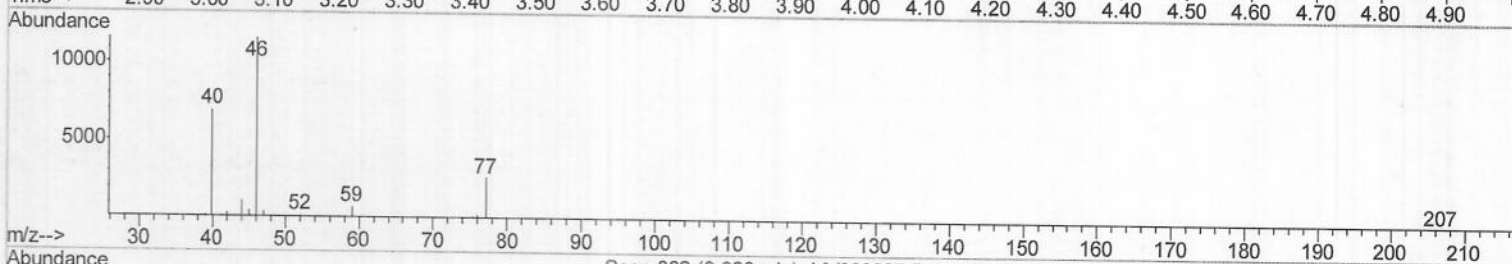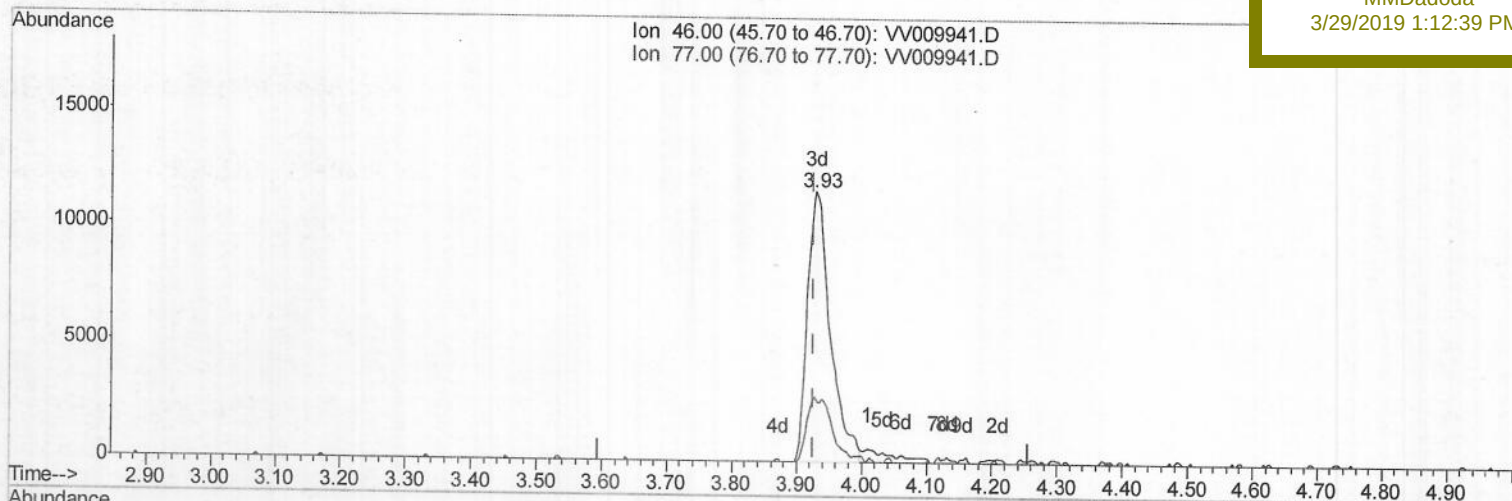

(20) 2-Butanone-d5 (S)

3.929min (+0.003) 50.75ug/L m

response 28379

Ion	Exp%	Act%
46.00	100	100
77.00	23.10	0.30#
0.00	0.00	0.00
0.00	0.00	0.00

M.D
4/11/19

Data File : VV009941.D
Acq On : 27 Mar 2019 22:10
Operator : SY/MD
Sample : K2128-03
Misc : 5.75G/10mL/MSVOA_V/SOIL
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
Client Sampled :
BF0L8

Quant Time: Mar 29 13:19:11 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM032619S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 28 07:17:22 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
3/29/2019 1:12:39 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	5.66	114	147866	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	143575	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	50998	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	66918	22.30	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	89.20%		
7) Chloroethane-d5	1.56	69	82295	25.39	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	101.56%		
10) 1,1-Dichloroethene-d2	2.12	63	156080	19.02	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	76.08%		
20) 2-Butanone-d5	3.93	46	28379m	50.75	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	101.50%		
24) Chloroform-d	4.40	84	83920	22.28	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	89.12%		
26) 1,2-Dichloroethane-d4	5.08	65	57332	25.29	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	101.16%		
29) Benzene-d6	5.10	84	198846	26.37	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	105.48%		
33) 1,2-Dichloropropane-d6	6.12	67	60018	27.21	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	108.84%		
37) Toluene-d8	7.36	98	170920	23.95	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	95.80%		
38) trans-1,3-Dichloropropene-	7.66	79	18631	20.65	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	82.60%		
39) 2-Hexanone-d5	8.13	63	21423	52.03	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	104.06%		
48) 1,1,2,2-Tetrachloroethane-	10.26	84	52105	23.86	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	95.44%		
61) 1,2-Dichlorobenzene-d4	11.67	152	49718	25.61	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	102.44%		

Target Compounds					Qvalue
13) Acetone	2.18	43	13220	15.616 ug/L	93
16) Methylene chloride	2.53	84	5168	2.122 ug/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

M.D
4/11/19