


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032719\
Data File : VV009918.D
Acq On : 27 Mar 2019 09:26
Operator : SY/MD
Sample : BFB77
Misc : 5.00G/10mL/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB77

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM032619S.M
Title : VOC Analysis
Last Update : Tue Apr 02 06:39:31 2019

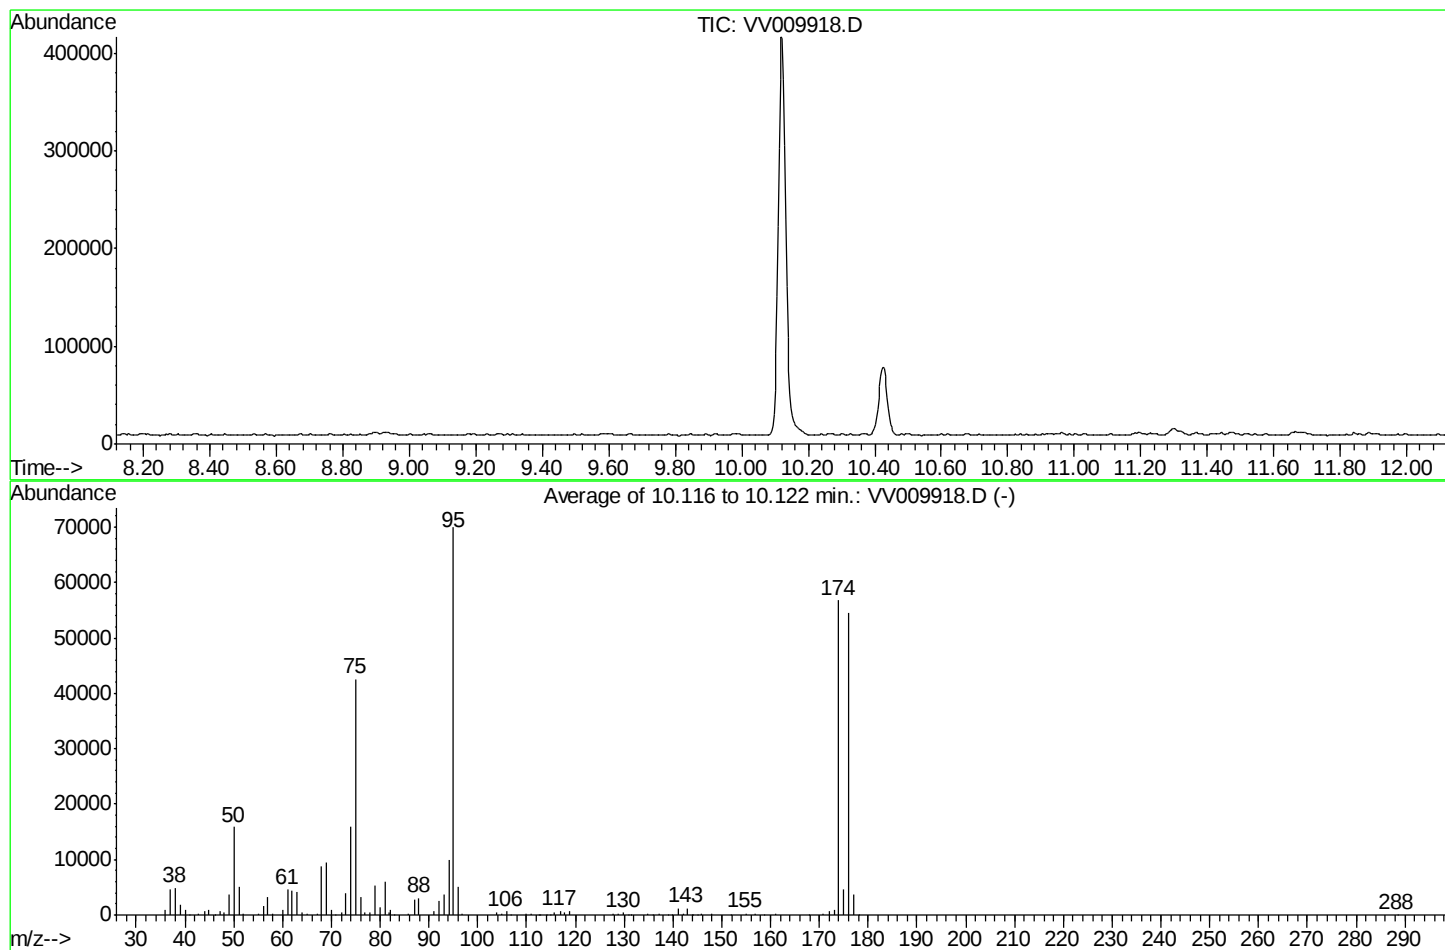

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.8	15929	PASS
75	95	30	80	60.9	42586	PASS
95	95	100	100	100.0	69973	PASS
96	95	5	9	7.2	5069	PASS
173	174	0.00	2	1.8	1000	PASS
174	95	50	120	81.1	56738	PASS
175	174	5	9	8.2	4652	PASS
176	174	95	101	96.1	54541	PASS
177	176	5	9	6.7	3666	PASS

m/z	Abundance
35.90	814.0
37.00	4891.0
38.00	4979.0
39.10	1976.0
40.00	10397.0
42.90	107.0
44.00	938.0
44.90	984.0
46.10	152.0
47.10	715.0
48.00	491.0
49.00	3756.0
50.00	16381.0
51.00	5199.0
52.00	195.0
54.90	304.0
56.00	1663.0
57.00	3250.0
58.00	197.0
60.00	1027.0
61.00	4461.0
62.00	4290.0
63.00	4417.0
64.00	438.0
64.90	227.0
67.10	305.0
68.00	8822.0
69.00	9890.0
70.10	809.0
72.00	382.0
73.00	4120.0
74.00	16043.0
75.00	44272.0
76.00	3465.0
77.00	545.0
77.80	358.0
78.90	5588.0
80.00	1373.0
80.90	6350.0
82.00	1263.0
85.70	192.0
87.00	3126.0
87.90	3096.0
90.90	665.0
92.00	2630.0
93.00	4091.0
94.10	9837.0
95.00	71408.0
96.10	5087.0
96.90	171.0
103.90	527.0
104.90	230.0
106.00	696.0
106.70	145.0
109.90	143.0
110.90	244.0
112.50	132.0
114.20	105.0
114.90	184.0
115.70	429.0
116.90	748.0
117.80	432.0
118.90	708.0
127.80	320.0
128.70	202.0
129.90	388.0
131.30	132.0
134.80	321.0
137.10	286.0
139.90	174.0
141.10	1267.0
142.00	170.0
142.90	1228.0
144.10	128.0
145.10	110.0
145.90	194.0
147.80	134.0
155.00	221.0
156.90	160.0
158.70	127.0
161.00	135.0
170.70	105.0
172.00	772.0
173.00	1558.0
174.00	59584.0
175.00	4917.0
176.00	57768.0
176.90	3841.0
178.00	187.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

m/z	Abundance
35.90	959.0
37.00	4753.0
38.00	5113.0
39.10	1997.0
40.00	10195.0
40.90	120.0
42.80	154.0
44.00	854.0
44.90	952.0
46.10	113.0
47.10	743.0
48.00	524.0
49.00	3856.0
50.00	16488.0
51.00	5408.0
52.00	237.0
54.90	276.0
56.00	1621.0
57.00	3394.0
58.00	226.0
60.00	1017.0
61.00	4815.0
62.00	4306.0
63.00	4400.0
64.00	450.0
64.90	248.0
67.10	358.0
68.00	9114.0
69.00	9814.0
70.10	931.0
72.10	400.0
73.00	4084.0
74.00	16712.0
75.00	44080.0
76.00	3354.0
76.90	553.0
77.90	393.0
78.90	5525.0
80.00	1439.0
80.90	6248.0
82.00	1206.0
83.00	149.0
85.80	148.0
87.00	2887.0
87.90	3276.0
90.90	666.0
92.00	2634.0
93.00	3952.0
94.10	10251.0
95.00	72720.0
96.10	5201.0
96.80	207.0
103.90	591.0
104.90	208.0
106.00	621.0
106.70	121.0
109.90	225.0
110.90	209.0
112.70	114.0
114.80	146.0
115.70	418.0
116.90	840.0
117.80	408.0
118.90	648.0
127.80	267.0
128.70	208.0
129.90	385.0
130.80	140.0
134.80	356.0
135.80	110.0
137.10	262.0
138.90	100.0
139.90	155.0
141.00	1298.0
142.10	208.0
142.90	1323.0
143.90	104.0
145.90	260.0
148.00	159.0
151.90	110.0
155.00	265.0
156.90	162.0
158.70	104.0
161.00	126.0
167.90	161.0
170.60	168.0
171.90	752.0
173.00	1444.0
174.00	58792.0
175.00	4754.0
176.00	56256.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

177.003820.0

178.00140.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

m/z	Abundance
36.00	994.0
37.00	4151.0
38.00	4578.0
39.10	1829.0
40.00	9437.0
40.90	102.0
42.90	190.0
44.00	769.0
44.90	802.0
47.10	765.0
48.00	554.0
49.00	3682.0
50.00	14919.0
51.00	4908.0
52.00	252.0
55.00	303.0
56.00	1632.0
57.00	3183.0
58.00	183.0
60.00	839.0
61.00	4566.0
62.00	4299.0
63.00	3852.0
64.00	390.0
64.90	262.0
67.10	283.0
68.00	8415.0
69.00	8767.0
70.10	864.0
70.80	101.0
72.10	432.0
73.00	3738.0
74.00	15393.0
75.00	39408.0
76.10	3120.0
77.00	517.0
77.90	399.0
78.90	4766.0
79.90	1384.0
81.00	5489.0
81.80	1083.0
82.90	209.0
85.80	111.0
87.00	2464.0
87.90	3011.0
90.90	620.0
91.90	2332.0
93.00	3405.0
94.00	9777.0
95.00	65792.0
96.00	4919.0
96.80	201.0
104.00	606.0
104.90	195.0
105.90	569.0
109.90	212.0
110.90	154.0
112.90	113.0
115.80	416.0
116.90	740.0
117.80	370.0
118.80	537.0
127.80	178.0
128.70	168.0
129.90	307.0
130.80	143.0
134.70	327.0
137.00	208.0
140.90	1163.0
142.10	190.0
142.90	1247.0
145.90	237.0
148.00	178.0
155.00	251.0
156.90	112.0
160.90	146.0
168.00	182.0
170.70	195.0
172.00	684.0
174.00	51840.0
175.00	4287.0
176.00	49600.0
176.90	3338.0
288.50	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

m/z	Abundance
40.00	9040.0
43.10	117.0
44.00	238.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77